

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
 Data File : BF128896.D
 Acq On : 21 Jun 2022 12:02
 Operator : CG\JU
 Sample : PB145625BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145625BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128896.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.422	529	533	554	rBV	3599320	3603959	78.34%	13.810%
2	6.428	699	704	707	rBV	3159742	3501452	76.11%	13.417%
3	6.769	758	762	766	rBV	923772	737537	16.03%	2.826%
4	7.340	853	859	862	rBV	2152837	2472831	53.75%	9.476%
5	8.051	975	980	984	rBV	920434	902899	19.63%	3.460%
6	9.134	1157	1164	1167	rBV	4825065	4600512	100.00%	17.629%
7	9.810	1273	1279	1282	rBV	1265733	1108509	24.10%	4.248%
8	10.604	1408	1414	1417	rBV	2811281	2520961	54.80%	9.660%
9	11.298	1526	1532	1535	rBV	1452870	1183954	25.74%	4.537%
10	12.892	1797	1803	1806	rBV	4094623	3981847	86.55%	15.258%
11	13.939	1977	1981	1985	rBV	834030	757323	16.46%	2.902%
12	14.033	1991	1997	2004	rBV	94002	109616	2.38%	0.420%
13	15.392	2223	2228	2239	rBV	507508	614893	13.37%	2.356%




Sum of corrected areas: 26096293

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
Data File : BF128896.D
Acq On : 21 Jun 2022 12:02
Operator : CG\JU
Sample : PB145625BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145625BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

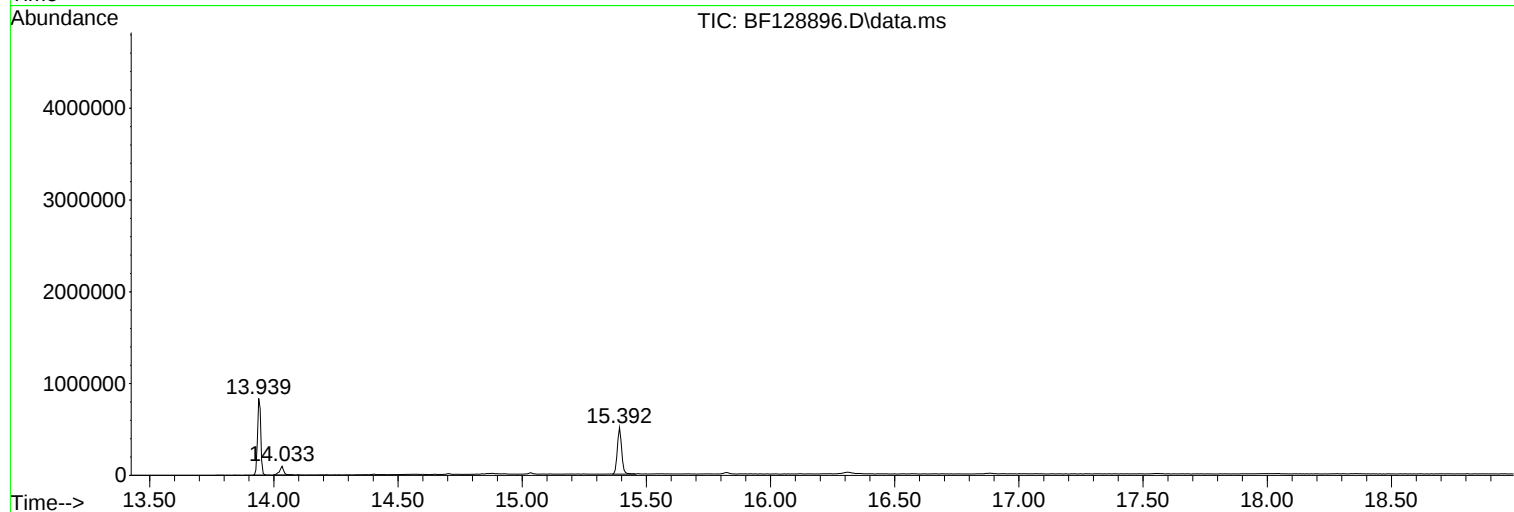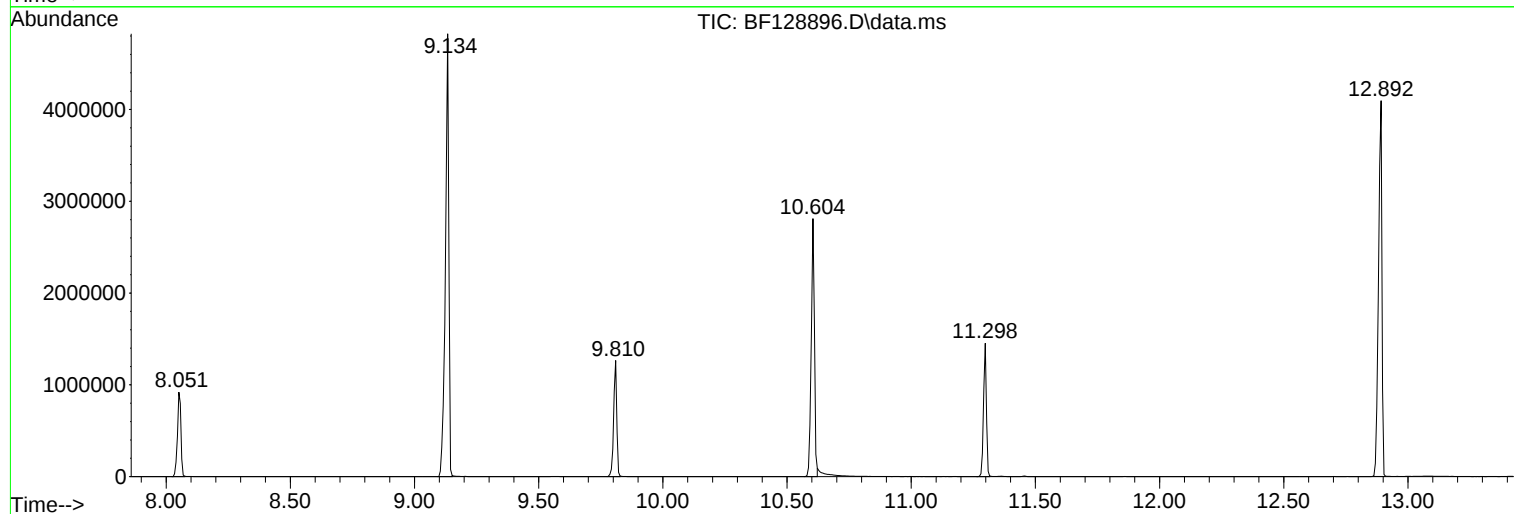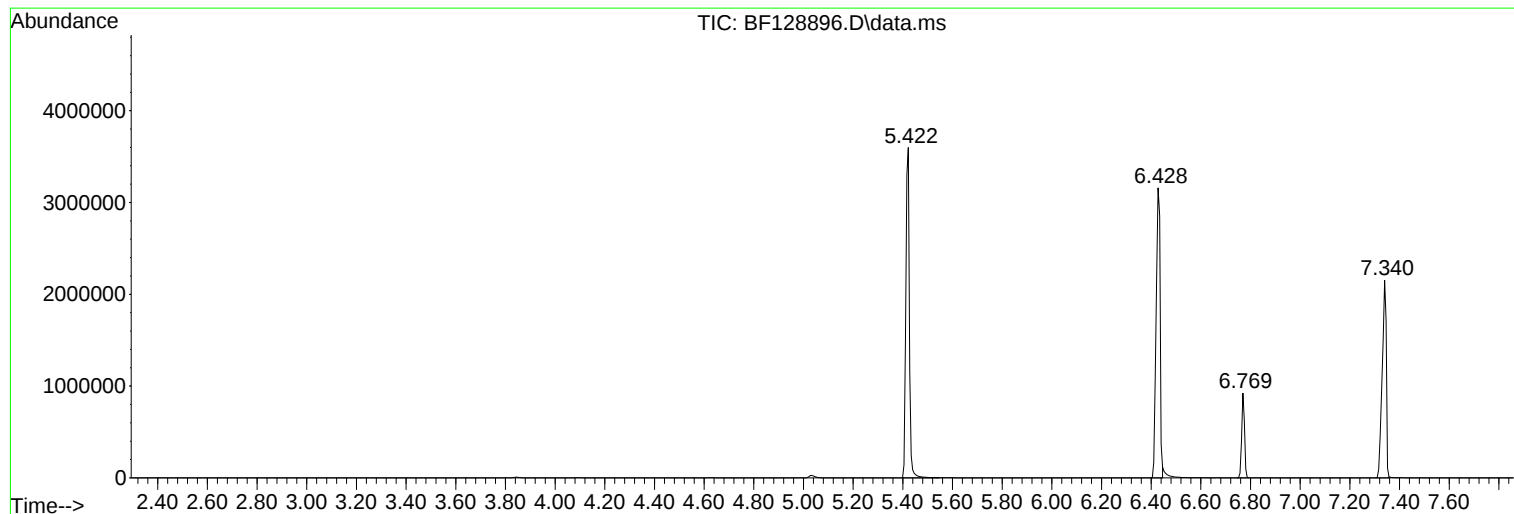

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
Data File : BF128896.D
Acq On : 21 Jun 2022 12:02
Operator : CG\JU
Sample : PB145625BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145625BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.033	2.89 ng	109616	Chrysene-d12	13.939

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	98
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	70
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	38
4			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	28
5			2-Phenyl-6-(trifluoromethyl)-1H...	277	C15H10F3NO	1000387-59-3	9

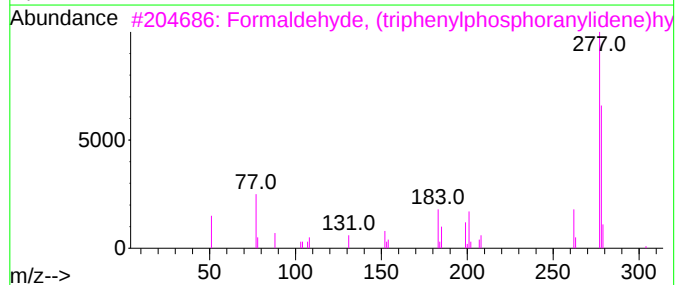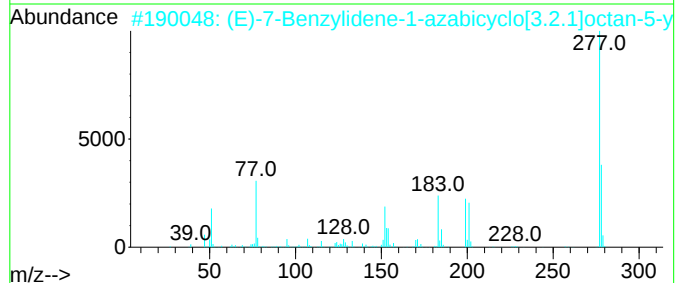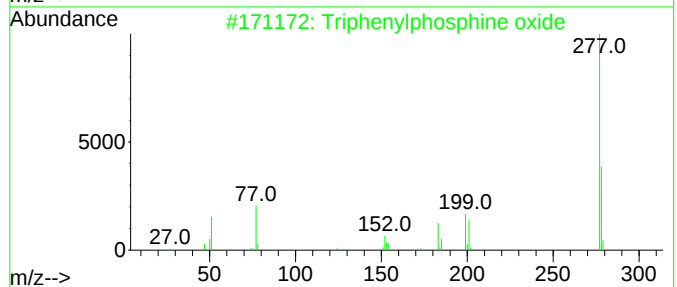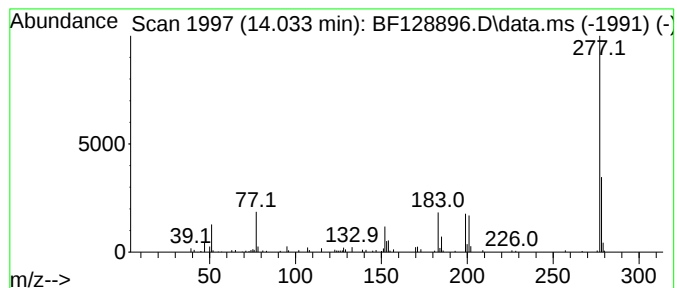

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
Data File : BF128896.D
Acq On : 21 Jun 2022 12:02
Operator : CG\JU
Sample : PB145625BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145625BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.033	2.9	ng	109616	5	13.939	757323	20.0