


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
 Data File : BF128892.D
 Acq On : 21 Jun 2022 09:12
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 22 01:02:29 2022

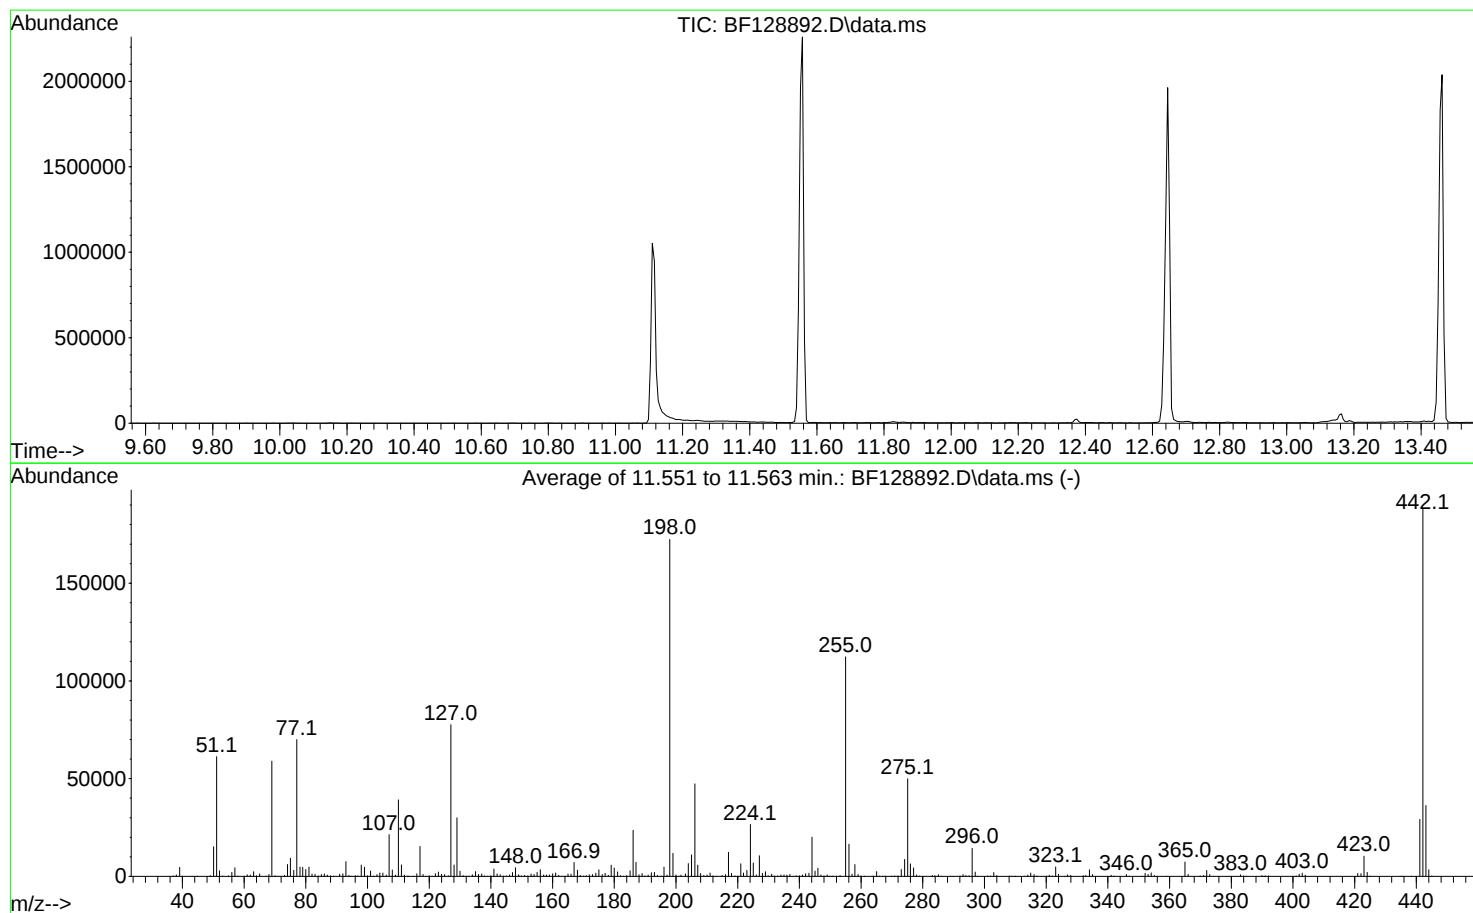




AutoFind: Scans 1575, 1576, 1577; Background Corrected with Scan 1569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	61281	PASS
68	69	0.00	2	1.7	979	PASS
69	198	0.00	100	34.2	58953	PASS
70	69	0.00	2	0.6	335	PASS
127	198	10	80	45.0	77595	PASS
197	198	0.00	2	0.4	698	PASS
198	198	100	100	100.0	172443	PASS
199	198	5	9	6.8	11792	PASS
275	198	10	60	29.0	49939	PASS
365	198	1	100	4.3	7357	PASS
441	198	0.01	100	16.9	29155	PASS
442	442	50	100	100.0	188224	PASS
443	442	15	24	19.3	36267	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
Data File : BF128892.D
Acq On : 21 Jun 2022 09:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 22 01:45:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:02:29 2022
Response via : Initial Calibration

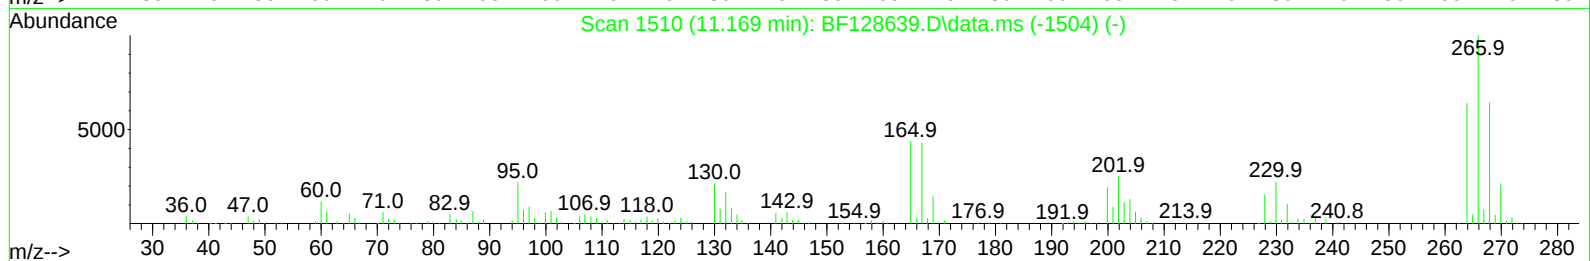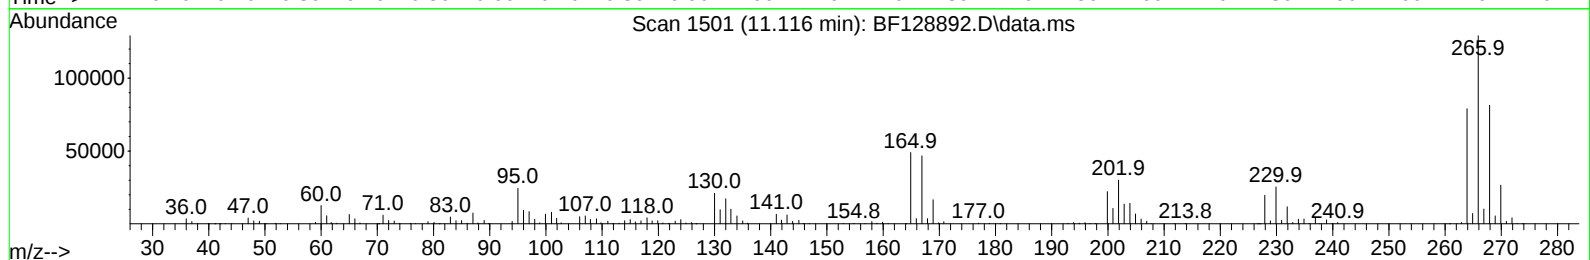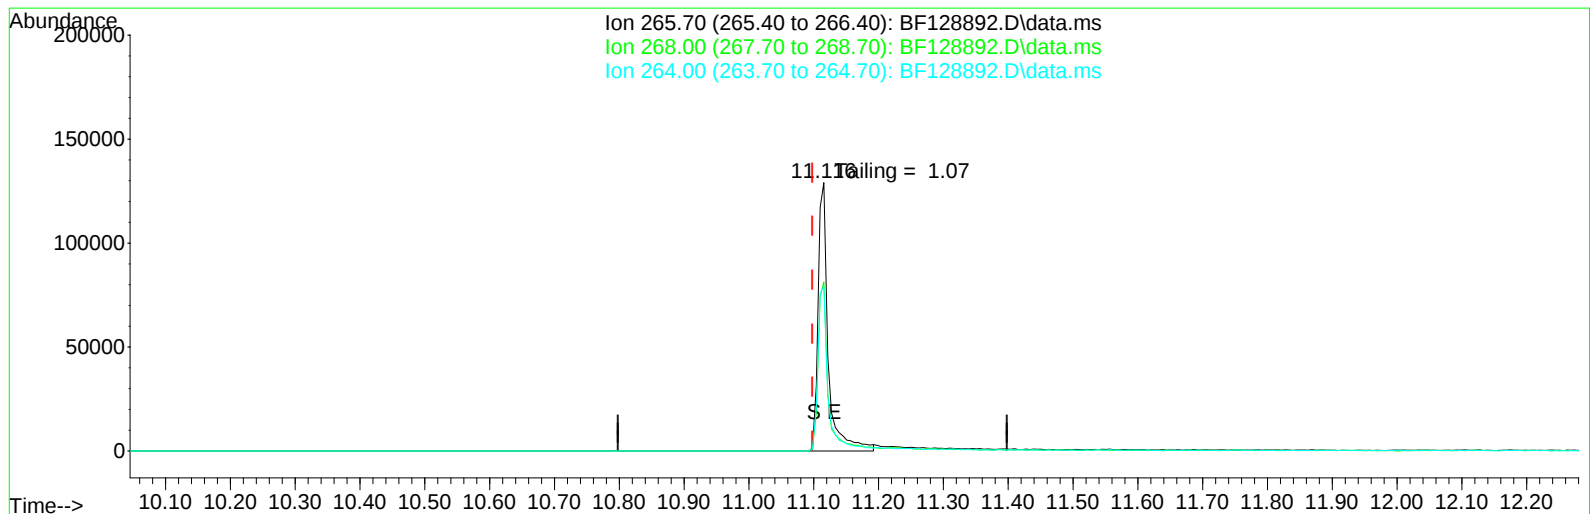

TIC: BF128892.D\data.ms

(70) Pentachlorophenol (C)

11.116min (+ 0.018) 309691.14 ng

response 151252

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.03
264.00	61.80	61.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/21/2022	BNA_F	<u>BF128892.D</u>
Compound Name	Response	Retention Time
DDT	376257	13.463
DDD	10111	13.163
DDE	1771	12.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11882	388139	3.06

Instrument :
BNA_F
ClientSampleId :
DFTPP