
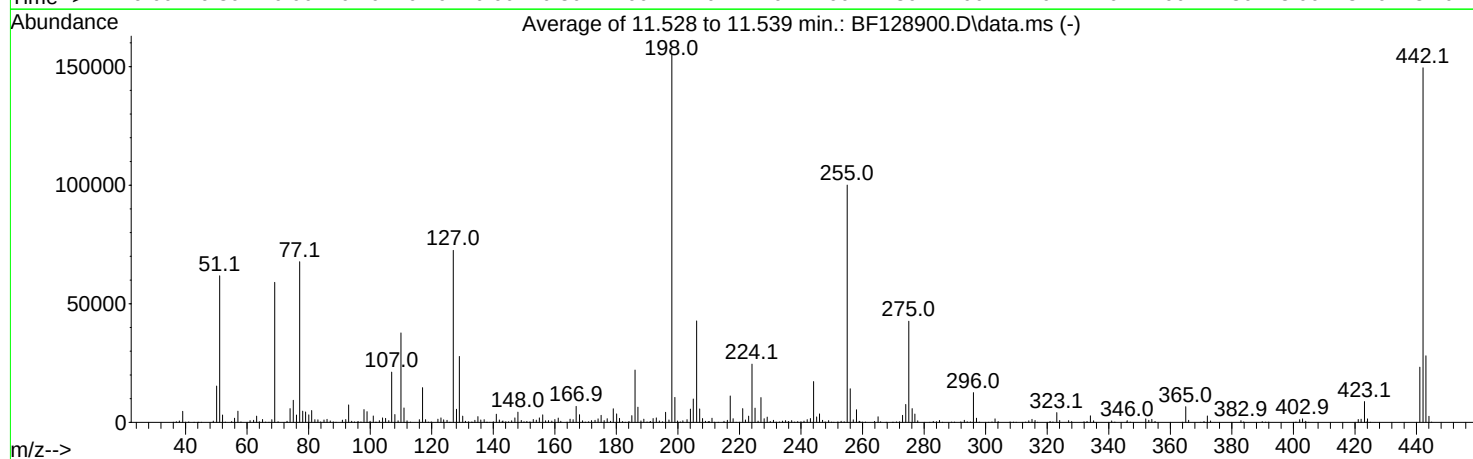


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
 Data File : BF128900.D
 Acq On : 21 Jun 2022 16:33
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 22 01:02:29 2022

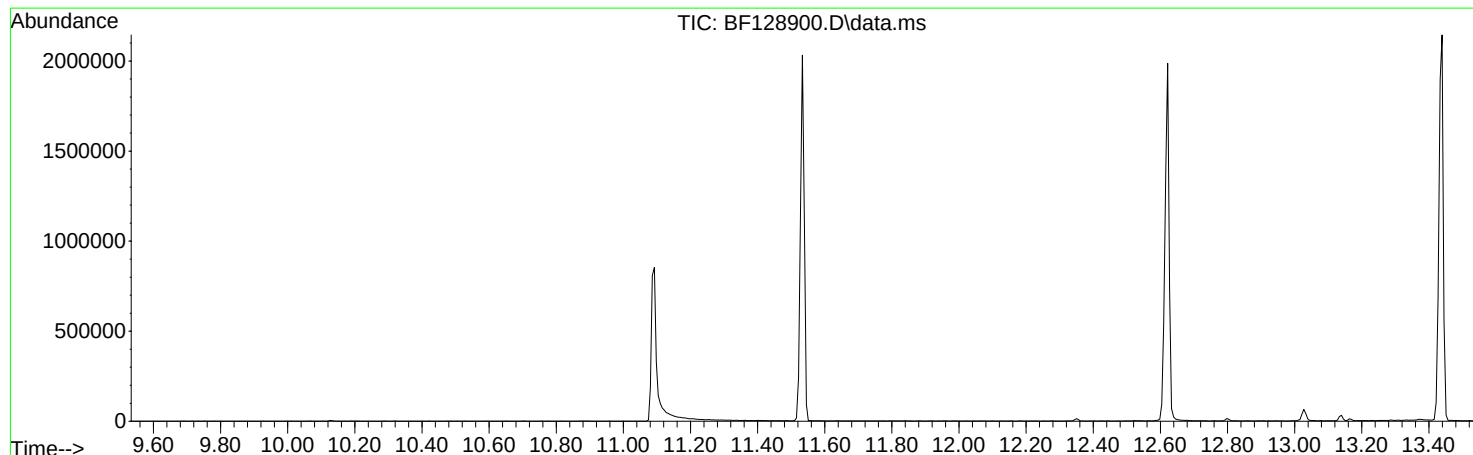




AutoFind: Scans 1571, 1572, 1573; Background Corrected with Scan 1565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	61811	PASS
68	69	0.00	2	1.9	1129	PASS
69	198	0.00	100	38.0	59011	PASS
70	69	0.00	2	0.4	240	PASS
127	198	10	80	46.8	72552	PASS
197	198	0.00	2	0.7	1035	PASS
198	198	100	100	100.0	155115	PASS
199	198	5	9	6.8	10525	PASS
275	198	10	60	27.5	42624	PASS
365	198	1	100	4.3	6643	PASS
441	198	0.01	100	15.0	23298	PASS
442	442	50	100	100.0	149504	PASS
443	442	15	24	18.8	28081	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
Data File : BF128900.D
Acq On : 21 Jun 2022 16:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 22 01:50:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:02:29 2022
Response via : Initial Calibration

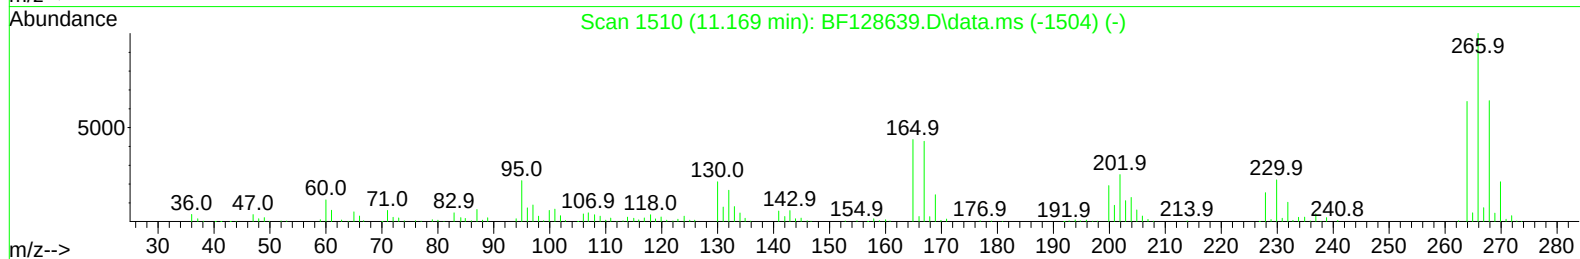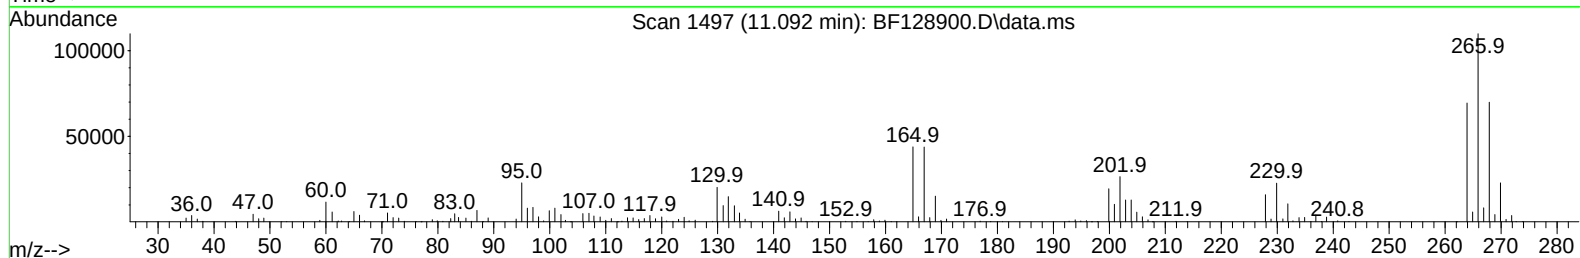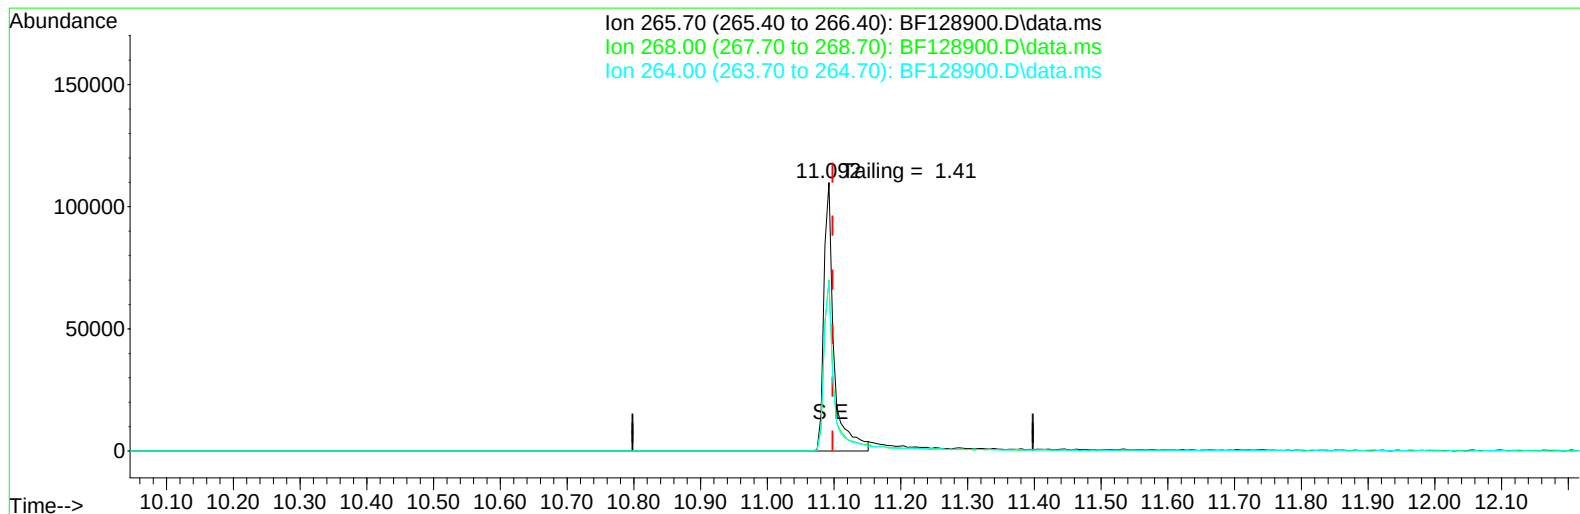

TIC: BF128900.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.006) 225666.68 ng




response 124166

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.60
264.00	61.80	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062122\
Data File : BF128900.D
Acq On : 21 Jun 2022 16:33
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 22 01:50:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 01:02:29 2022
Response via : Initial Calibration

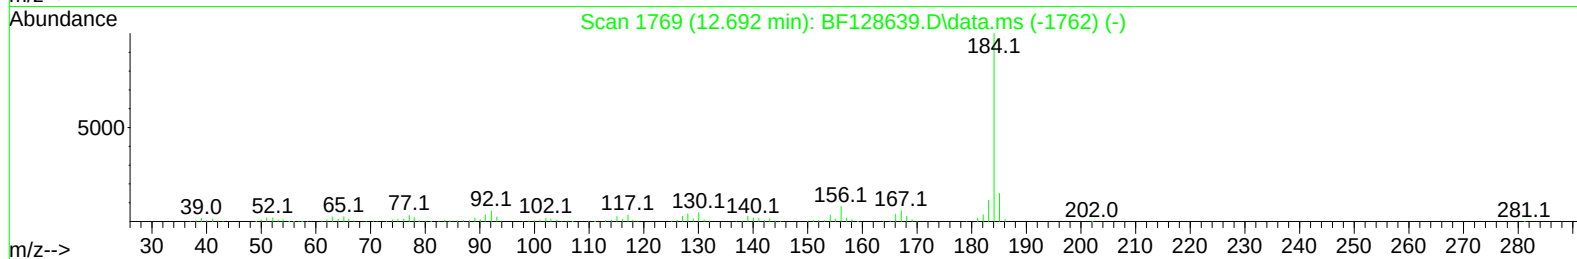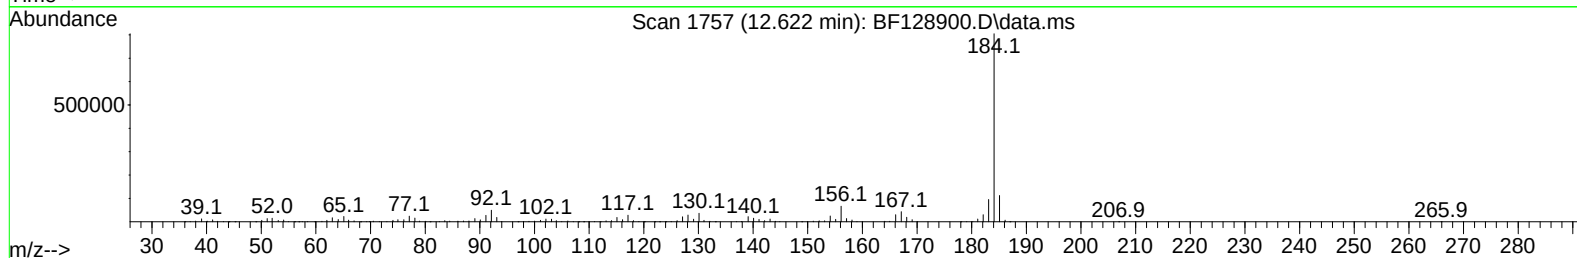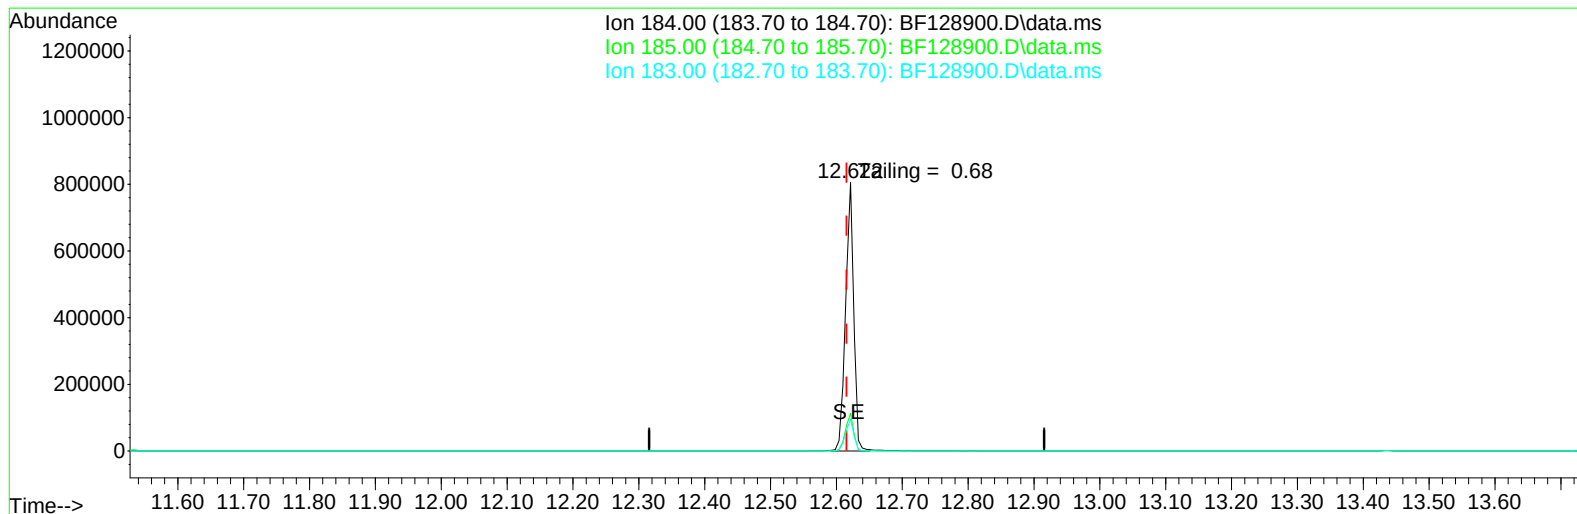

TIC: BF128900.D\data.ms

(77) Benzidine

12.622min (+ 0.006) 202435.55 ng

response 698132

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.00
183.00	11.60	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/21/2022	BNA_F	<u>BF128900.D</u>
Compound Name	Response	Retention Time
DDT	373005	13.439
DDD	7477	13.139
DDE	2317	12.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9794	382799	2.56

Instrument :
BNA_F
ClientSampleId :
DFTPP