

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
 Data File : BF128947.D
 Acq On : 23 Jun 2022 11:12
 Operator : CG\JU
 Sample : PB145651BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145651BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.375	521	525	544	rBV	3825860	3828126	68.98%	12.365%
2	6.392	693	698	701	rBV	3450089	3862864	69.61%	12.478%
3	6.734	752	756	759	rBV	943347	812523	14.64%	2.625%
4	7.304	847	853	856	rBV	2413992	2731444	49.22%	8.823%
5	8.016	969	974	977	rBV	1240152	1078841	19.44%	3.485%
6	9.098	1151	1158	1161	rBV	4940244	4933882	88.91%	15.937%
7	9.769	1266	1272	1276	rBV	1437428	1279735	23.06%	4.134%
8	10.569	1401	1408	1411	rBV	3168612	2959739	53.33%	9.560%
9	11.257	1519	1525	1529	rBV	1510248	1379908	24.87%	4.457%
10	12.857	1791	1797	1800	rBV	5370307	5549584	100.00%	17.926%
11	13.904	1971	1975	1979	rBV	1426251	1242433	22.39%	4.013%
12	13.998	1985	1991	1996	rBV	144585	162257	2.92%	0.524%
13	15.345	2215	2220	2230	rVB	902104	1072121	19.32%	3.463%
14	16.474	2404	2412	2414	rBV4	31008	64975	1.17%	0.210%




Sum of corrected areas: 30958432

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128947.D
Acq On : 23 Jun 2022 11:12
Operator : CG\JU
Sample : PB145651BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145651BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

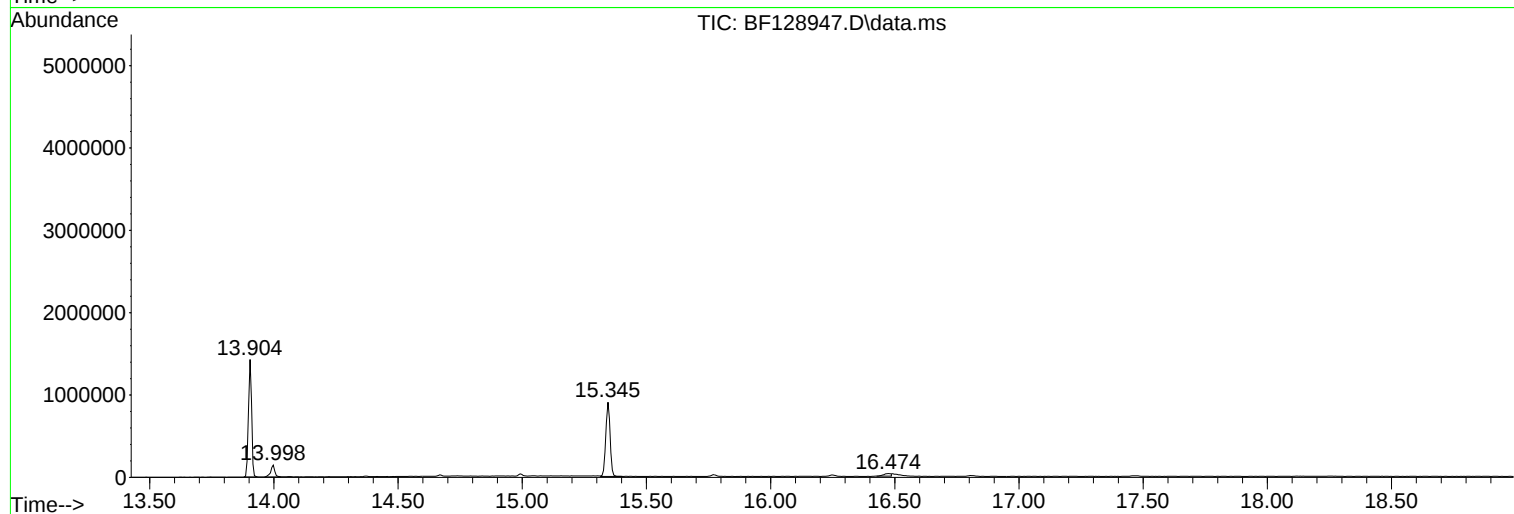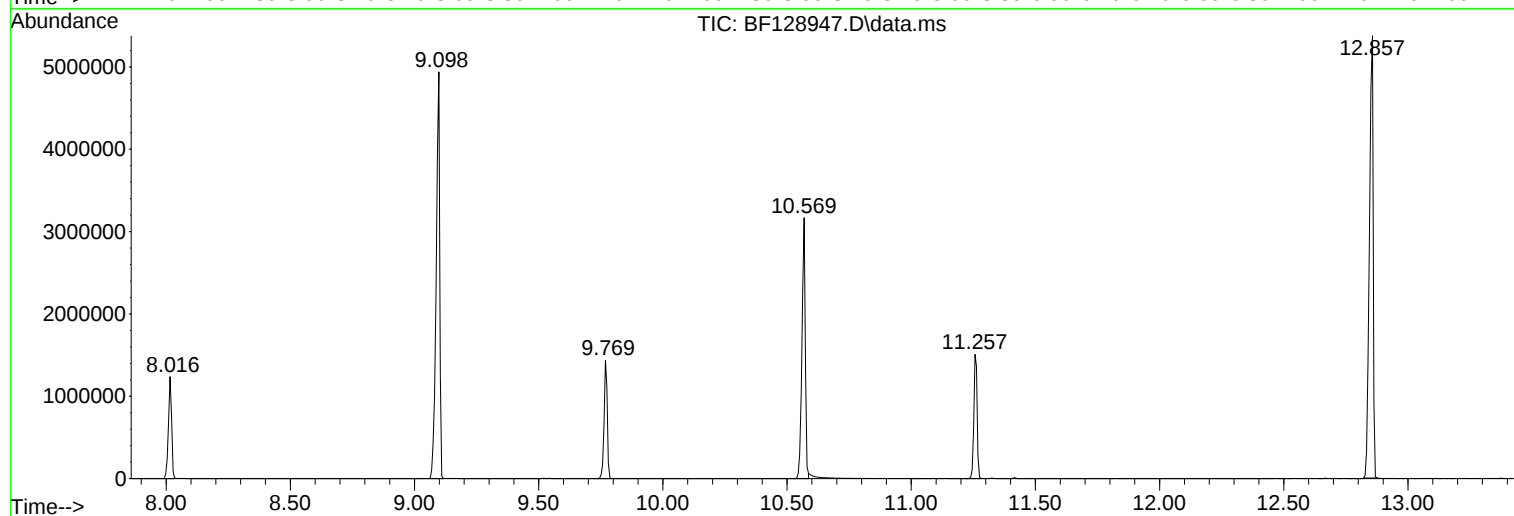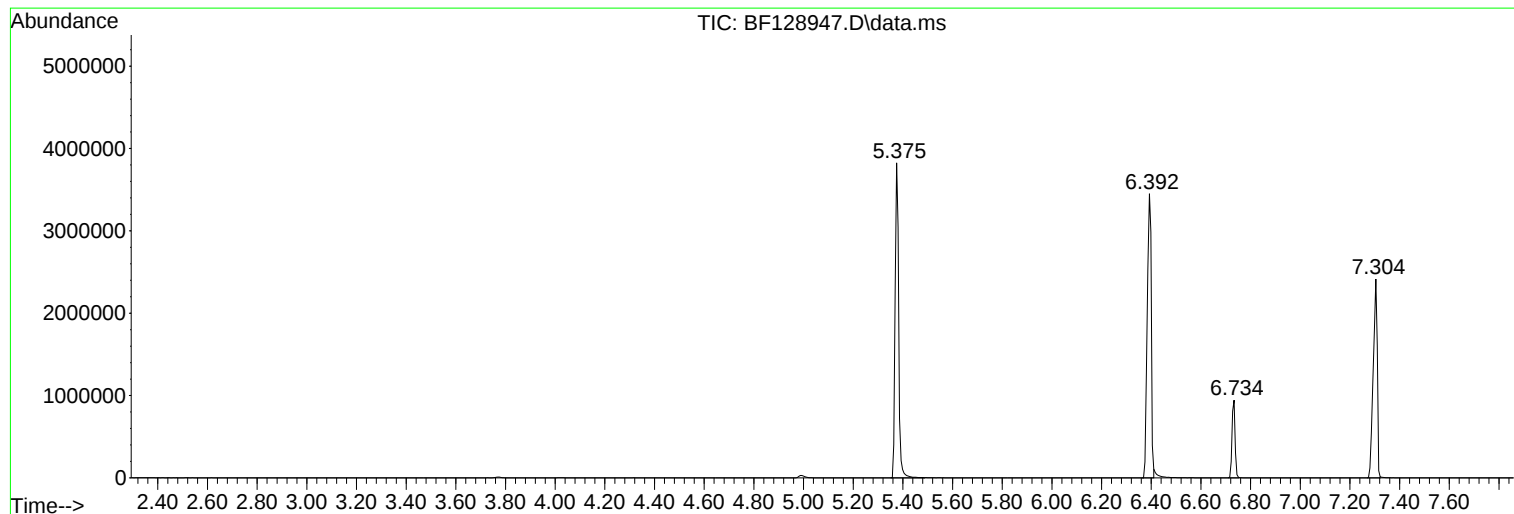

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128947.D
Acq On : 23 Jun 2022 11:12
Operator : CG\JU
Sample : PB145651BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145651BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128947.D
Acq On : 23 Jun 2022 11:12
Operator : CG\JU
Sample : PB145651BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145651BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------