

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
 Data File : BF128949.D
 Acq On : 23 Jun 2022 12:10
 Operator : CG\JU
 Sample : PB145641BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145641BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	456	460	468	rBV2	32348	52697	1.18%	0.206%
2	5.375	522	525	539	rBV	3708215	3968813	89.24%	15.531%
3	6.392	693	698	701	rBV	2757666	3034423	68.23%	11.875%
4	6.734	752	756	759	rBV	690202	585232	13.16%	2.290%
5	7.304	847	853	856	rBV	1999096	2117460	47.61%	8.286%
6	8.016	969	974	977	rBV	893683	772394	17.37%	3.023%
7	9.098	1151	1158	1161	rBV	3996441	3950498	88.83%	15.460%
8	9.769	1267	1272	1276	rBV	1029508	915028	20.58%	3.581%
9	10.569	1401	1408	1411	rBV	2553465	2371675	53.33%	9.281%
10	11.257	1520	1525	1529	rBV	1139626	991826	22.30%	3.881%
11	12.857	1791	1797	1800	rBV	4388630	4447241	100.00%	17.403%
12	13.904	1971	1975	1979	rBV	1372496	1190923	26.78%	4.660%
13	13.998	1985	1991	1999	rBV	138186	156867	3.53%	0.614%
14	15.345	2215	2220	2228	rBV	812982	998729	22.46%	3.908%




Sum of corrected areas: 25553806

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128949.D
Acq On : 23 Jun 2022 12:10
Operator : CG\JU
Sample : PB145641BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145641BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

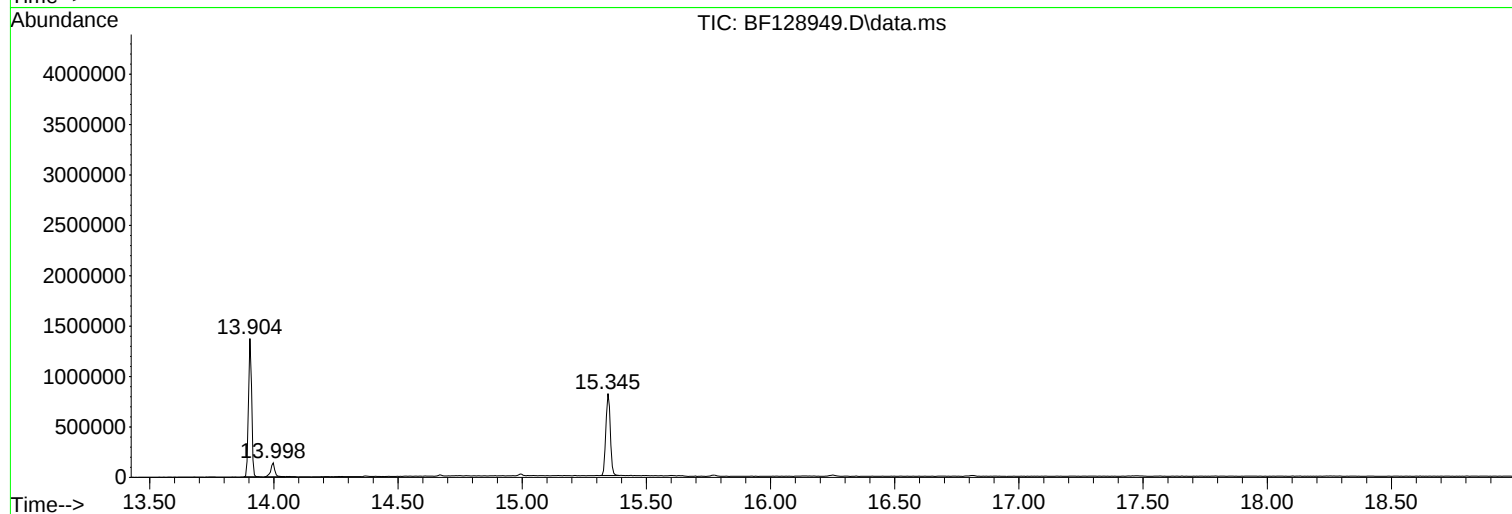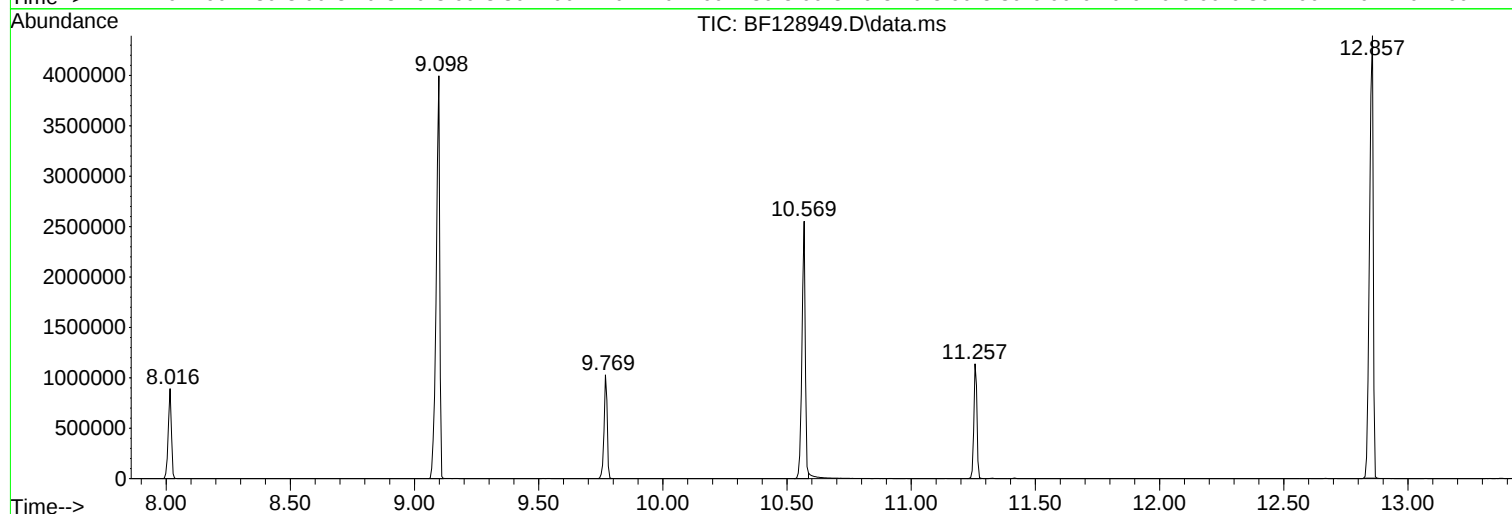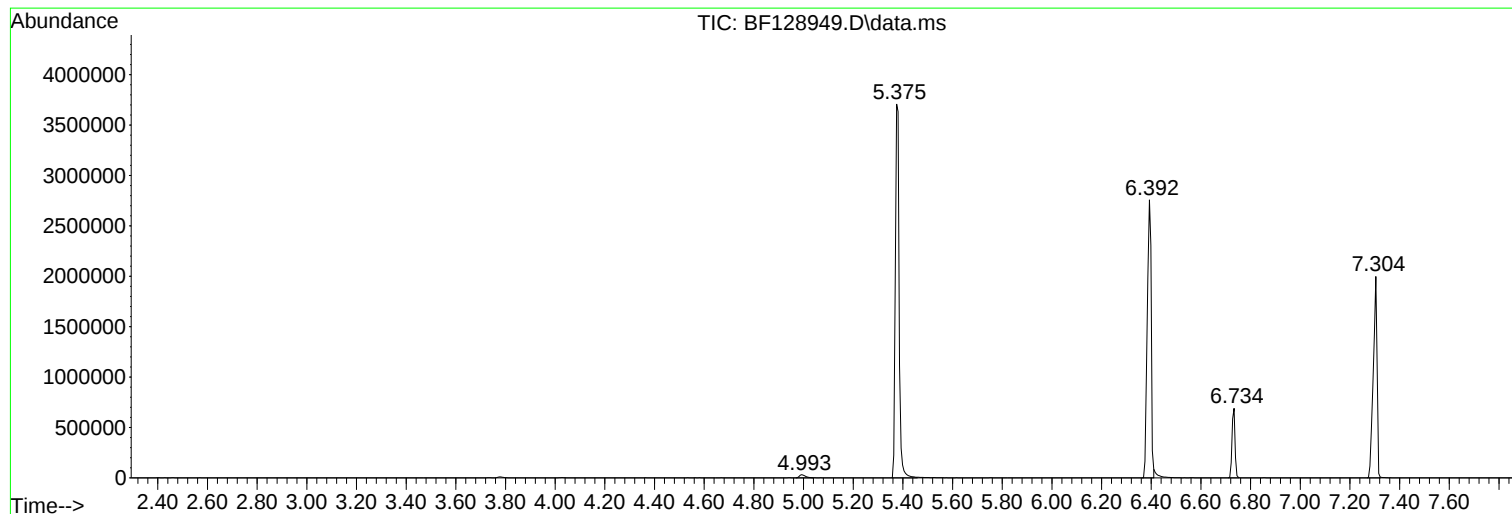

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128949.D
Acq On : 23 Jun 2022 12:10
Operator : CG\JU
Sample : PB145641BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145641BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.998	2.63 ng	156867	Chrysene-d12	13.904

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	38
4			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	25
5			2-Indolinone, 2TMS derivative	277	C14H23NOSi2	010416-65-6	9

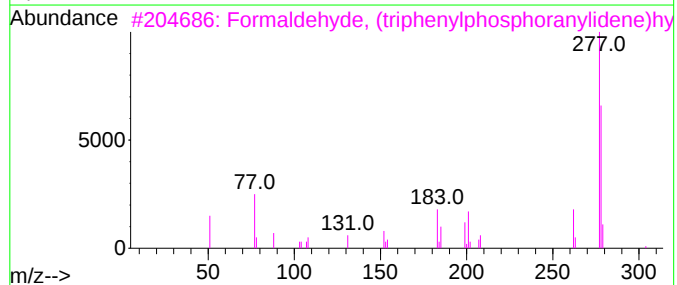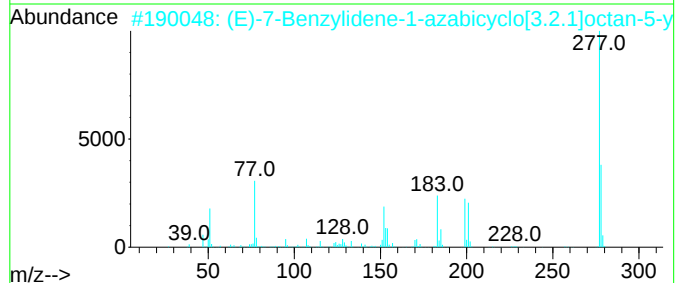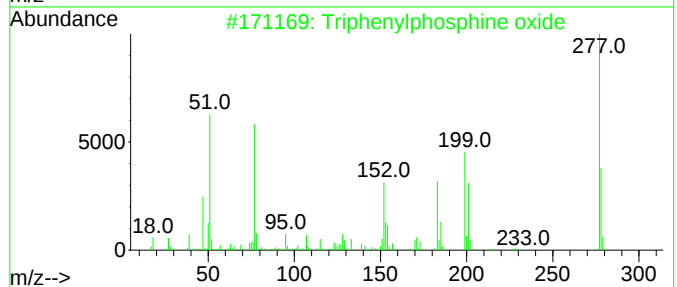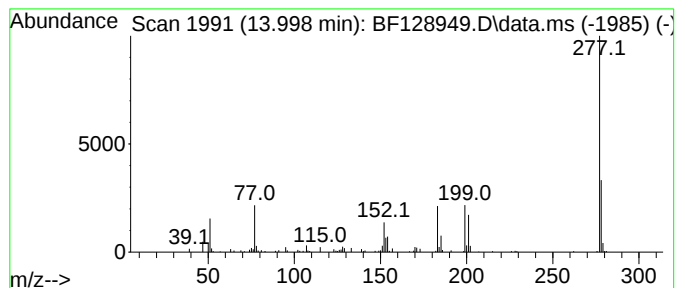

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128949.D
Acq On : 23 Jun 2022 12:10
Operator : CG\JU
Sample : PB145641BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145641BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	13.998	2.6	ng	156867	5	13.904	1190920	20.0