

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
 Data File : BF128954.D
 Acq On : 23 Jun 2022 14:59
 Operator : CG\JU
 Sample : PB145641BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145641BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.375	521	525	544	rBV	3697096	3839187	69.25%	12.445%
2	6.392	693	698	701	rBV	3445336	3851964	69.48%	12.486%
3	6.733	752	756	759	rBV	933132	818835	14.77%	2.654%
4	7.304	847	853	856	rBV	2488423	2768426	49.93%	8.974%
5	8.016	969	974	978	rBV	1210120	1085130	19.57%	3.517%
6	9.098	1151	1158	1161	rBV	5007302	5003212	90.24%	16.218%
7	9.769	1266	1272	1276	rBV	1391326	1292050	23.31%	4.188%
8	10.569	1401	1408	1411	rBV	3084560	3057070	55.14%	9.909%
9	11.257	1519	1525	1529	rBV	1467780	1399275	25.24%	4.536%
10	12.857	1791	1797	1800	rVB	5266722	5544072	100.00%	17.971%
11	13.904	1971	1975	1979	rBV	1287939	1184053	21.36%	3.838%
12	13.998	1985	1991	1999	rVB	89460	103072	1.86%	0.334%
13	15.345	2215	2220	2227	rBV	586789	788690	14.23%	2.557%
14	15.768	2288	2292	2298	rVB3	37062	59349	1.07%	0.192%
15	16.250	2369	2374	2382	rVB4	28840	55721	1.01%	0.181%




Sum of corrected areas: 30850106

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128954.D
Acq On : 23 Jun 2022 14:59
Operator : CG\JU
Sample : PB145641BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145641BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

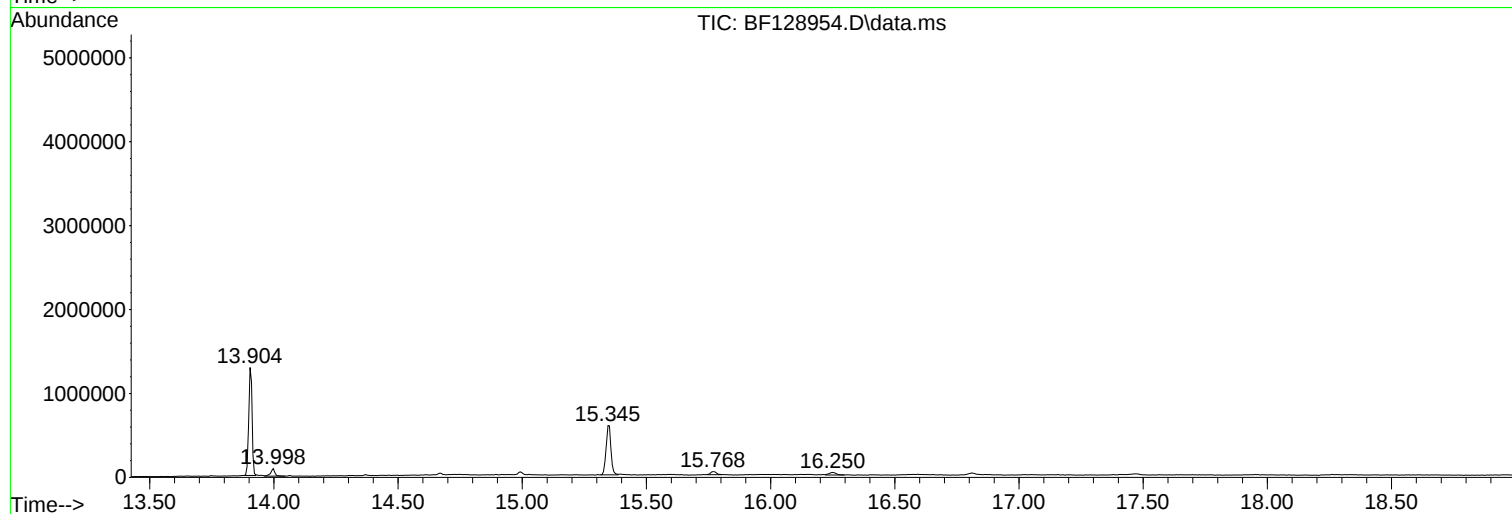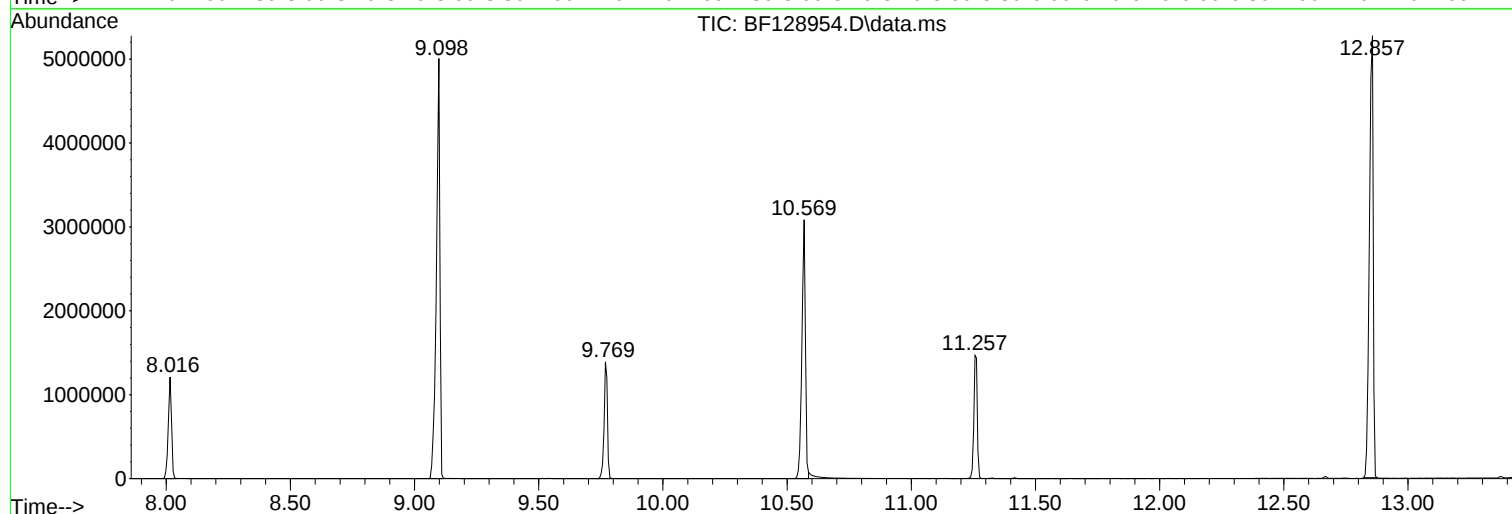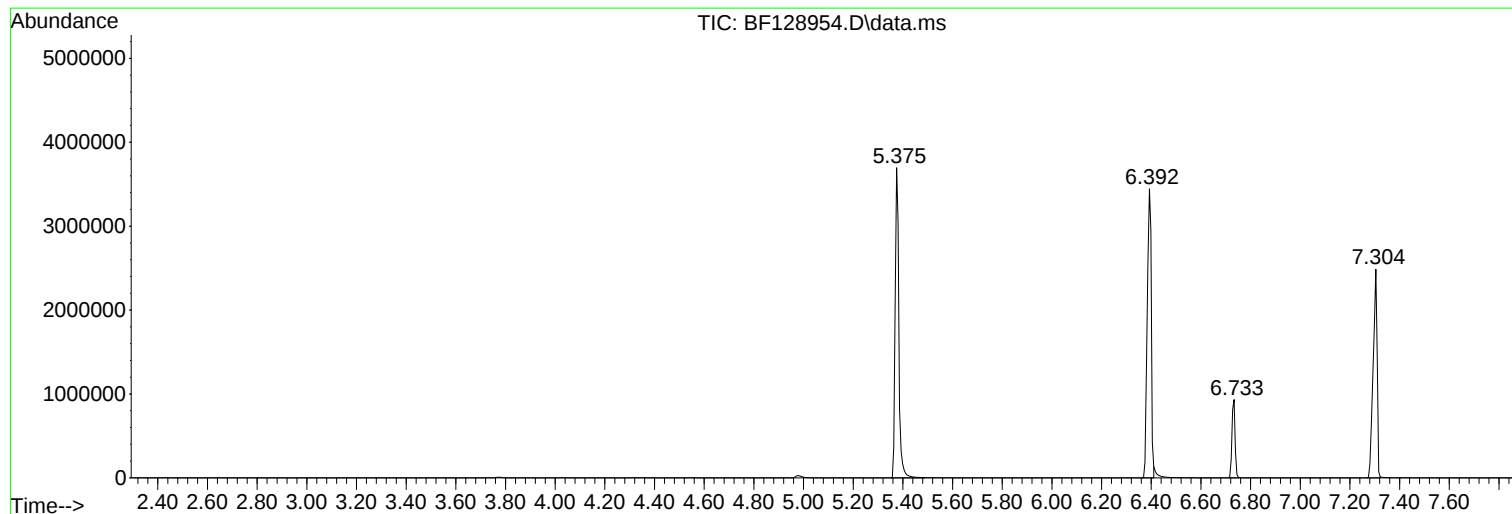

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128954.D
Acq On : 23 Jun 2022 14:59
Operator : CG\JU
Sample : PB145641BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145641BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128954.D
Acq On : 23 Jun 2022 14:59
Operator : CG\JU
Sample : PB145641BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145641BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------