

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
 Data File : BF128962.D
 Acq On : 23 Jun 2022 20:08
 Operator : CG\JU
 Sample : N3469-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 XRDS-SCREENED-CLEAN-FILL-SP-1-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.357	519	522	548	rBV	2464598	2529533	81.24%	12.215%
2	6.381	693	696	710	rBV	2436939	2510569	80.63%	12.124%
3	6.722	751	754	761	rBV	853904	699041	22.45%	3.376%
4	7.292	846	851	854	rBV	1792606	1712275	54.99%	8.269%
5	8.010	968	973	976	rBV	930066	893619	28.70%	4.315%
6	9.086	1150	1156	1159	rBV	3561247	3113682	100.00%	15.036%
7	9.763	1266	1271	1274	rBV	1247482	997730	32.04%	4.818%
8	10.557	1401	1406	1409	rBV	1832834	1757453	56.44%	8.487%
9	11.251	1520	1524	1526	rBV	1065732	1017121	32.67%	4.912%
10	11.269	1526	1527	1531	rVV	161174	118120	3.79%	0.570%
11	11.322	1531	1536	1539	rVB	35408	37587	1.21%	0.182%
12	11.639	1586	1590	1596	rBV2	33548	35682	1.15%	0.172%
13	11.780	1611	1614	1618	rBV2	49140	46465	1.49%	0.224%
14	11.863	1624	1628	1630	rBV	43295	43549	1.40%	0.210%
15	12.463	1726	1730	1734	rBV	225762	195531	6.28%	0.944%
16	12.692	1763	1769	1774	rBV	209836	234147	7.52%	1.131%
17	12.839	1789	1794	1797	rBV	2947680	2741863	88.06%	13.241%
18	13.892	1967	1973	1976	rBV	810568	799797	25.69%	3.862%
19	13.916	1976	1977	1980	rVB	81945	54070	1.74%	0.261%
20	13.986	1985	1989	1995	rVB	145574	156906	5.04%	0.758%
21	14.915	2144	2147	2154	rBV	72044	117170	3.76%	0.566%
22	15.210	2194	2197	2203	rVB	40413	52325	1.68%	0.253%
23	15.268	2204	2207	2212	rVV	61446	75346	2.42%	0.364%
24	15.327	2212	2217	2229	rVB	534073	663116	21.30%	3.202%
25	16.739	2453	2457	2463	rVB	27770	45245	1.45%	0.218%
26	17.157	2525	2528	2539	rVB2	27079	59866	1.92%	0.289%




Sum of corrected areas: 20707808

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128962.D
Acq On : 23 Jun 2022 20:08
Operator : CG\JU
Sample : N3469-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
XRDS-SCREENED-CLEAN-FILL-SP-1-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

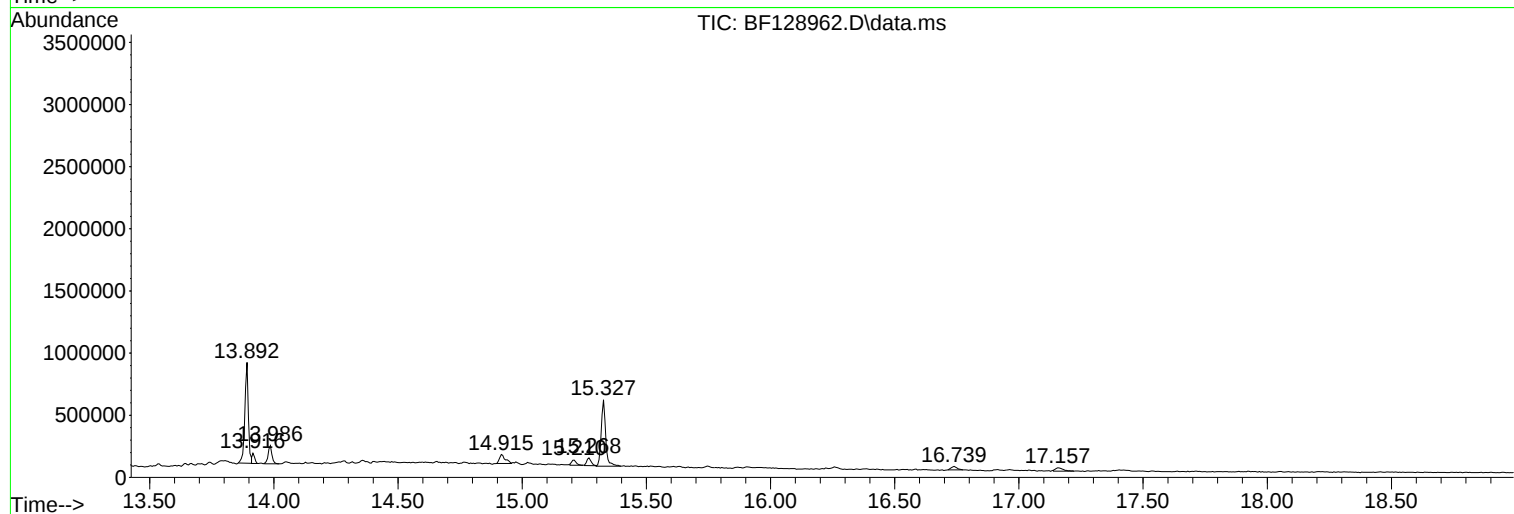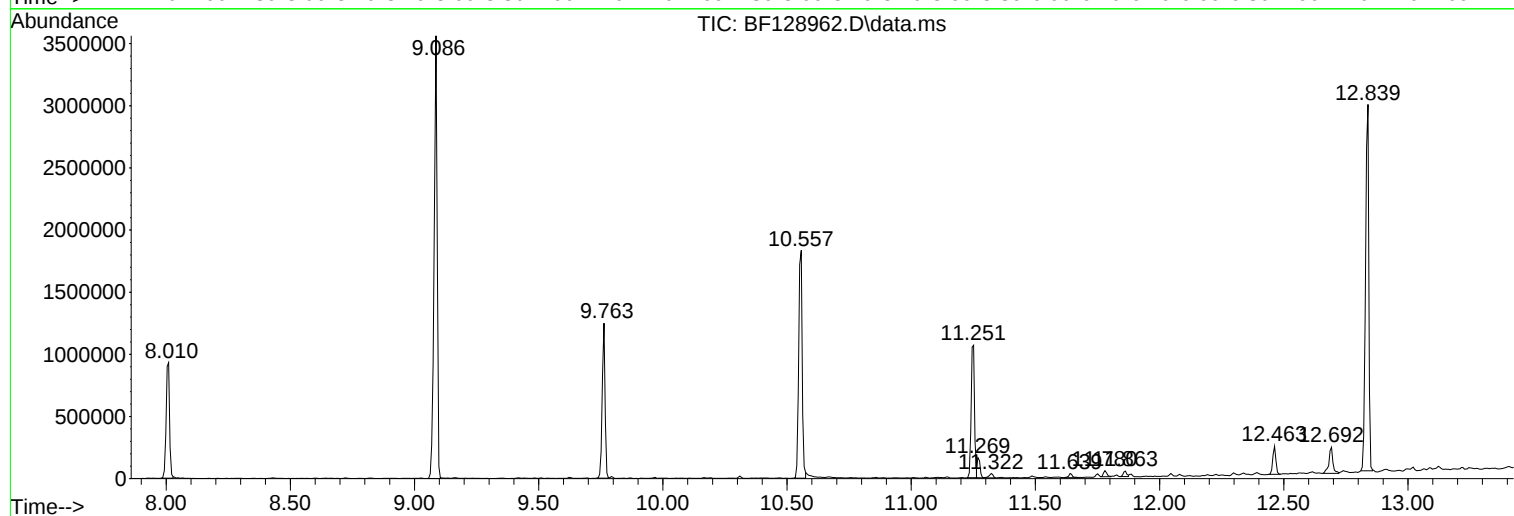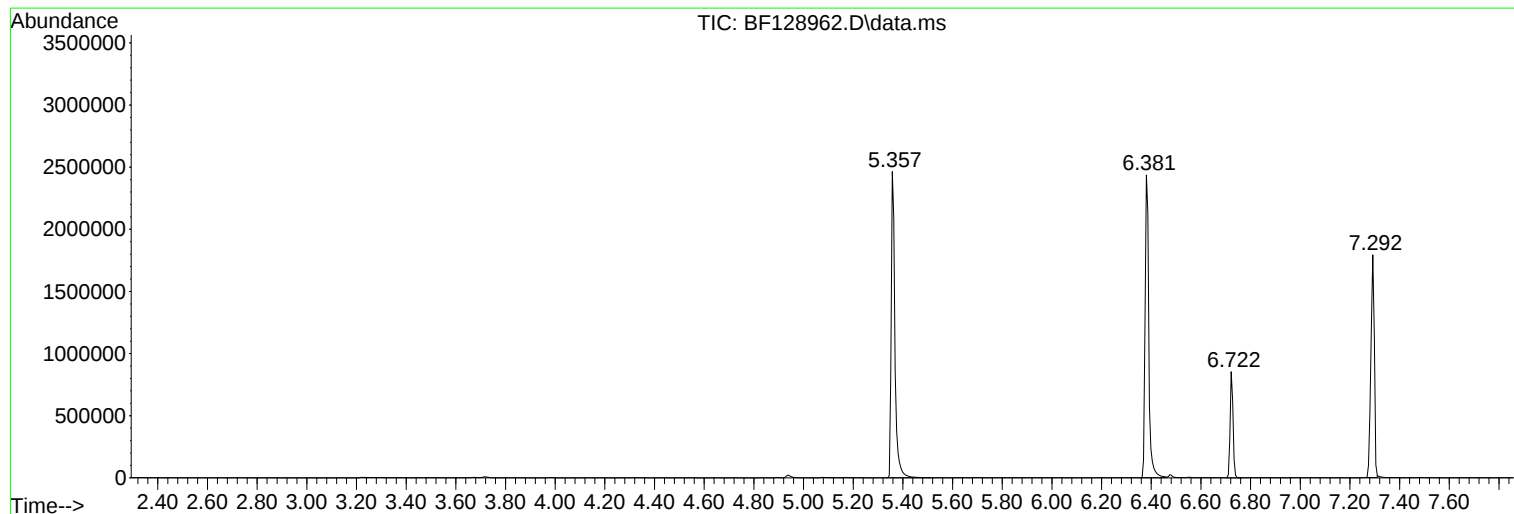

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128962.D
Acq On : 23 Jun 2022 20:08
Operator : CG\JU
Sample : N3469-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
XRDS-SCREENED-CLEAN-FILL-SP-1-COMP










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.986	3.92 ng	156906	Chrysene-d12	13.892

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	47
4			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
5			3-(3,4-Dichlorophenyl)-2-thioxo-...	277	C9H5Cl2NOS2	017046-34-3	43

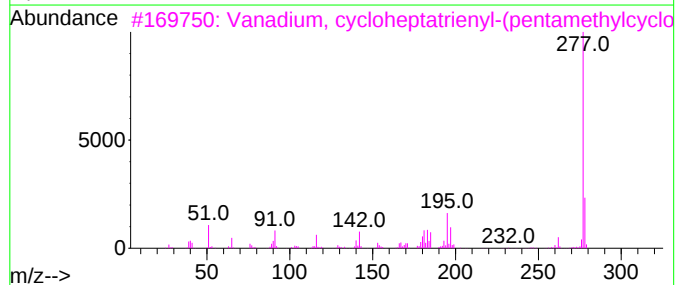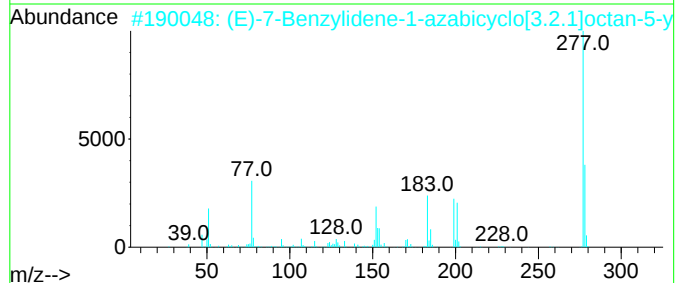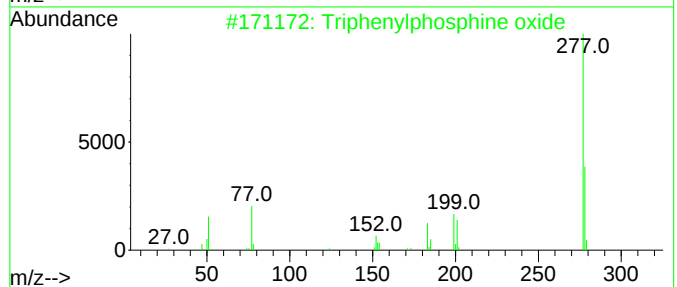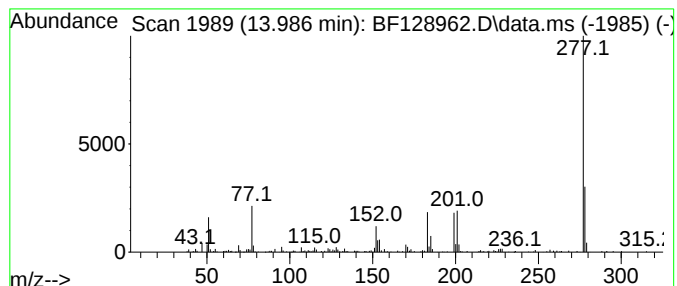

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128962.D
Acq On : 23 Jun 2022 20:08
Operator : CG\JU
Sample : N3469-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
XRDS-SCREENED-CLEAN-FILL-SP-1-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	13.986	3.9	ng	156906	5	13.892	799797	20.0