

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
 Data File : BF128963.D
 Acq On : 23 Jun 2022 20:37
 Operator : CG\JU
 Sample : N3467-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 QA-QC-COMP-XRDS008-22

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128963.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.957	450	454	464	rBV	27605	43043	1.00%	0.158%
2	5.363	519	523	541	rBV	3657893	3604406	84.10%	13.272%
3	6.386	692	697	700	rBV	3500478	3535725	82.50%	13.019%
4	6.722	751	754	761	rVB	794920	692288	16.15%	2.549%
5	7.298	846	852	855	rBV	2402872	2521519	58.83%	9.284%
6	8.010	968	973	976	rBV	914390	879497	20.52%	3.238%
7	9.086	1150	1156	1159	rBV	4371023	4285885	100.00%	15.781%
8	9.763	1263	1271	1274	rBV	1234161	1009099	23.54%	3.716%
9	10.410	1376	1381	1388	rBV2	32599	46853	1.09%	0.173%
10	10.557	1401	1406	1409	rBV	2770370	2506497	58.48%	9.229%
11	10.674	1422	1426	1433	rVB3	67953	100327	2.34%	0.369%
12	11.145	1503	1506	1509	rVB	46972	49810	1.16%	0.183%
13	11.245	1520	1523	1526	rBV	1062059	1020048	23.80%	3.756%
14	11.268	1526	1527	1531	rVV	224616	178177	4.16%	0.656%
15	11.321	1532	1536	1539	rVB	56030	61889	1.44%	0.228%
16	11.639	1587	1590	1596	rVB2	50070	57442	1.34%	0.212%
17	11.780	1611	1614	1618	rBV2	55522	63586	1.48%	0.234%
18	12.463	1726	1730	1735	rVB	301023	265901	6.20%	0.979%
19	12.692	1763	1769	1774	rBV	255904	281634	6.57%	1.037%
20	12.839	1789	1794	1797	rBV	4119368	3756545	87.65%	13.832%
21	13.398	1886	1889	1895	rBV2	64741	71535	1.67%	0.263%
22	13.780	1950	1954	1965	rVV8	30790	97172	2.27%	0.358%
23	13.892	1966	1973	1976	rVV	750306	807593	18.84%	2.974%
24	13.915	1976	1977	1981	rVV	93679	67195	1.57%	0.247%
25	13.986	1984	1989	1994	rVB	149728	165441	3.86%	0.609%
26	14.915	2144	2147	2150	rBV	81775	113021	2.64%	0.416%
27	15.204	2193	2196	2202	rVB	51080	61300	1.43%	0.226%
28	15.268	2203	2207	2212	rVV	64695	84416	1.97%	0.311%
29	15.327	2212	2217	2228	rVB	478001	618839	14.44%	2.279%
30	16.733	2452	2456	2464	rBV2	31747	59399	1.39%	0.219%
31	17.156	2524	2528	2535	rVB2	25546	52636	1.23%	0.194%




Sum of corrected areas: 27158718

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128963.D
Acq On : 23 Jun 2022 20:37
Operator : CG\JU
Sample : N3467-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
QA-QC-COMP-XRDS008-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

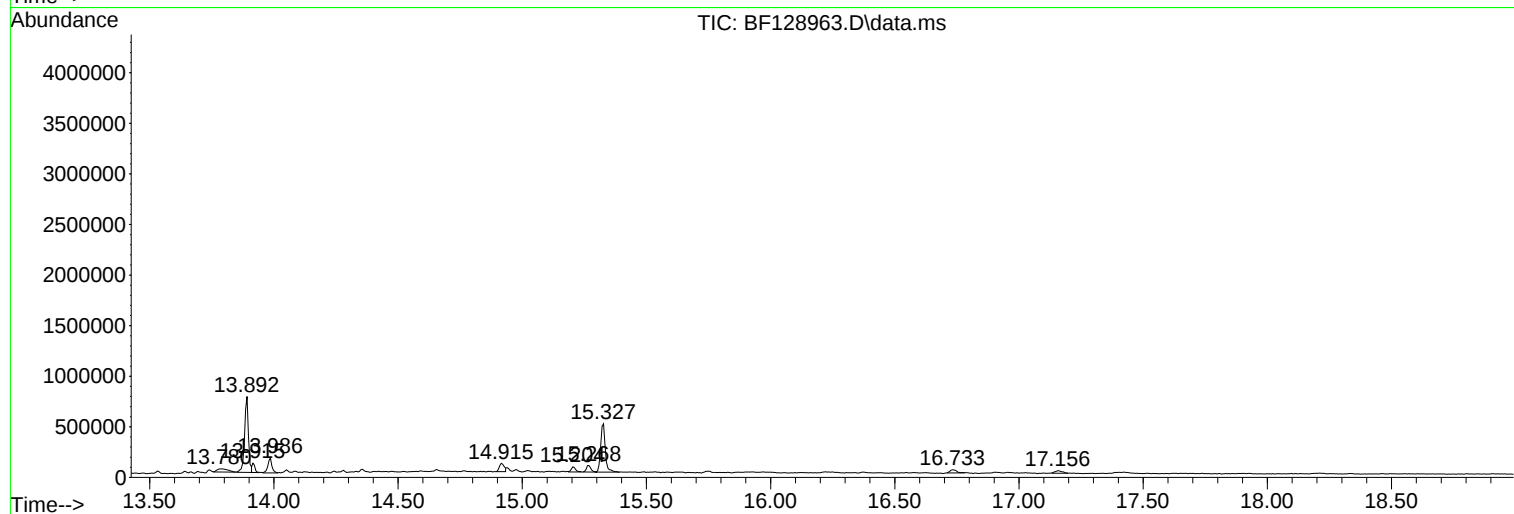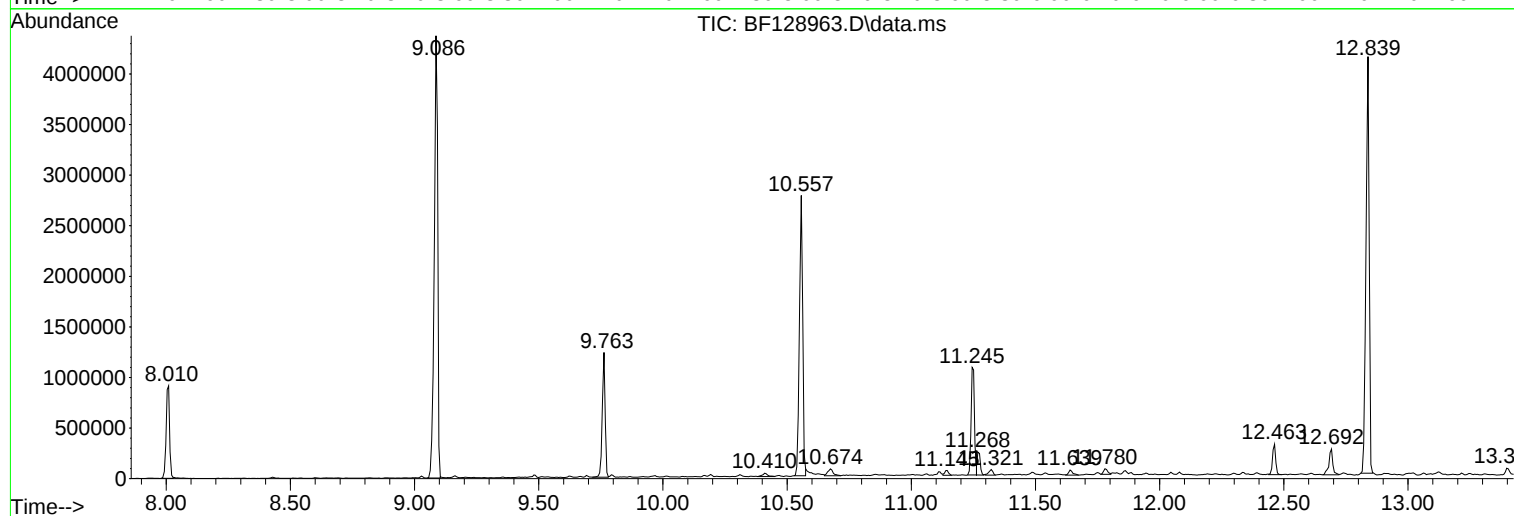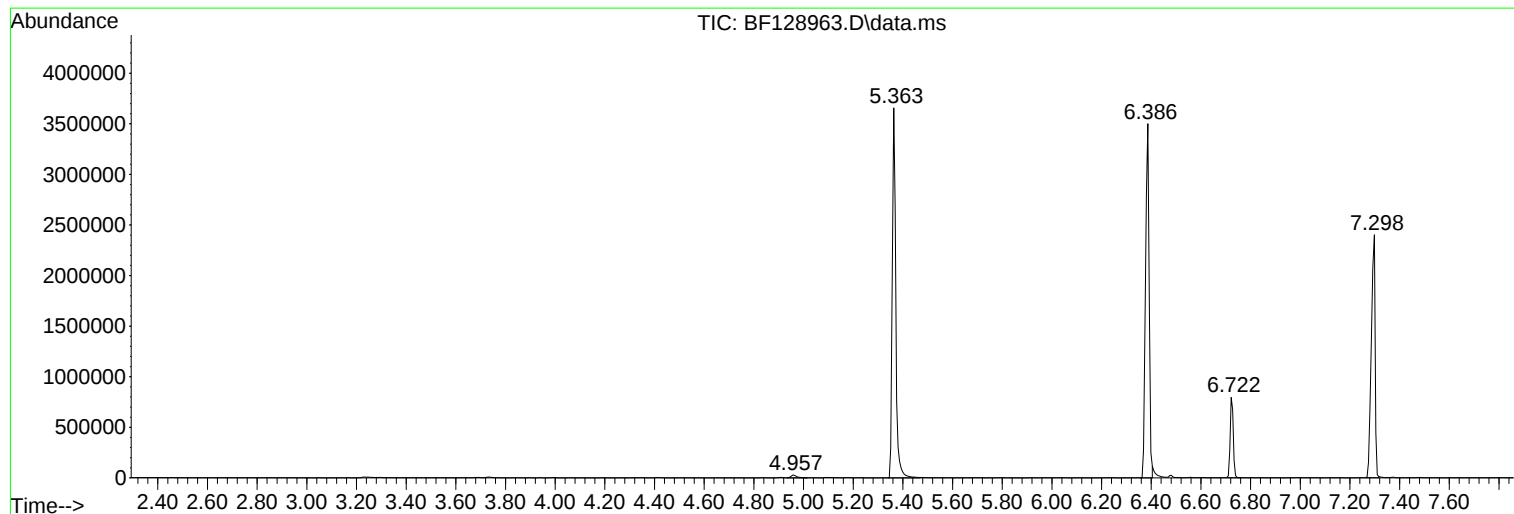

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128963.D
Acq On : 23 Jun 2022 20:37
Operator : CG\JU
Sample : N3467-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
QA-QC-COMP-XRDS008-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128963.D
Acq On : 23 Jun 2022 20:37
Operator : CG\JU
Sample : N3467-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
QA-QC-COMP-XRDS008-22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------