


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
 Data File : BF128945.D
 Acq On : 23 Jun 2022 09:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 00:50:48 2022

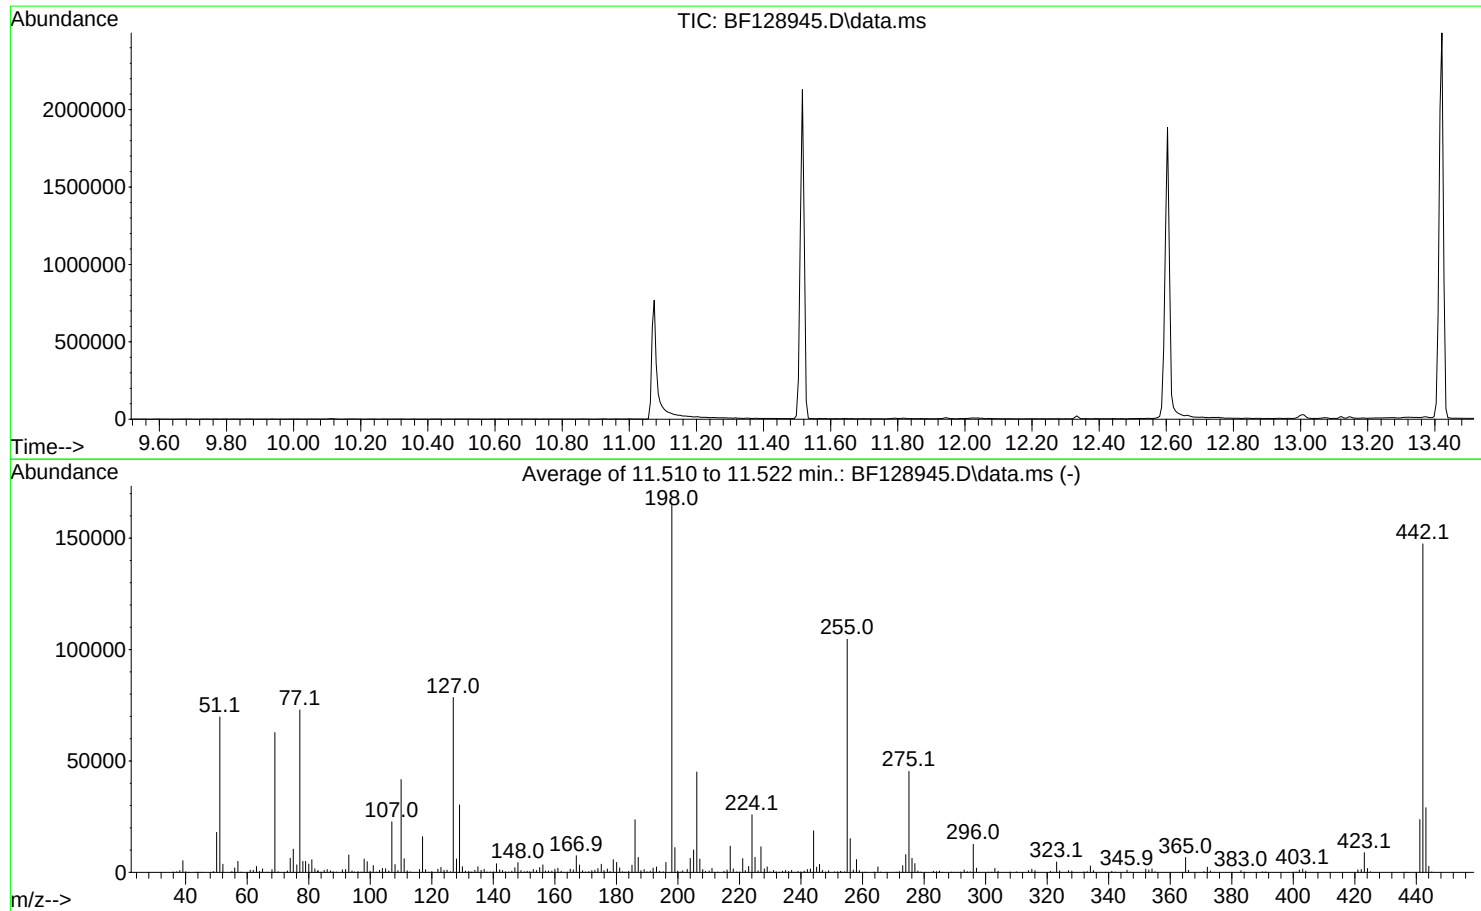




AutoFind: Scans 1568, 1569, 1570; Background Corrected with Scan 1562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	69773	PASS
68	69	0.00	2	1.9	1212	PASS
69	198	0.00	100	38.0	62781	PASS
70	69	0.00	2	0.5	287	PASS
127	198	10	80	47.6	78515	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	165115	PASS
199	198	5	9	6.7	11115	PASS
275	198	10	60	27.4	45323	PASS
365	198	1	100	4.1	6696	PASS
441	198	0.01	100	14.3	23676	PASS
442	442	50	100	100.0	147448	PASS
443	442	15	24	19.7	28993	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
 Data File : BF128945.D
 Acq On : 23 Jun 2022 09:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 23 15:03:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 23 14:30:33 2022
 Response via : Initial Calibration

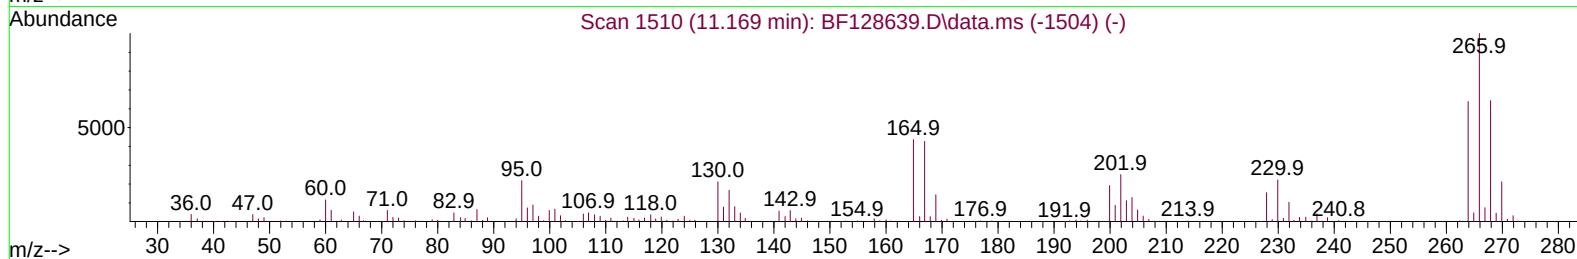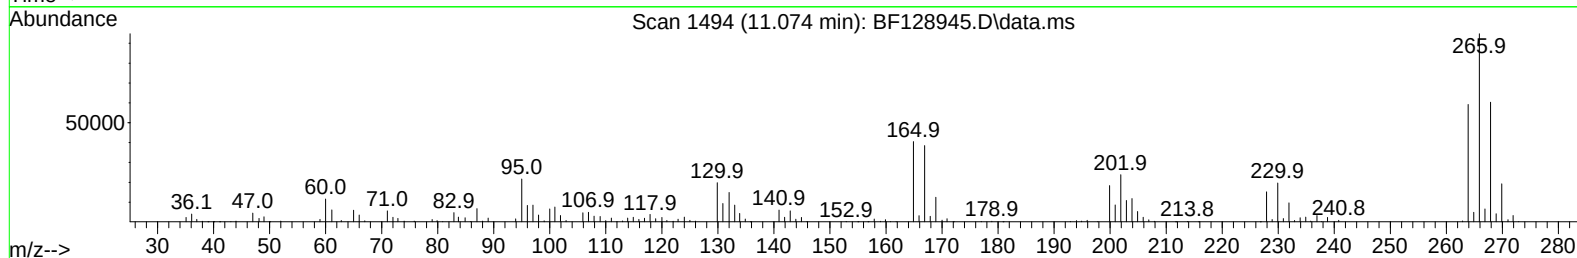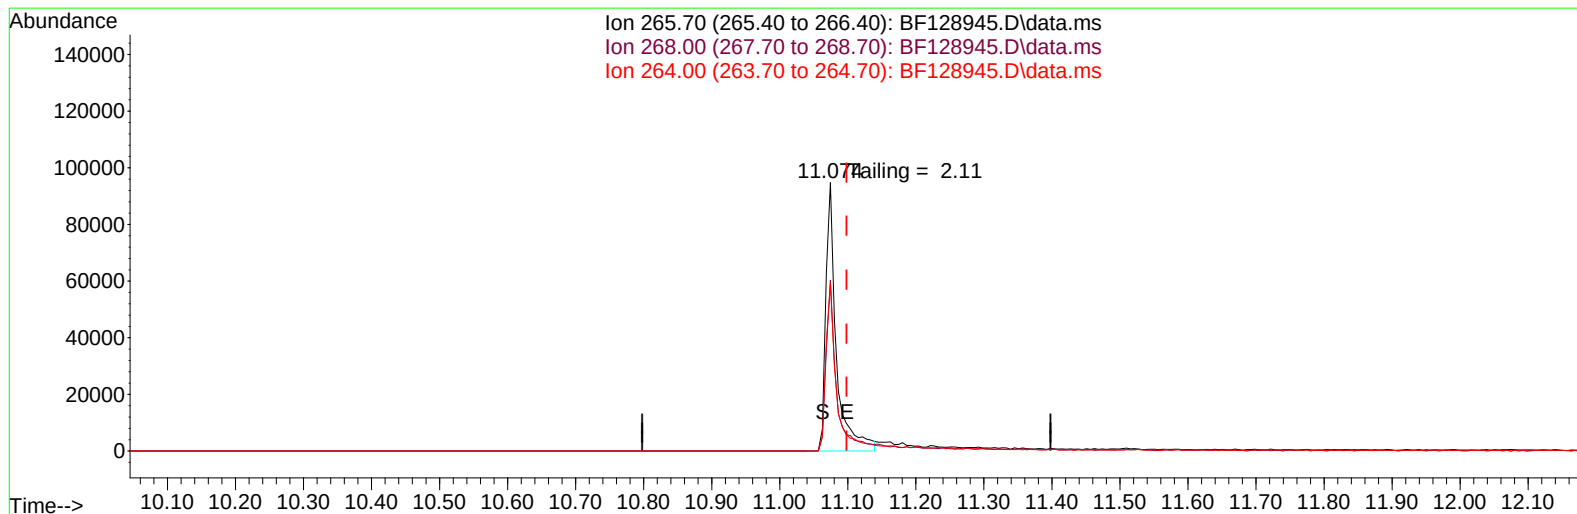

TIC: BF128945.D\data.ms

(70) Pentachlorophenol (C)

11.074min (-0.024) 21534.45 ng




response 108768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.60
264.00	61.80	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062322\
Data File : BF128945.D
Acq On : 23 Jun 2022 09:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 23 15:03:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 23 14:30:33 2022
Response via : Initial Calibration

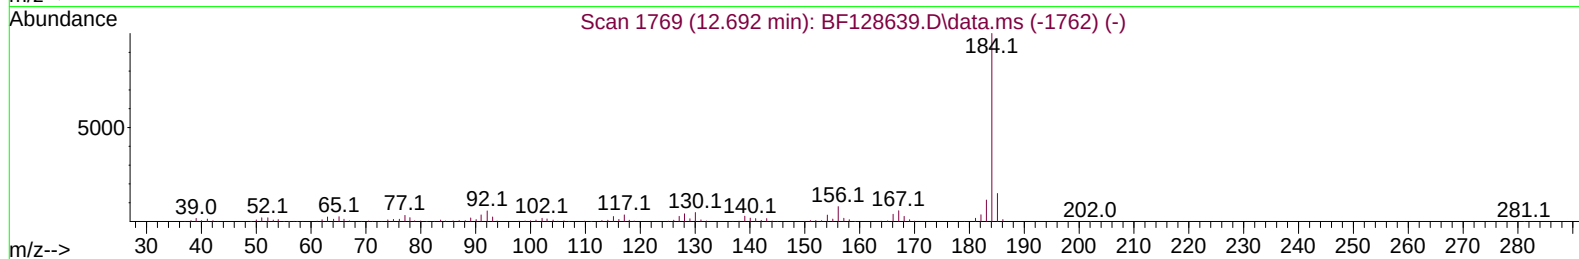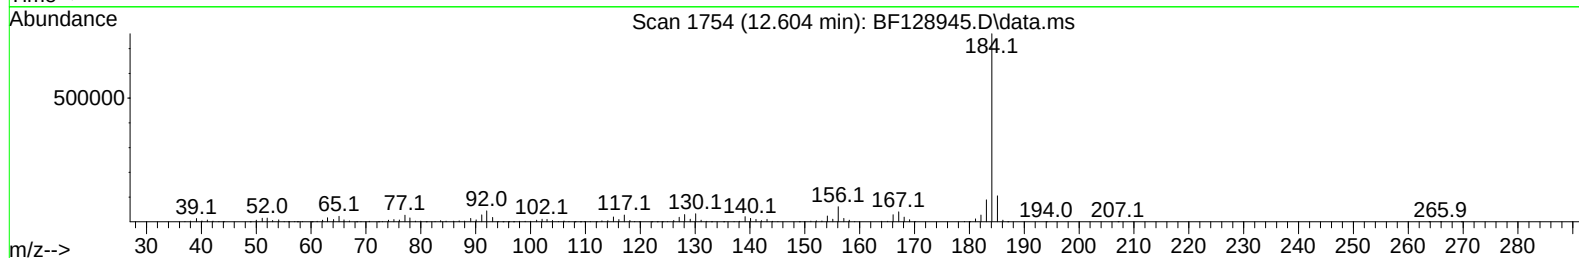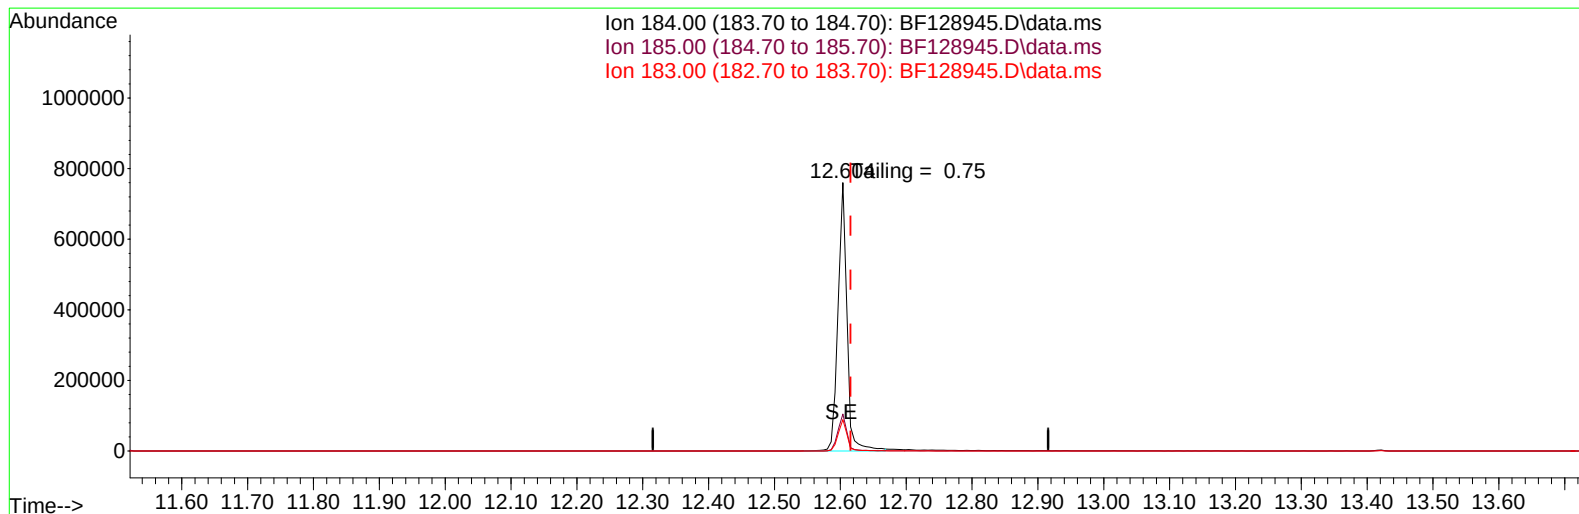

TIC: BF128945.D\data.ms

(77) Benzidine

12.604min (-0.012) 0.00 ng

response 730841

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.79
183.00	11.60	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/23/2022	BNA_F	<u>BF128945.D</u>
Compound Name	Response	Retention Time
DDT	417846	13.42
DDD	2704	13.12
DDE	0	12.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2704	420550	0.64

Instrument :
BNA_F
ClientSampleId :
DFTPP