


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062322\  
 Data File : BF128956.D  
 Acq On : 23 Jun 2022 16:42  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF060222.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jun 24 00:50:48 2022

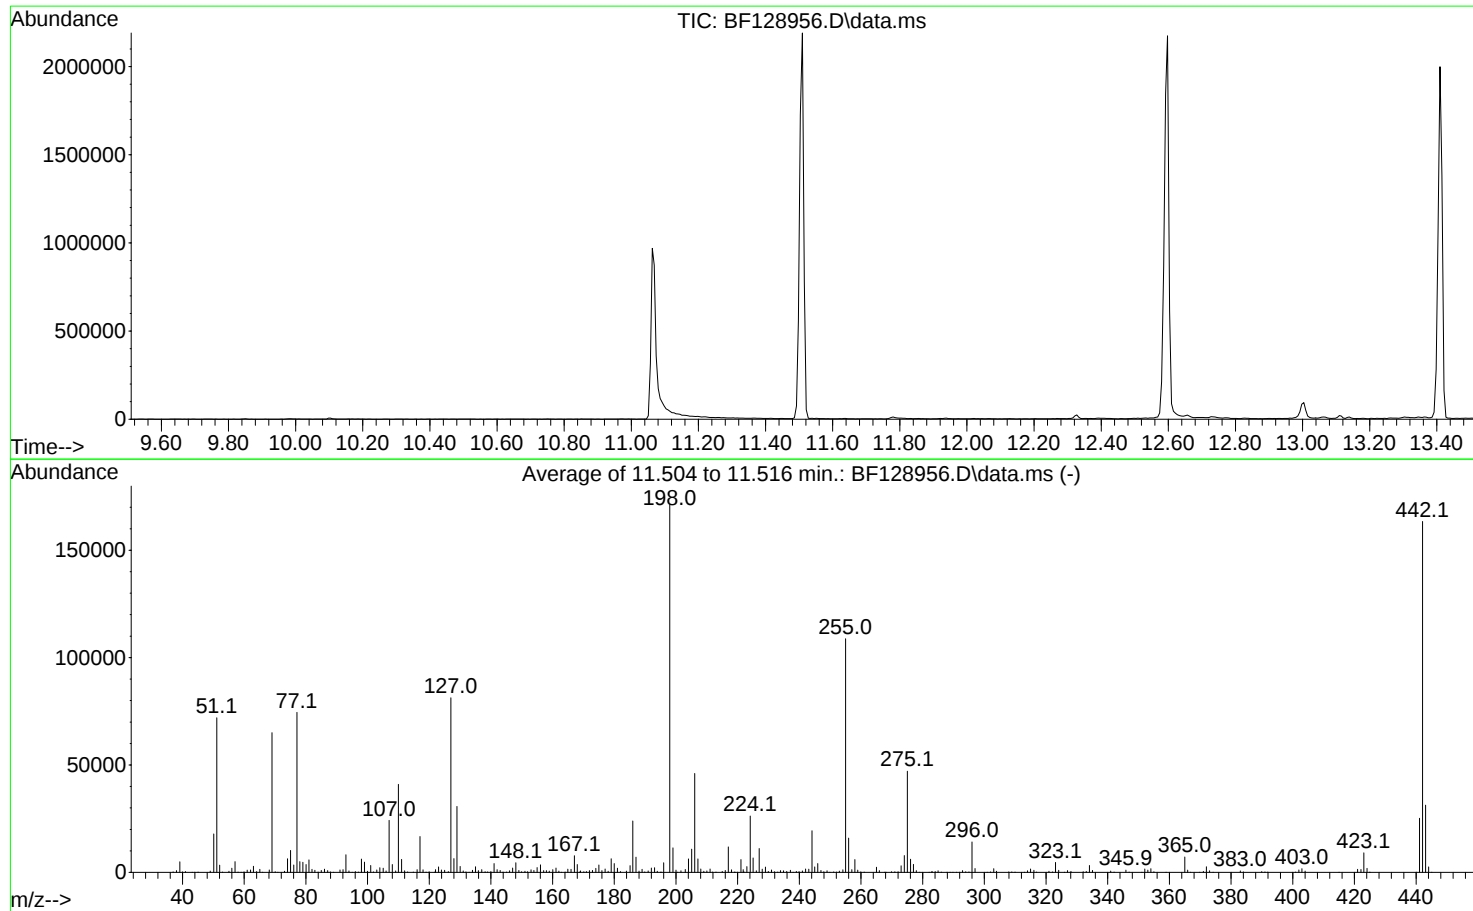




AutoFind: Scans 1567, 1568, 1569; Background Corrected with Scan 1561

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 42.0         | 71944      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 1100       | PASS                |
| 69             | 198             | 0.00            | 100             | 38.0         | 65021      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 343        | PASS                |
| 127            | 198             | 10              | 80              | 47.4         | 81267      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 171304     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 11419      | PASS                |
| 275            | 198             | 10              | 60              | 27.5         | 47131      | PASS                |
| 365            | 198             | 1               | 100             | 4.2          | 7175       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.7         | 25211      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 163395     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 31333      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062322\  
Data File : BF128956.D  
Acq On : 23 Jun 2022 16:42  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jun 24 04:31:15 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF060222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 24 00:50:48 2022  
Response via : Initial Calibration

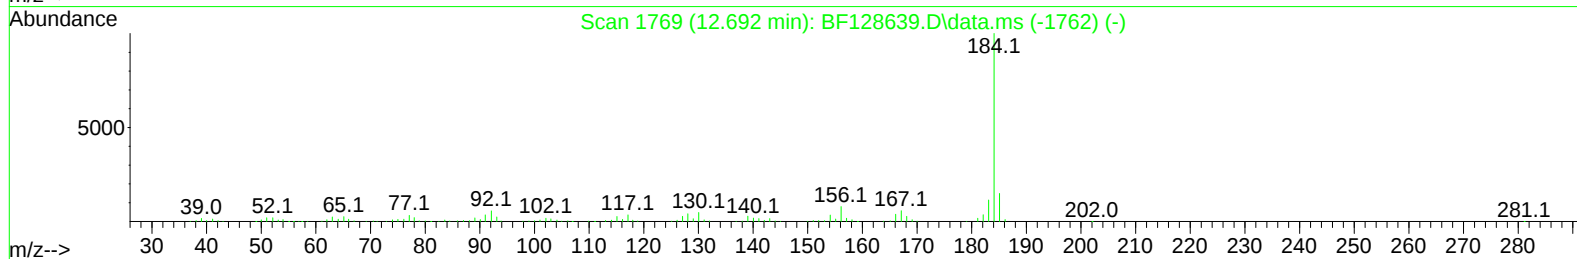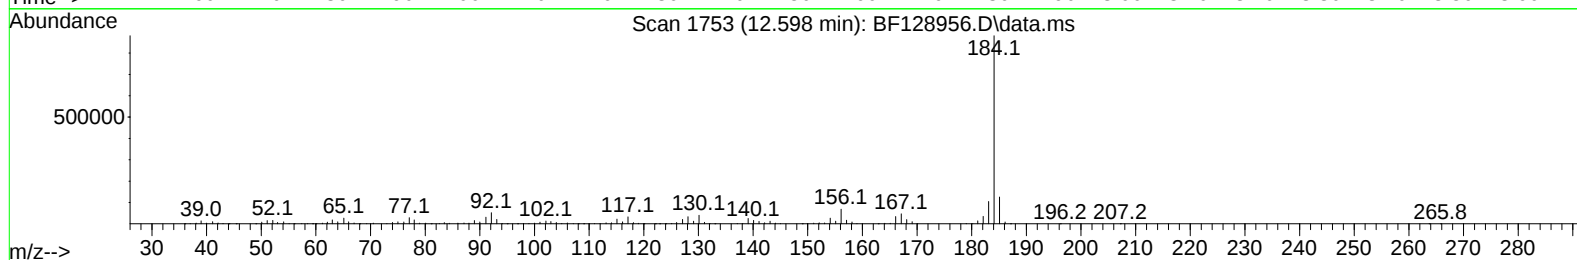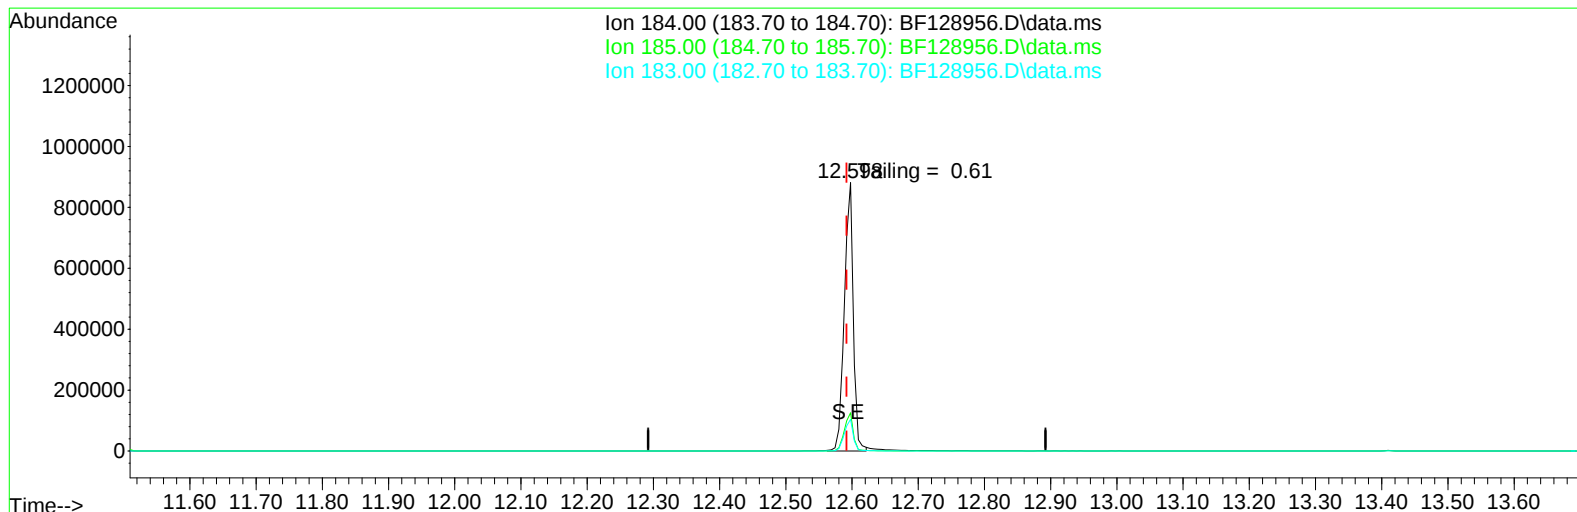

TIC: BF128956.D\data.ms

**(77) Benzidine**

**12.598min (+ 0.006) 0.00 ng**




**response 843265**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 14.25  |
| 183.00 | 11.60  | 11.83  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF062322\  
Data File : BF128956.D  
Acq On : 23 Jun 2022 16:42  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jun 24 04:31:15 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF060222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 24 00:50:48 2022  
Response via : Initial Calibration

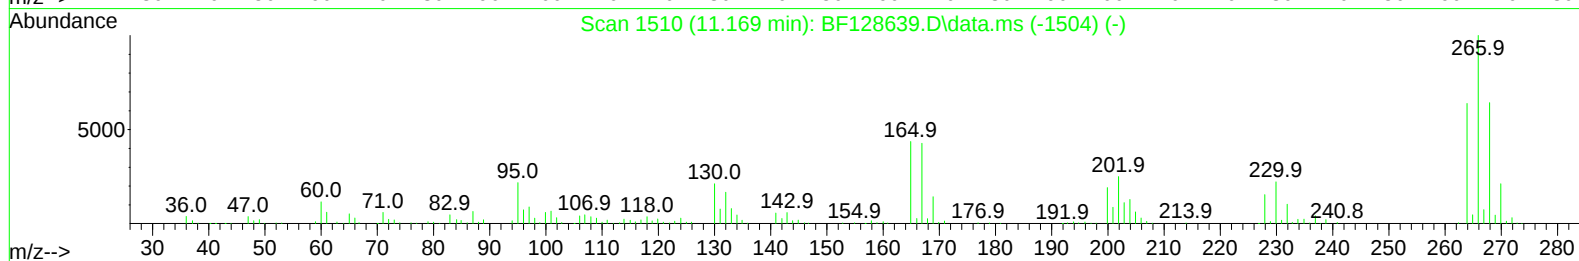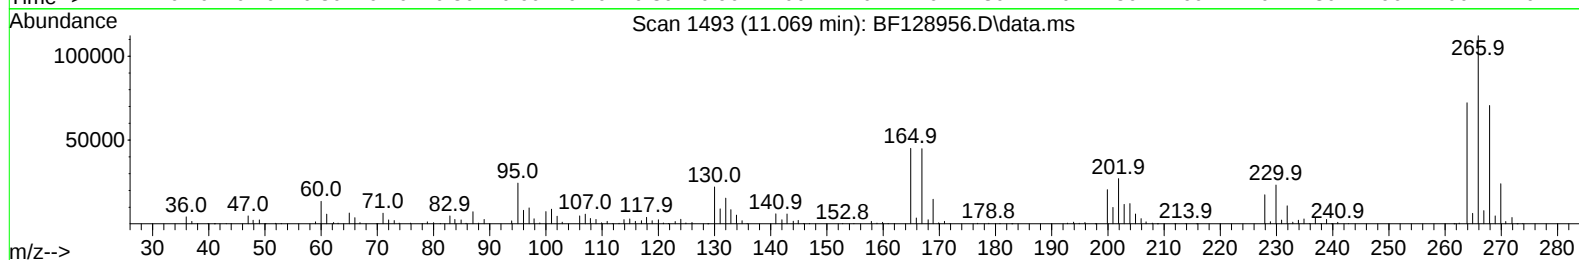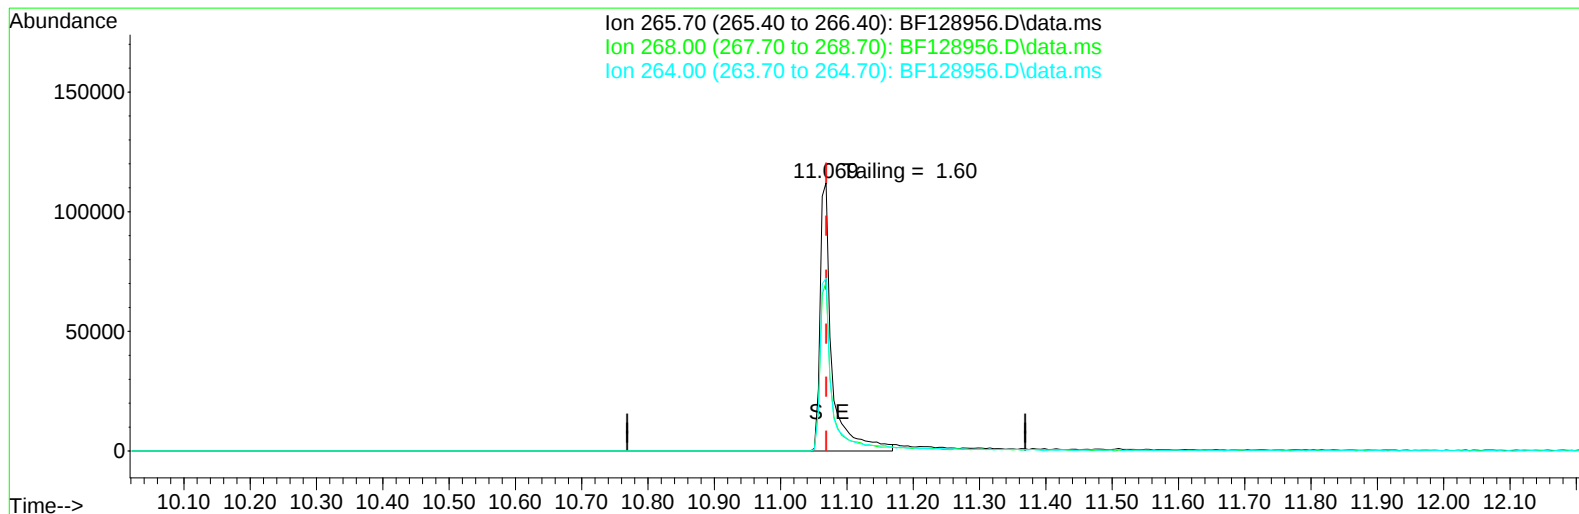

TIC: BF128956.D\data.ms

**(70) Pentachlorophenol (C)**

**11.069min (-0.000) 32512.98 ng**

**response 145727**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.70  | 62.93  |
| 264.00 | 61.80  | 64.37  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/23/2022     | BNA_F            | <u>BF128956.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 335127           | 13.42              |
| DDD           | 4931             | 13.11              |
| DDE           | 752              | 12.7               |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 5683          | 340810           | 1.67               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP