
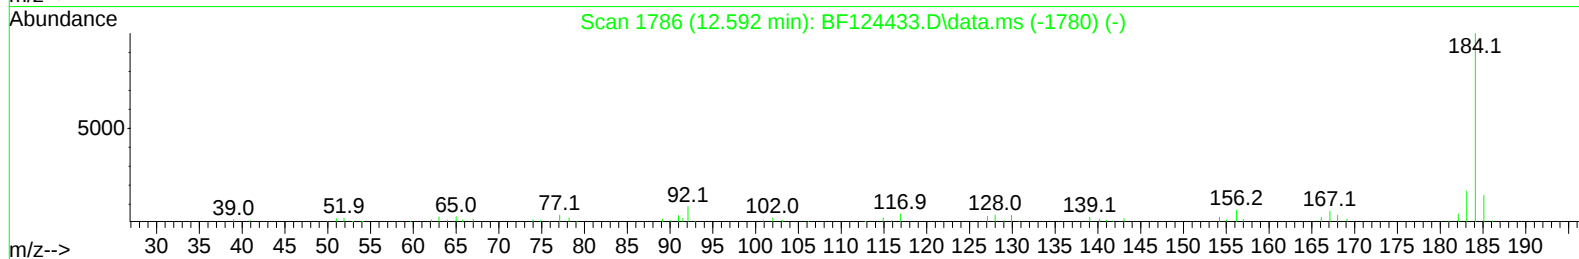
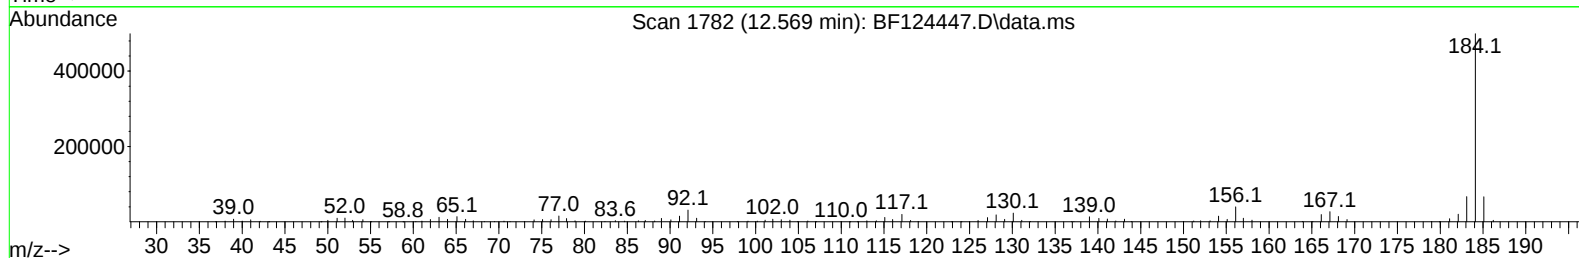


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124447.D
Acq On : 25 Jun 2021 12:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 13:19:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 18:48:27 2021
Response via : Initial Calibration

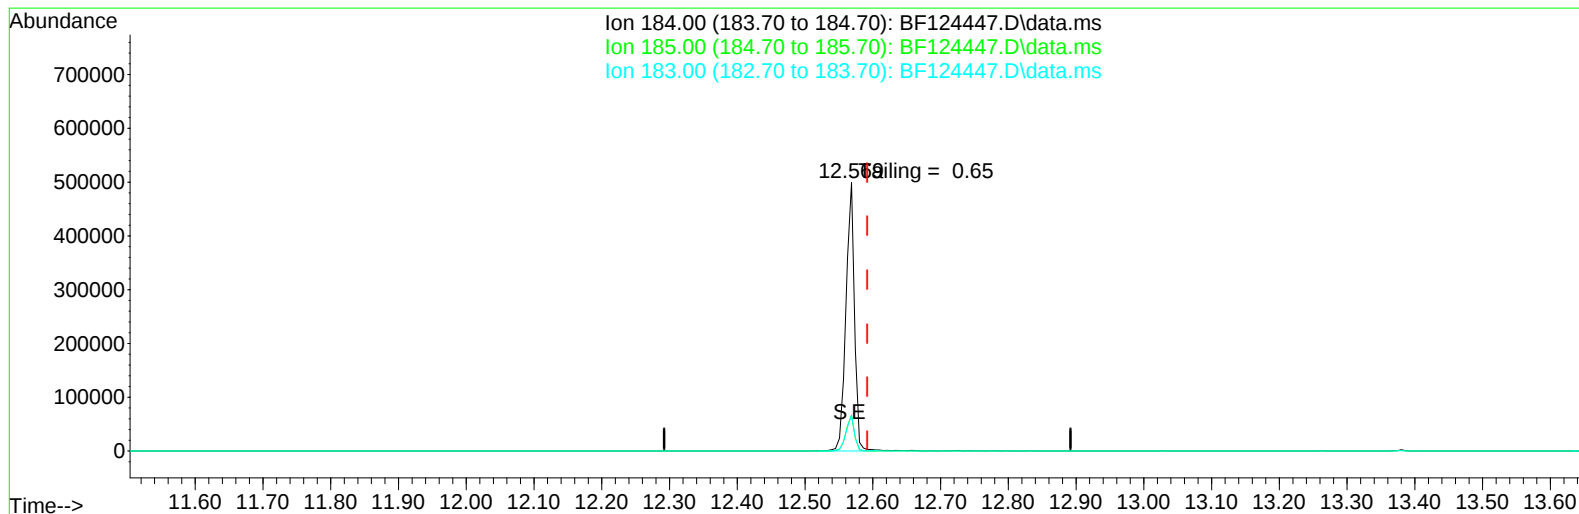

TIC: BF124447.D\data.ms

(77) Benzidine




12.569min (-0.024) 0.00 ng

response 440460

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.30
183.00	9.80	13.44#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124447.D
Acq On : 25 Jun 2021 12:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 25 13:19:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 18:48:27 2021
Response via : Initial Calibration

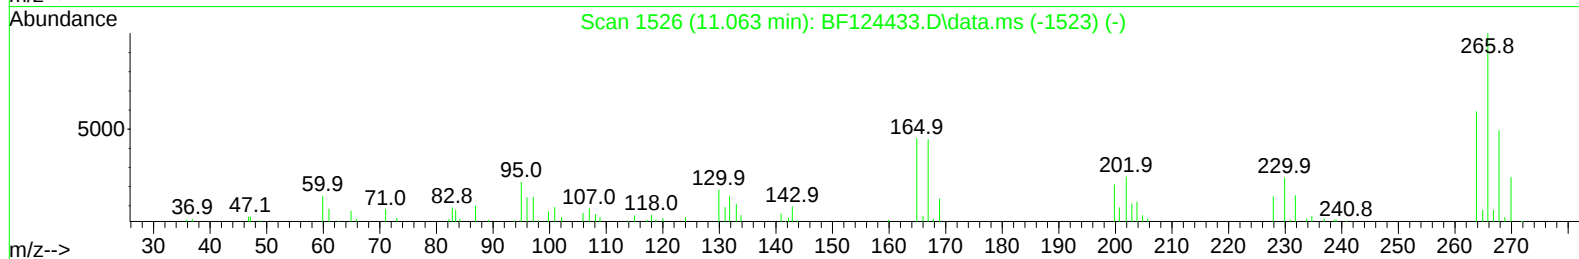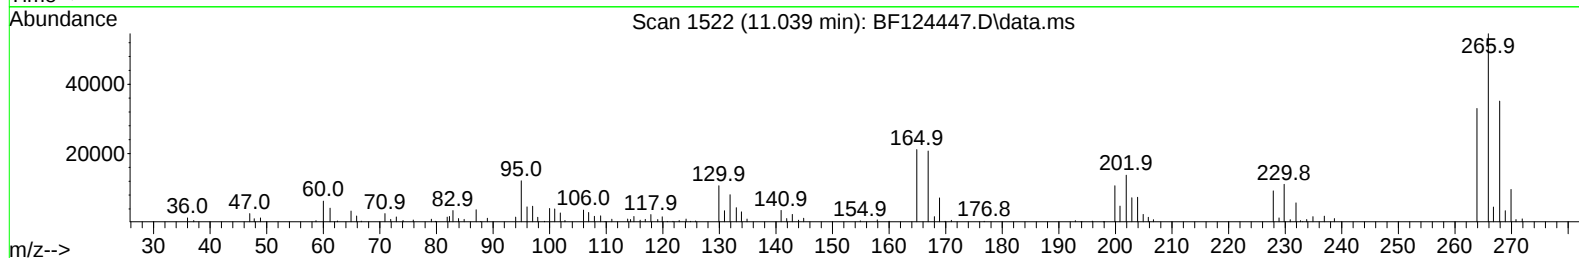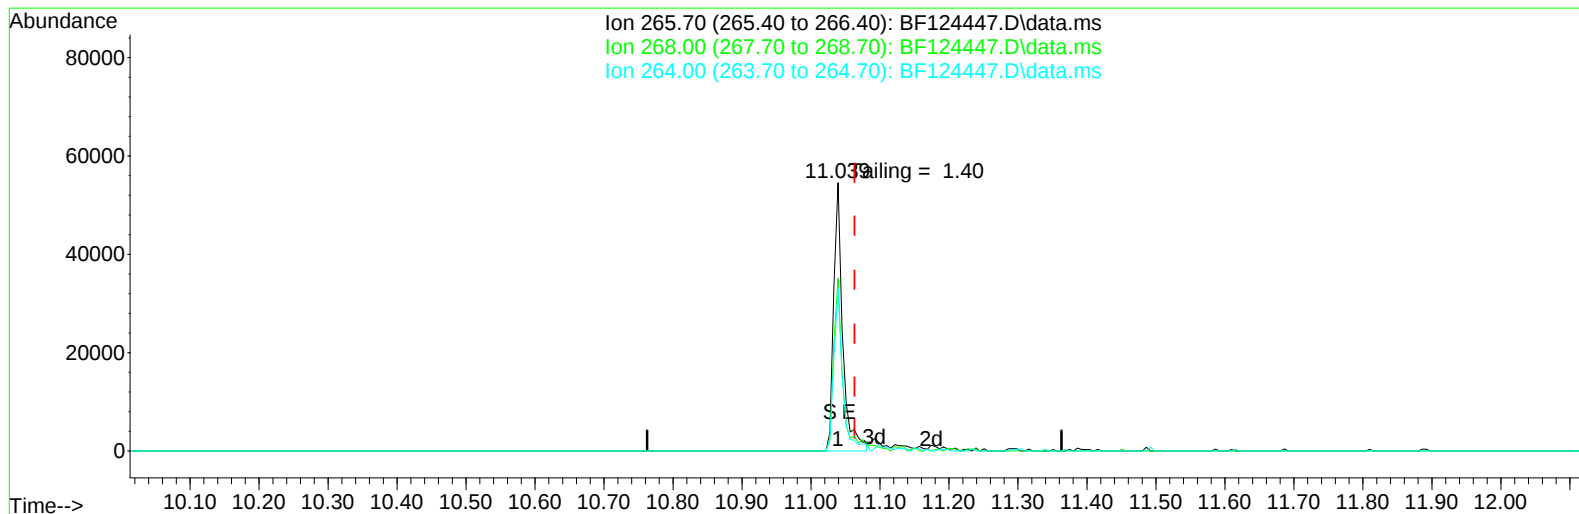

TIC: BF124447.D\data.ms

(70) Pentachlorophenol (C)

11.039min (-0.024) 68752.69 ng

response 49682

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.37
264.00	65.70	60.48
0.00	0.00	0.00