

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
 Data File : BF124464.D
 Acq On : 25 Jun 2021 21:55
 Operator : JU/CG
 Sample : M2829-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 15B-DUP-01

Quant Time: Jun 26 02:43:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 25 13:23:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.704	152	32981	20.000	ng	0.00
21) Naphthalene-d8	7.986	136	128596	20.000	ng	# 0.00
39) Acenaphthene-d10	9.739	164	69314	20.000	ng	0.00
64) Phenanthrene-d10	11.222	188	108878	20.000	ng	0.00
76) Chrysene-d12	13.863	240	84445	20.000	ng	0.00
86) Perylene-d12	15.286	264	86171	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	262305	125.079	ng	0.01
7) Phenol-d6	6.357	99	284707	103.977	ng	0.00
23) Nitrobenzene-d5	7.275	82	246889	79.603	ng	0.00
42) 2,4,6-Tribromophenol	10.533	330	102553	123.838	ng	0.00
45) 2-Fluorobiphenyl	9.063	172	475039	83.954	ng	0.00
79) Terphenyl-d14	12.810	244	419298	74.370	ng	0.00
Target Compounds						
77) Benzidine	12.563	184	63170	37.326	ng	Qvalue # 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124464.D
Acq On : 25 Jun 2021 21:55
Operator : JU/CG
Sample : M2829-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
15B-DUP-01

Quant Time: Jun 26 02:43:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 25 13:23:23 2021
Response via : Initial Calibration




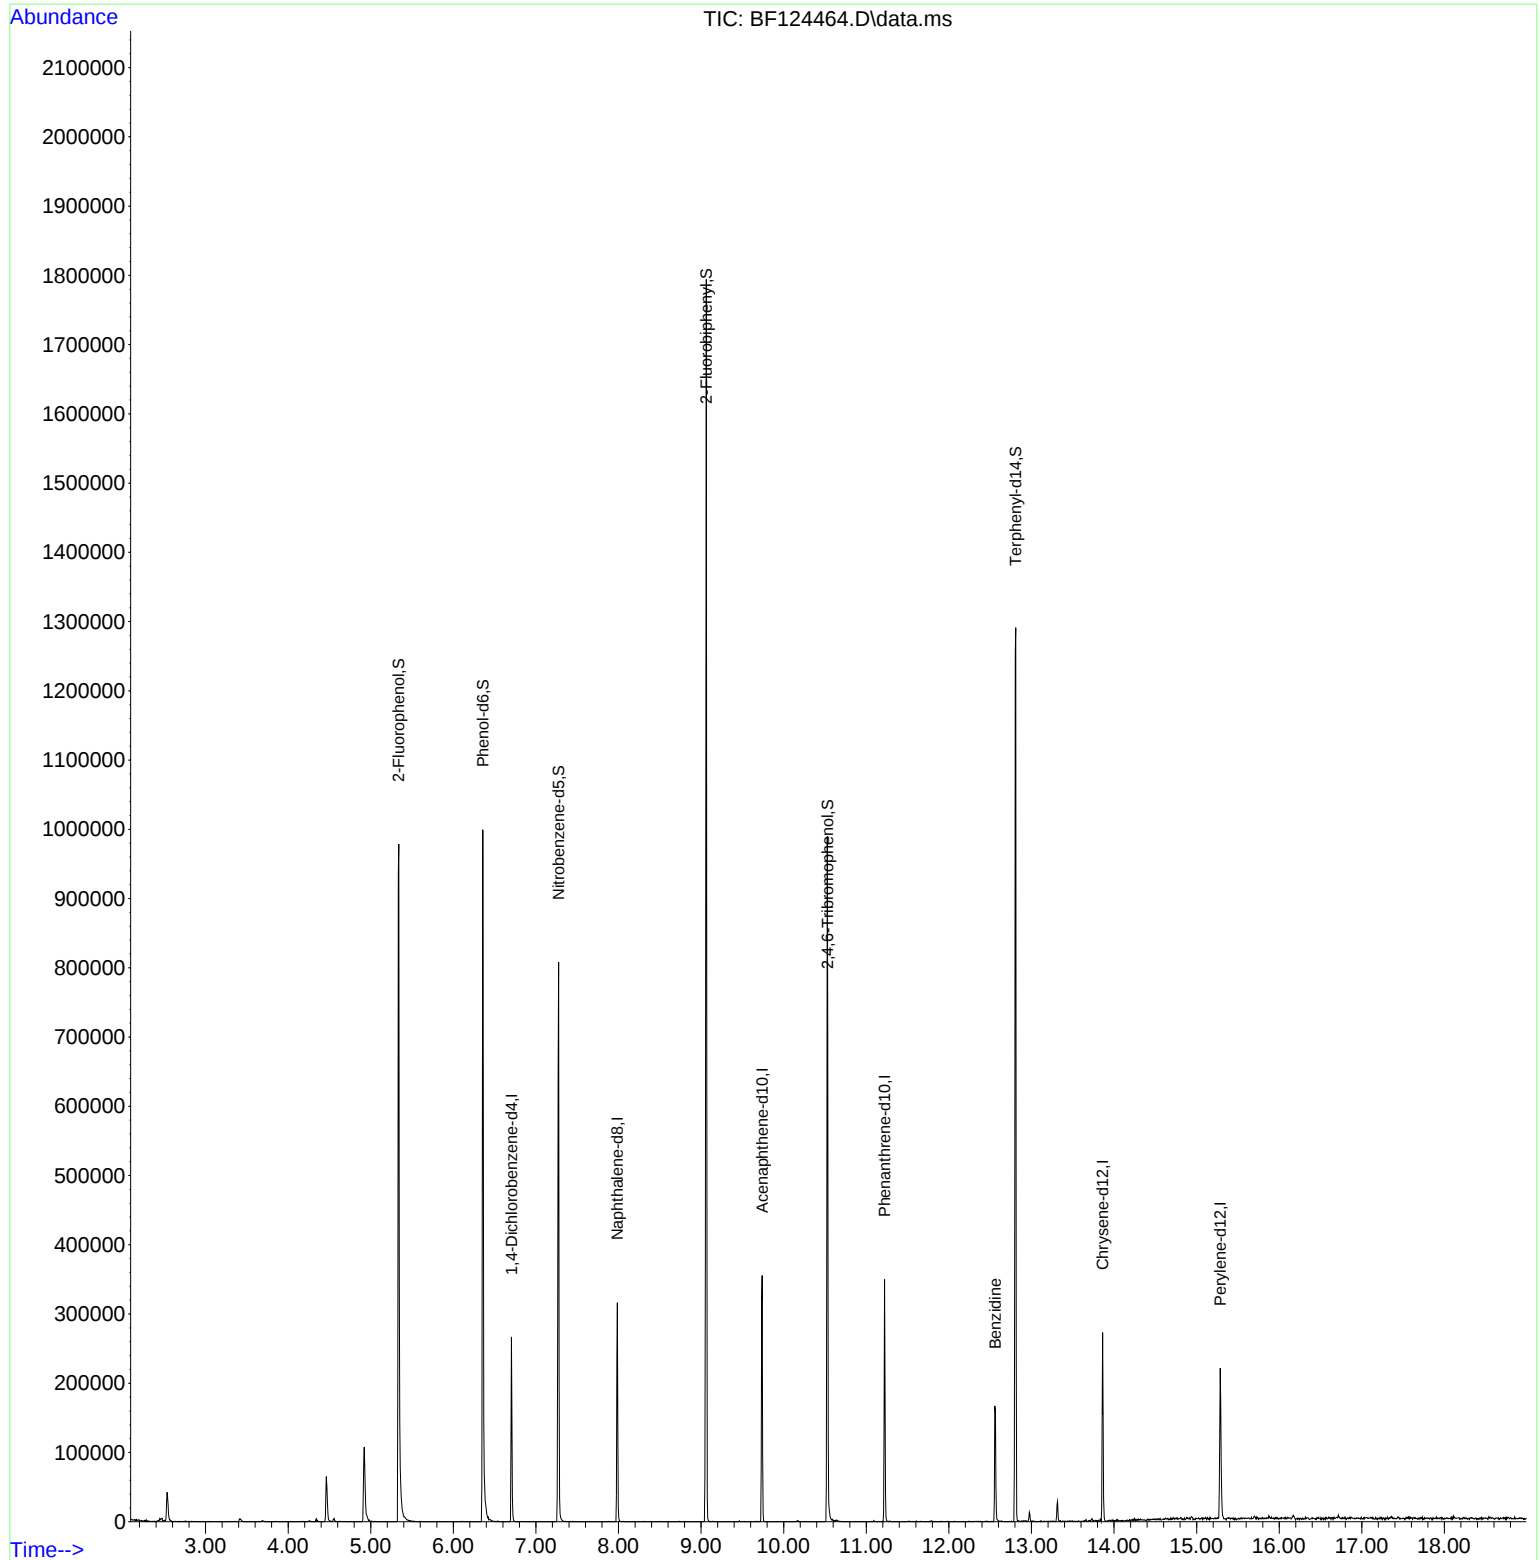


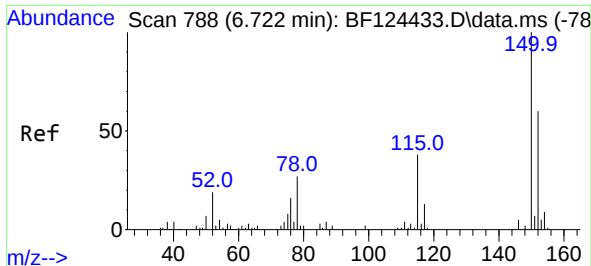

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.704 min Scan# 785
Delta R.T. 0.000 min
Lab File: BF124464.D
Acq: 25 Jun 2021 21:55




Instrument :
BNA_F
ClientSampleId :
15B-DUP-01

Tgt Ion:152 Resp: 32981
Ion Ratio Lower Upper
152 100
150 159.4 127.0 190.6
115 68.3 54.3 81.5

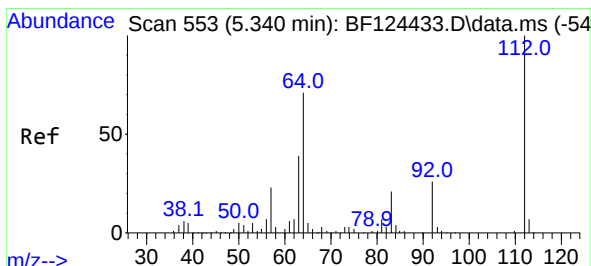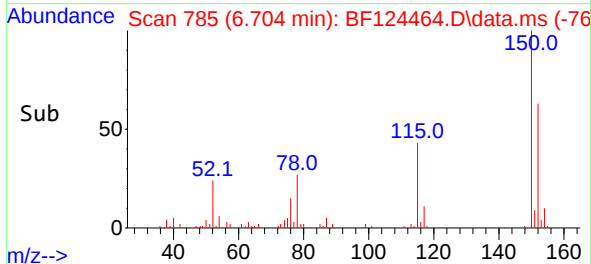
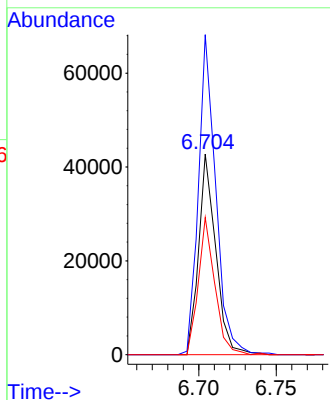
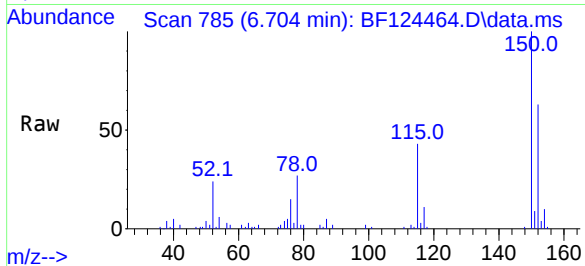


#5
2-Fluorophenol
Concen: 125.079 ng
RT: 5.340 min Scan# 553
Delta R.T. 0.012 min
Lab File: BF124464.D
Acq: 25 Jun 2021 21:55

Tgt Ion:112 Resp: 262305
Ion Ratio Lower Upper
112 100
64 64.5 61.4 92.0
63 37.0 33.0 49.4

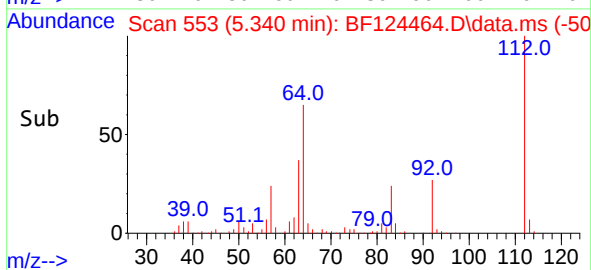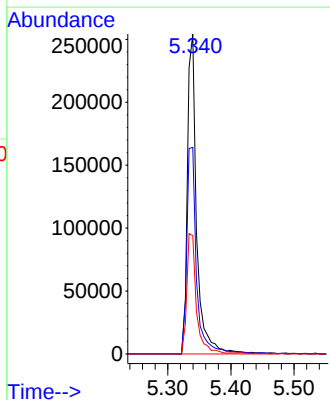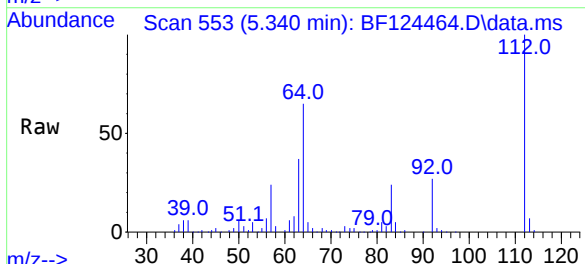

Abundance Scan 729 (6.375 min): BF124433.D\data.ms (-72

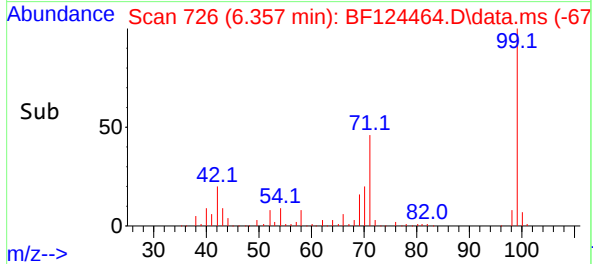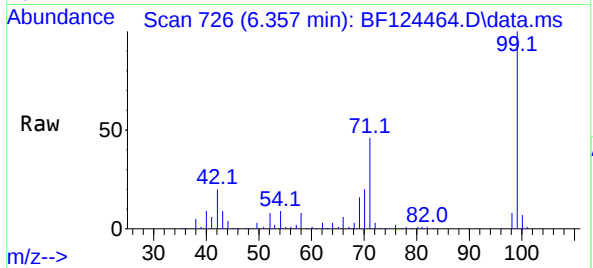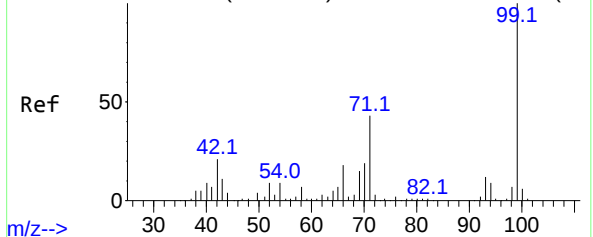

#7

Phenol-d6

Concen: 103.977 ng

RT: 6.357 min Scan# 726





Delta R.T. -0.006 min

Lab File: BF124464.D

Acq: 25 Jun 2021 21:55

Tgt Ion: 99 Resp: 284707

Ion	Ratio	Lower	Upper
99	100		
42	20.3	19.8	29.8
71	46.4	31.1	46.7

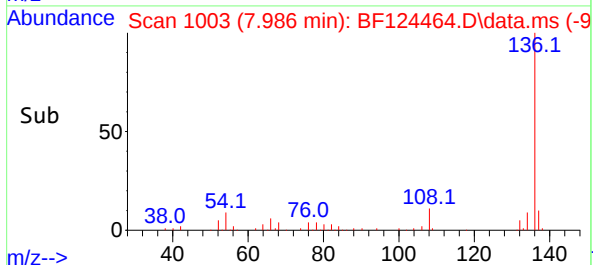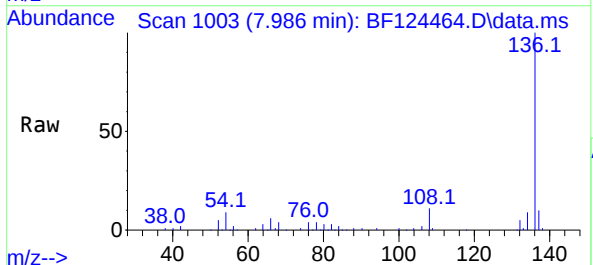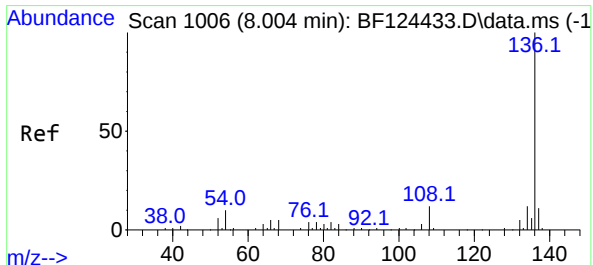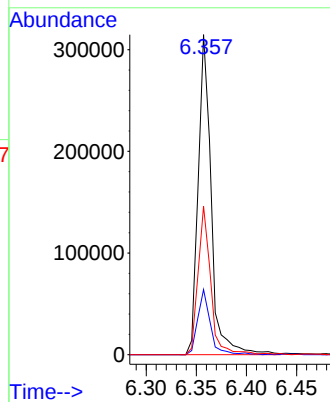

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.986 min Scan# 1003


Delta R.T. 0.000 min

Lab File: BF124464.D

Acq: 25 Jun 2021 21:55

Tgt Ion: 136 Resp: 128596

Ion	Ratio	Lower	Upper
136	100		
137	9.9	8.7	13.1
54	8.8	9.8	14.6#
68	3.9	4.1	6.1#

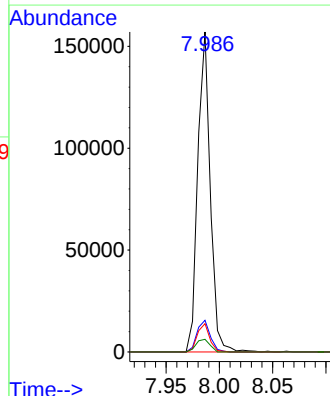


Instrument :

BNA_F

ClientSampleId :





15B-DUP-01

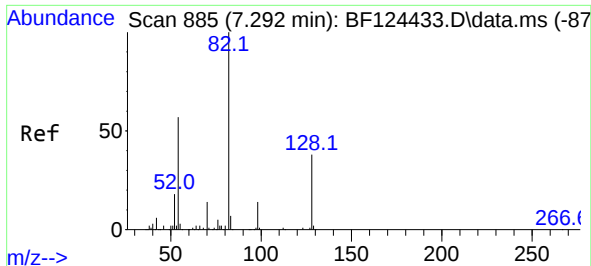

#23
Nitrobenzene-d5
Concen: 79.603 ng
RT: 7.275 min Scan# 882
Delta R.T. -0.006 min
Lab File: BF124464.D
Acq: 25 Jun 2021 21:55




Instrument :
BNA_F
ClientSampleId :
15B-DUP-01


Tgt Ion: 82 Resp: 246889
Ion Ratio Lower Upper
82 100
128 40.8 29.4 44.2
54 54.8 54.1 81.1

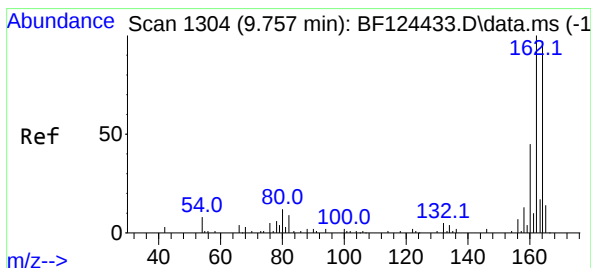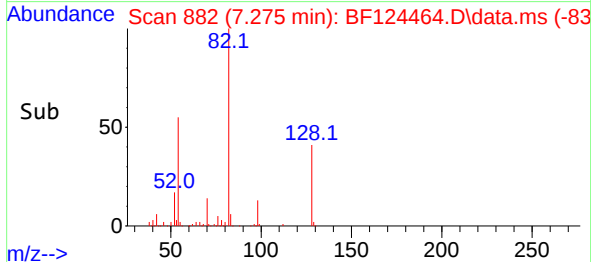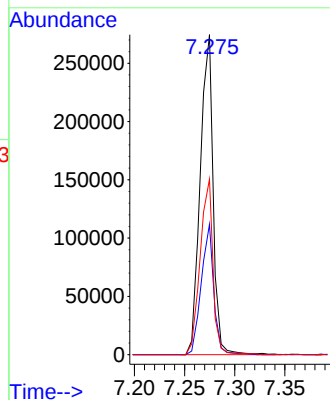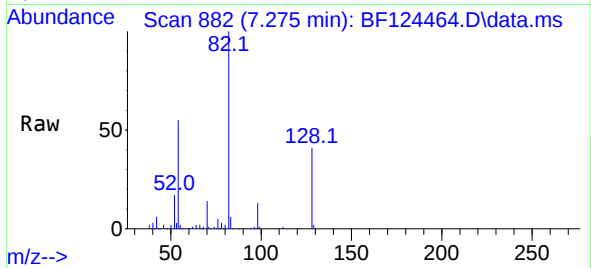

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.739 min Scan# 1301
Delta R.T. 0.000 min
Lab File: BF124464.D
Acq: 25 Jun 2021 21:55

Tgt Ion: 164 Resp: 69314
Ion Ratio Lower Upper
164 100
162 110.2 80.7 121.1
160 40.0 37.3 55.9


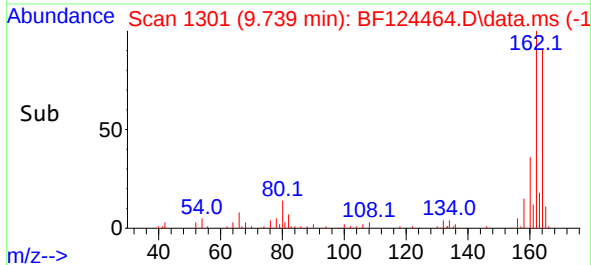
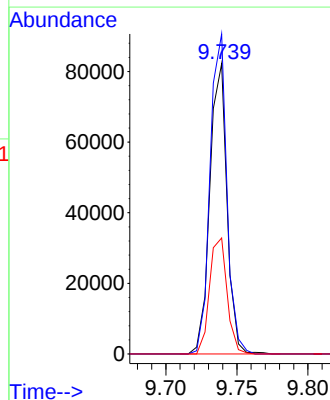
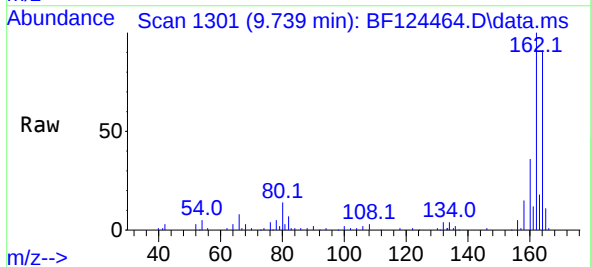


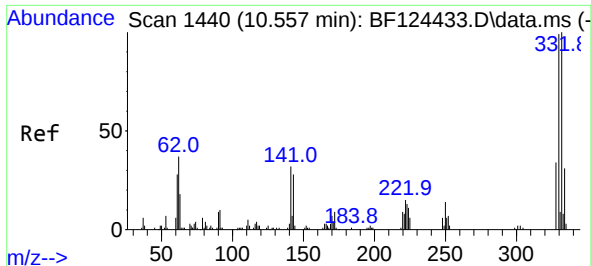

#42
2,4,6-Tribromophenol
Concen: 123.838 ng
RT: 10.533 min Scan# 1436
Delta R.T. 0.000 min
Lab File: BF124464.D
Acq: 25 Jun 2021 21:55




Instrument :
BNA_F
ClientSampleId :
15B-DUP-01


Tgt Ion:330 Resp: 102553
Ion Ratio Lower Upper
330 100
332 95.2 77.1 115.7
141 36.7 27.9 41.9

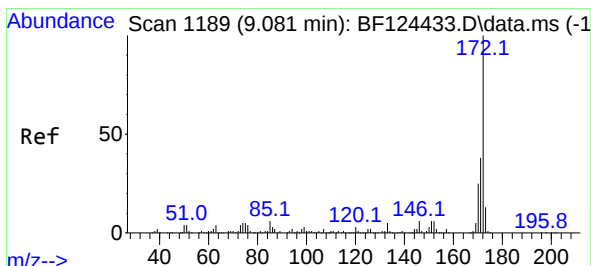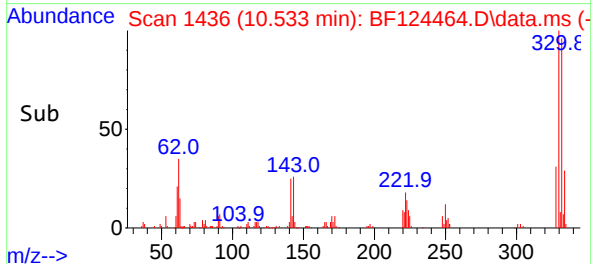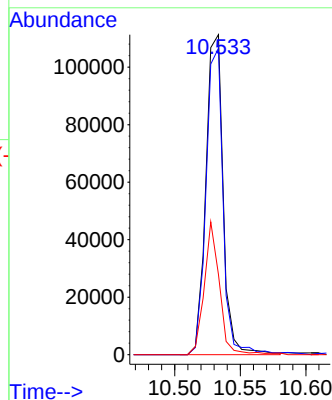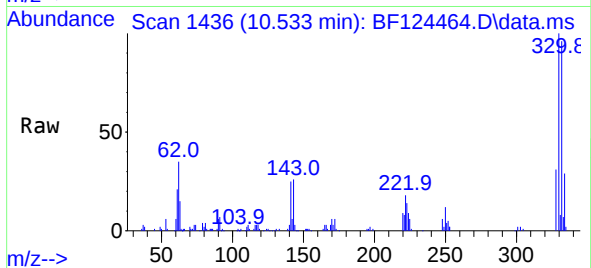

#45
2-Fluorobiphenyl
Concen: 83.954 ng
RT: 9.063 min Scan# 1186
Delta R.T. -0.006 min
Lab File: BF124464.D
Acq: 25 Jun 2021 21:55

Tgt Ion:172 Resp: 475039
Ion Ratio Lower Upper
172 100
171 38.2 28.1 42.1
170 24.0 19.2 28.8


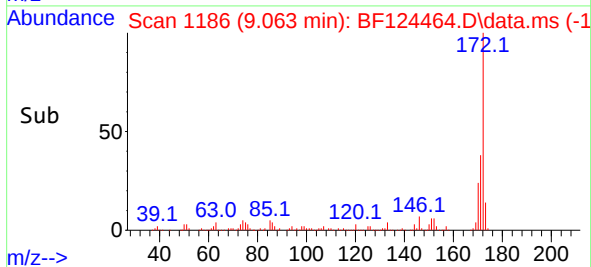
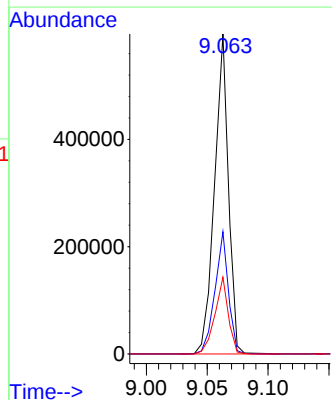
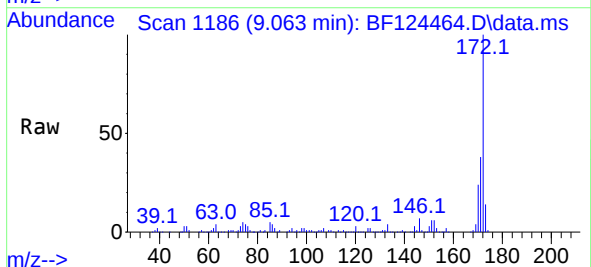


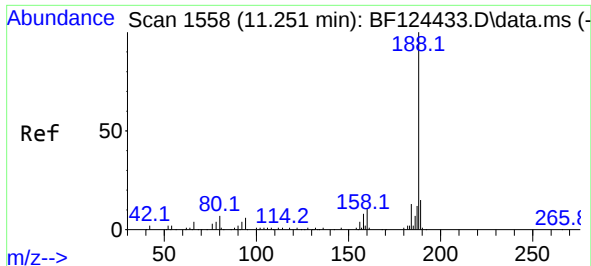

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.222 min Scan# 1553
Delta R.T. -0.006 min
Lab File: BF124464.D
Acq: 25 Jun 2021 21:55




Instrument :
BNA_F
ClientSampleId :
15B-DUP-01


Tgt Ion:188 Resp: 108878
Ion Ratio Lower Upper
188 100
94 7.8 6.9 10.3
80 9.7 8.2 12.2

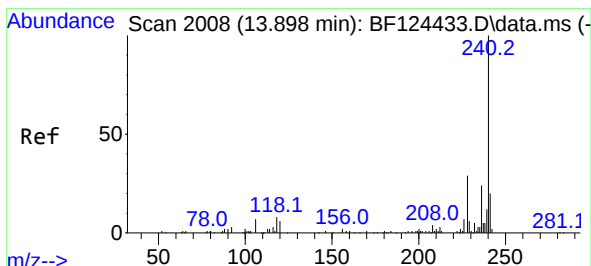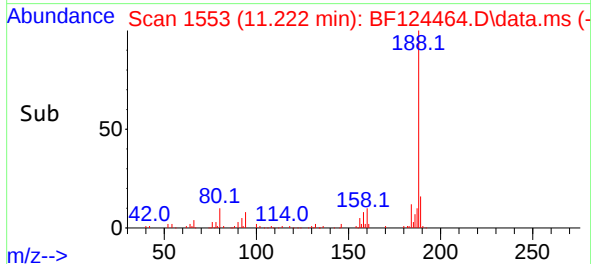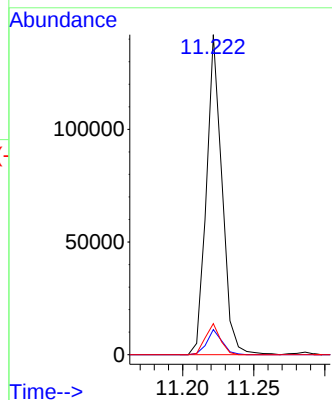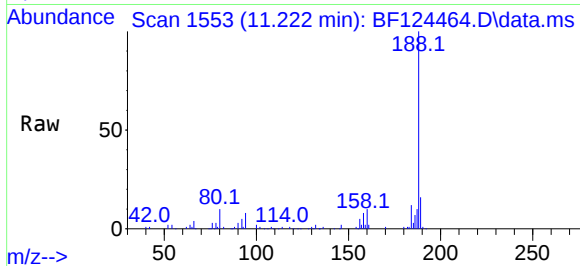

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.863 min Scan# 2002
Delta R.T. -0.006 min
Lab File: BF124464.D
Acq: 25 Jun 2021 21:55

Tgt Ion:240 Resp: 84445
Ion Ratio Lower Upper
240 100
120 7.4 7.2 10.8
236 24.5 19.0 28.4


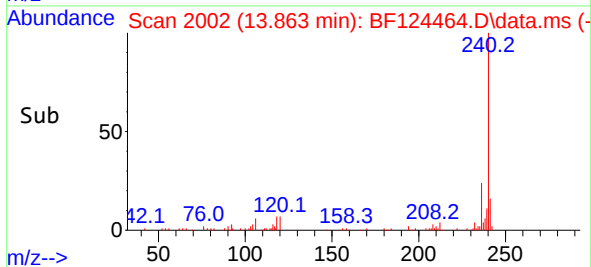
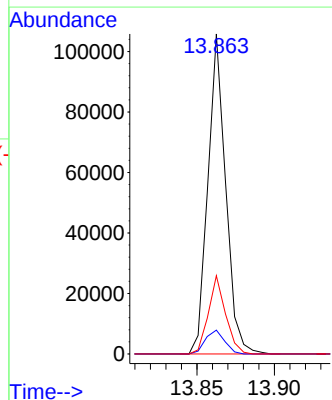
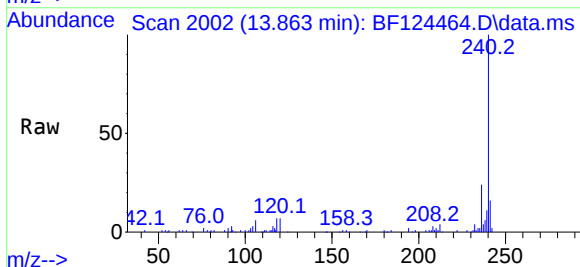


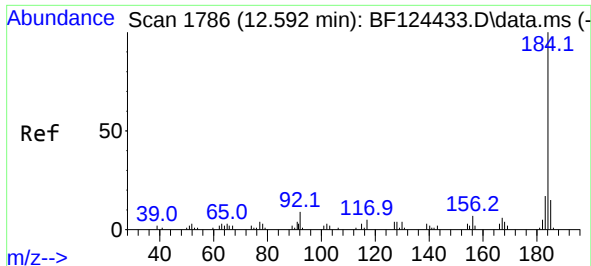

#77
Benzidine
Concen: 37.326 ng
RT: 12.563 min Scan# 1781
Delta R.T. 0.000 min
Lab File: BF124464.D
Acq: 25 Jun 2021 21:55




Instrument :
BNA_F
ClientSampleId :
15B-DUP-01


Tgt Ion:184 Resp: 63170
Ion Ratio Lower Upper
184 100
185 12.0 12.1 18.1#
183 14.0 7.8 11.8#

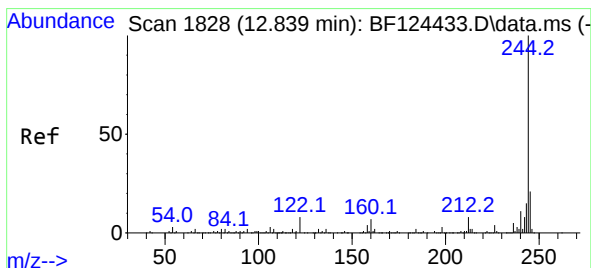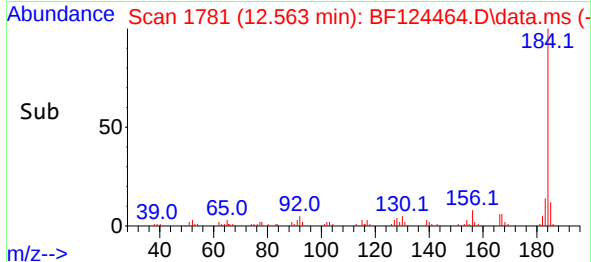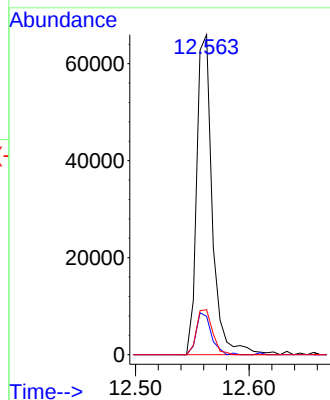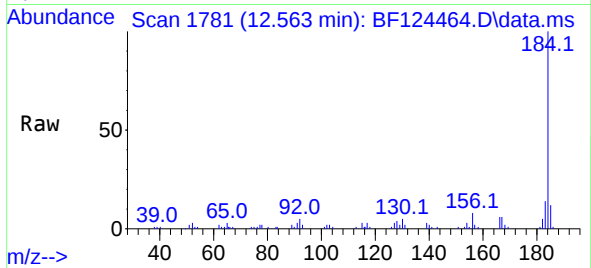

#79
Terphenyl-d14
Concen: 74.370 ng
RT: 12.810 min Scan# 1823
Delta R.T. 0.000 min
Lab File: BF124464.D
Acq: 25 Jun 2021 21:55

Tgt Ion:244 Resp: 419298
Ion Ratio Lower Upper
244 100
212 6.9 5.7 8.5
122 7.7 9.7 14.5#

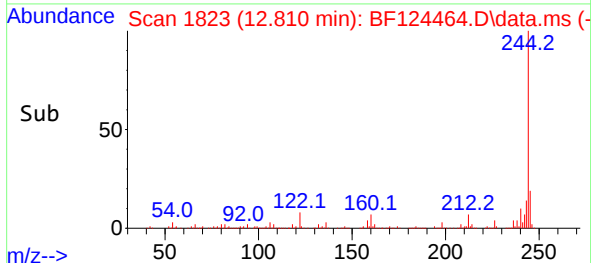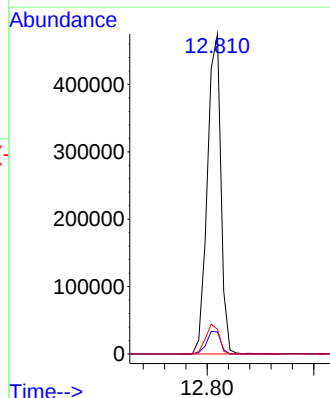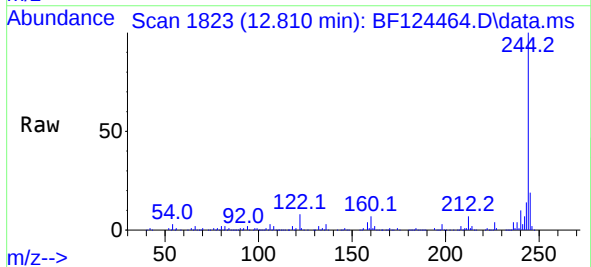

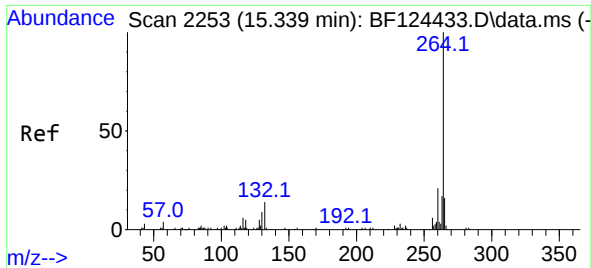

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.286 min Scan# 2244
 Delta R.T. -0.006 min
 Lab File: BF124464.D
 Acq: 25 Jun 2021 21:55

Instrument :
 BNA_F
 ClientSampleId :
 15B-DUP-01

Tgt Ion:264 Resp: 86171

Ion	Ratio	Lower	Upper
264	100		
260	21.4	18.7	28.1
265	23.0	17.8	26.8

