

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
 Data File : BF124449.D
 Acq On : 25 Jun 2021 13:22
 Operator : JU/CG
 Sample : PB137242BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137242BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.946	483	486	496	rBB	13484	21860	1.14%	0.217%
2	5.340	549	553	563	rBV	1416833	1240371	64.41%	12.338%
3	6.357	722	726	729	rBV	1254438	1156384	60.04%	11.503%
4	6.704	782	785	792	rBB	296717	248878	12.92%	2.476%
5	7.269	877	881	885	rBV	778643	807004	41.90%	8.028%
6	7.987	999	1003	1011	rBB	356071	320785	16.66%	3.191%
7	9.063	1181	1186	1189	rBV	1925714	1661767	86.29%	16.530%
8	9.739	1296	1301	1305	rBV	446673	385947	20.04%	3.839%
9	10.533	1431	1436	1439	rBV	1180121	1096256	56.92%	10.905%
10	11.222	1550	1553	1562	rBB	488724	416364	21.62%	4.142%
11	12.810	1819	1823	1826	rBV	2143455	1925888	100.00%	19.157%
12	13.863	1999	2002	2007	rVB	439322	353969	18.38%	3.521%
13	15.286	2240	2244	2251	rBV	255231	317541	16.49%	3.159%
14	15.698	2308	2314	2320	rVB4	16945	27705	1.44%	0.276%
15	16.168	2389	2394	2398	rBV4	14415	21116	1.10%	0.210%
16	16.239	2398	2406	2407	rBV6	19491	30075	1.56%	0.299%
17	16.715	2481	2487	2492	rVB5	10402	21082	1.09%	0.210%


Sum of corrected areas: 10052992

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124449.D
Acq On : 25 Jun 2021 13:22
Operator : JU/CG
Sample : PB137242BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137242BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

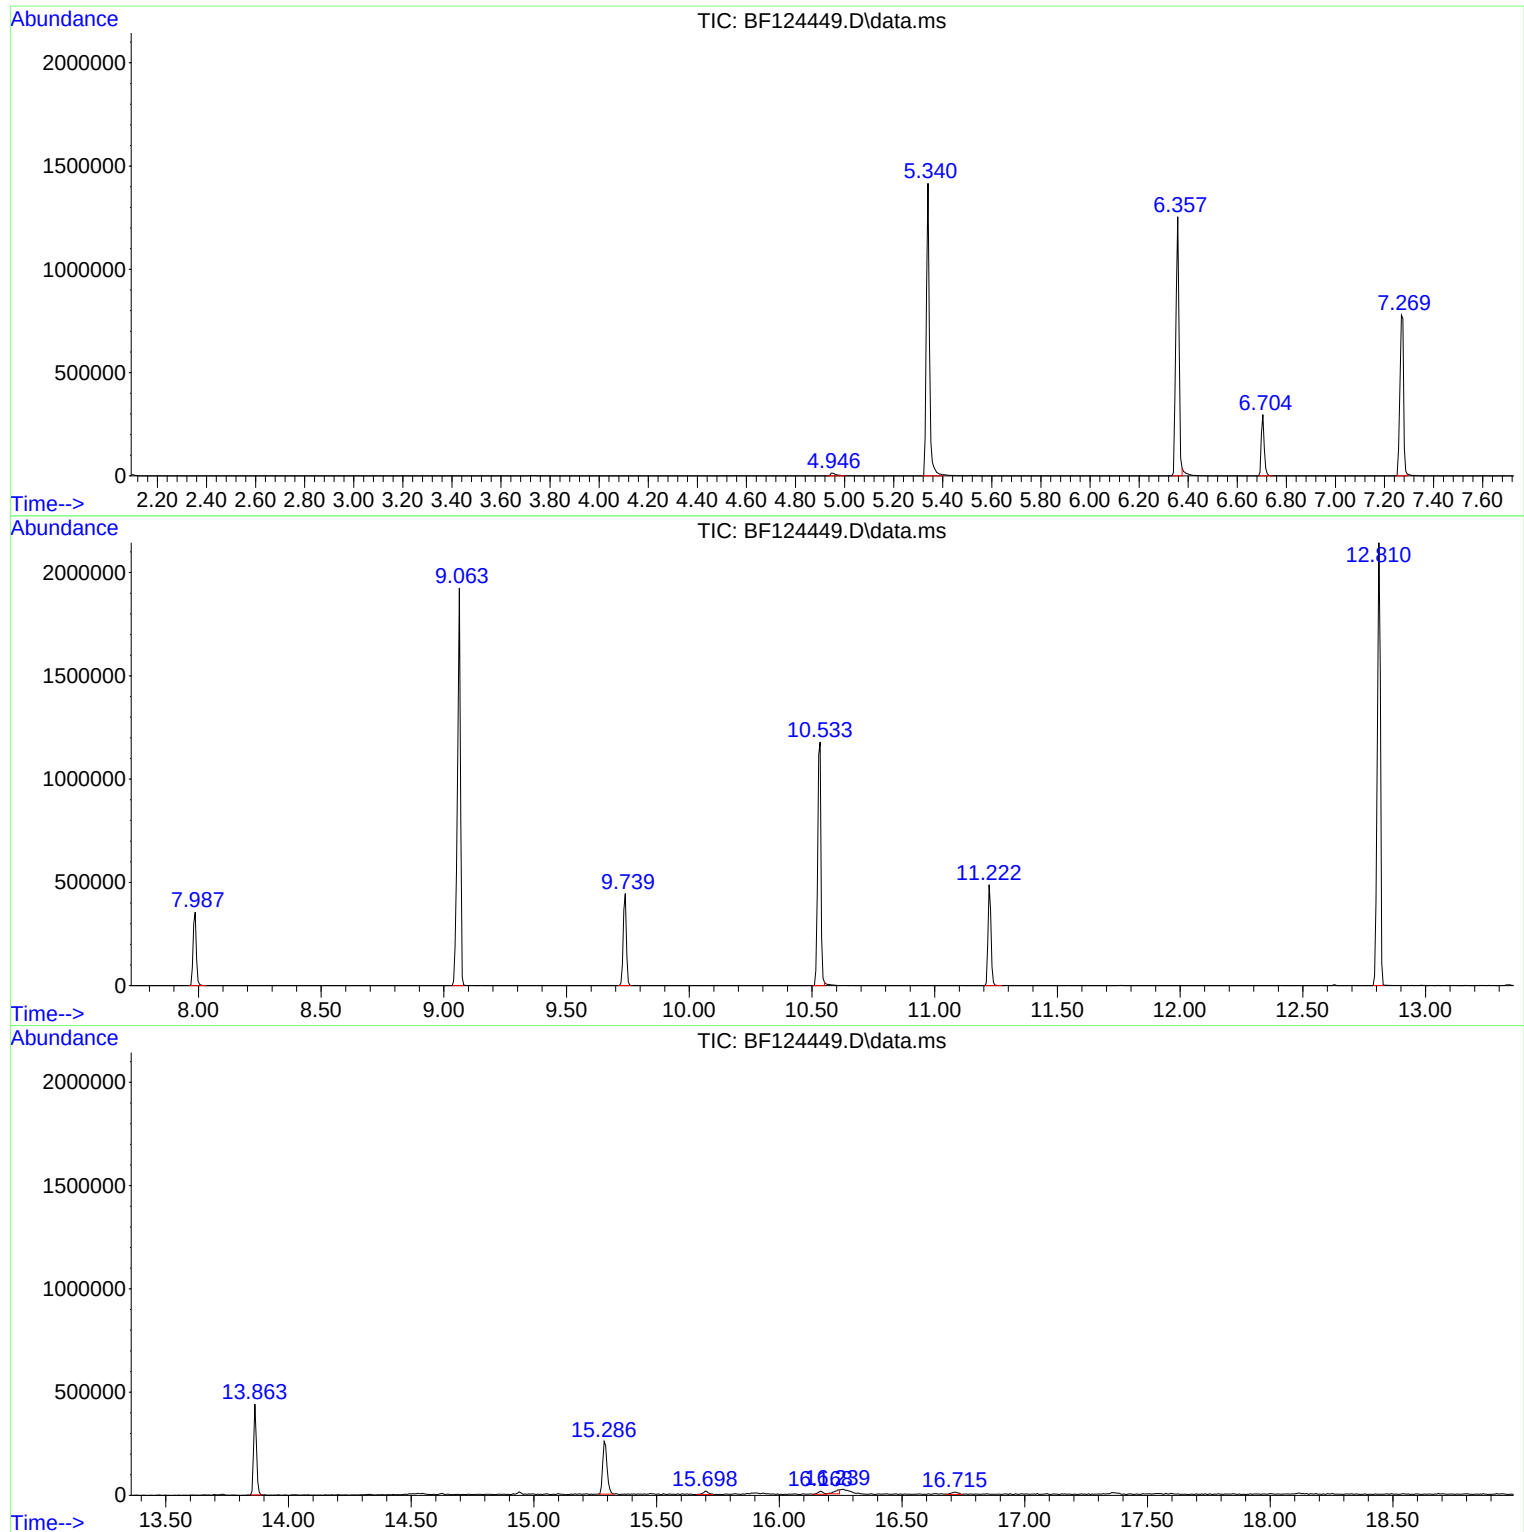

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124449.D
Acq On : 25 Jun 2021 13:22
Operator : JU/CG
Sample : PB137242BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137242BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124449.D
Acq On : 25 Jun 2021 13:22
Operator : JU/CG
Sample : PB137242BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137242BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------