

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
 Data File : BF124460.D
 Acq On : 25 Jun 2021 19:44
 Operator : JU/CG
 Sample : M2829-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 15B-STOCKPILE-2A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.116	3	5	7	rVB	2818745	1964596	100.00%	16.453%
2	2.563	78	81	89	rVB2	40089	54021	2.75%	0.452%
3	4.469	402	405	412	rBV	67726	75893	3.86%	0.636%
4	4.922	478	482	495	rBV3	158837	249224	12.69%	2.087%
5	5.340	550	553	564	rBV	1171422	1107329	56.36%	9.274%
6	6.363	723	727	742	rBV	966868	1000217	50.91%	8.376%
7	6.704	782	785	791	rBB	288670	225422	11.47%	1.888%
8	7.275	878	882	885	rBV	924611	821217	41.80%	6.877%
9	7.987	999	1003	1009	rVB	336222	289635	14.74%	2.426%
10	9.063	1181	1186	1189	rBV	2132077	1763895	89.78%	14.772%
11	9.739	1297	1301	1304	rBV	430818	374269	19.05%	3.134%
12	10.533	1431	1436	1439	rBV	1337737	1215076	61.85%	10.176%
13	11.222	1550	1553	1557	rBV	496804	385422	19.62%	3.228%
14	12.810	1818	1823	1826	rBV	2083531	1866970	95.03%	15.635%
15	13.863	1999	2002	2006	rBV	333508	274914	13.99%	2.302%
16	15.286	2240	2244	2254	rBV	220337	272678	13.88%	2.284%




Sum of corrected areas: 11940778

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124460.D
Acq On : 25 Jun 2021 19:44
Operator : JU/CG
Sample : M2829-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
15B-STOCKPILE-2A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

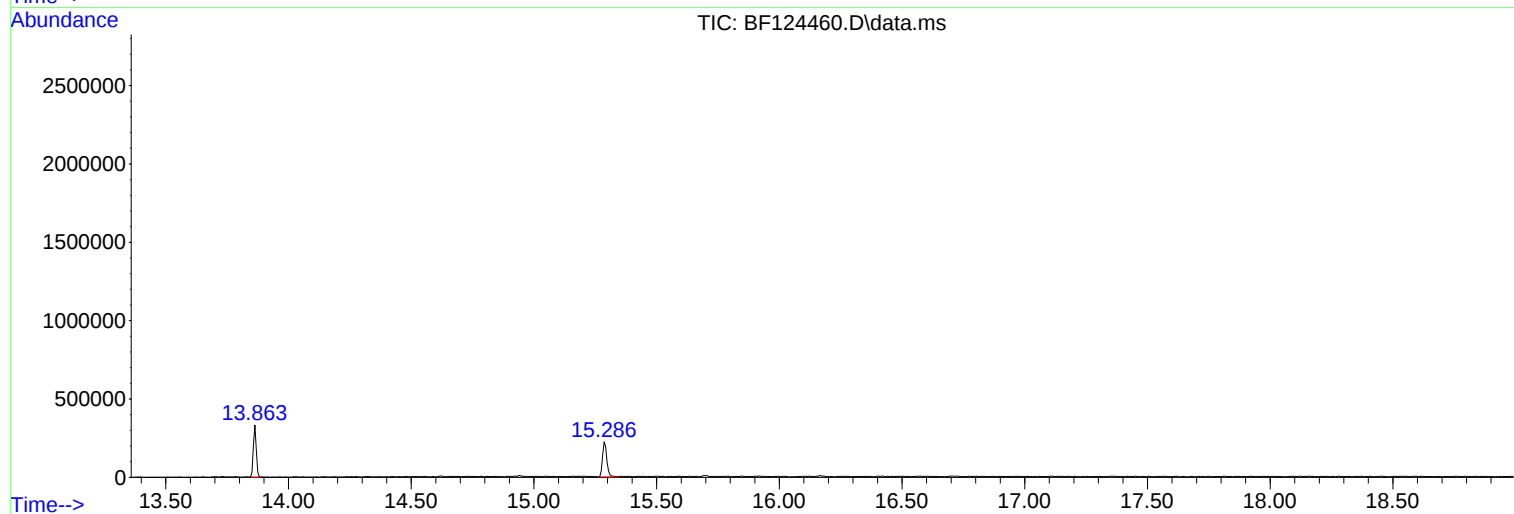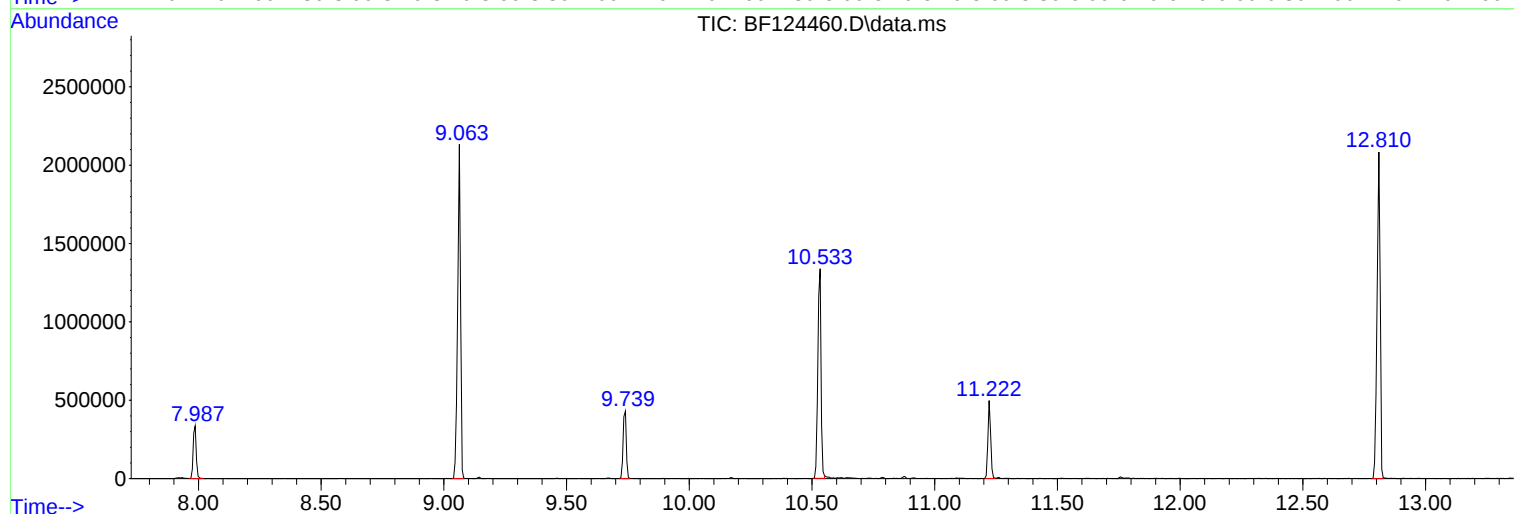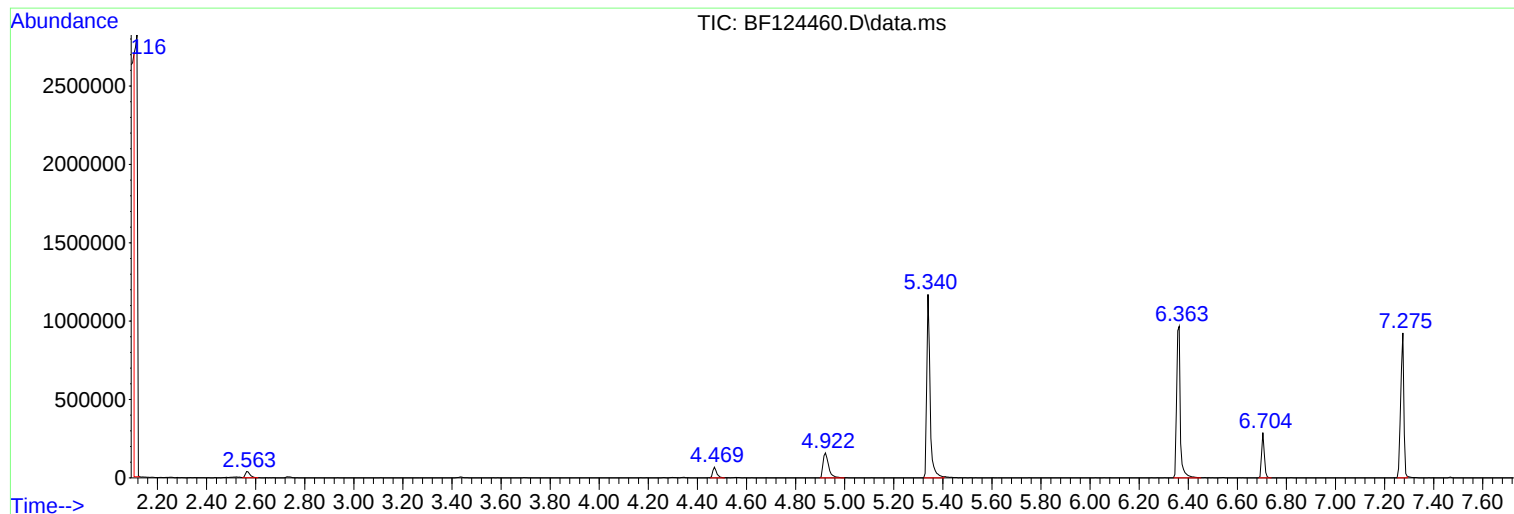

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124460.D
Acq On : 25 Jun 2021 19:44
Operator : JU/CG
Sample : M2829-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
15B-STOCKPILE-2A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124460.D
Acq On : 25 Jun 2021 19:44
Operator : JU/CG
Sample : M2829-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
15B-STOCKPILE-2A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------