

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
 Data File : BF124464.D
 Acq On : 25 Jun 2021 21:55
 Operator : JU/CG
 Sample : M2829-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 15B-DUP-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124464.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.534	72	76	86	rVB	42694	60396	4.26%	0.745%
2	4.463	401	404	412	rBV	65311	74265	5.24%	0.917%
3	4.922	478	482	491	rBV2	107670	153880	10.85%	1.899%
4	5.340	550	553	573	rBV	978133	1032713	72.84%	12.746%
5	6.357	723	726	738	rBV	999432	915324	64.56%	11.297%
6	6.704	782	785	793	rBB	266940	207388	14.63%	2.560%
7	7.275	878	882	892	rBV	808433	724404	51.10%	8.941%
8	7.986	1000	1003	1008	rBV	316310	263720	18.60%	3.255%
9	9.063	1181	1186	1189	rBV	1794127	1417716	100.00%	17.498%
10	9.739	1297	1301	1304	rBV	355754	304532	21.48%	3.759%
11	10.527	1432	1435	1445	rBV	989275	836557	59.01%	10.325%
12	11.222	1550	1553	1559	rBV	349890	268006	18.90%	3.308%
13	12.557	1777	1780	1792	rBV	167356	155593	10.97%	1.920%
14	12.810	1818	1823	1826	rBV	1290808	1187369	83.75%	14.655%
15	13.316	1905	1909	1912	rBV	29098	28628	2.02%	0.353%
16	13.863	1999	2002	2008	rVB	272757	226103	15.95%	2.791%
17	15.286	2240	2244	2252	rVB	217642	245587	17.32%	3.031%




Sum of corrected areas: 8102181

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124464.D
Acq On : 25 Jun 2021 21:55
Operator : JU/CG
Sample : M2829-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
15B-DUP-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

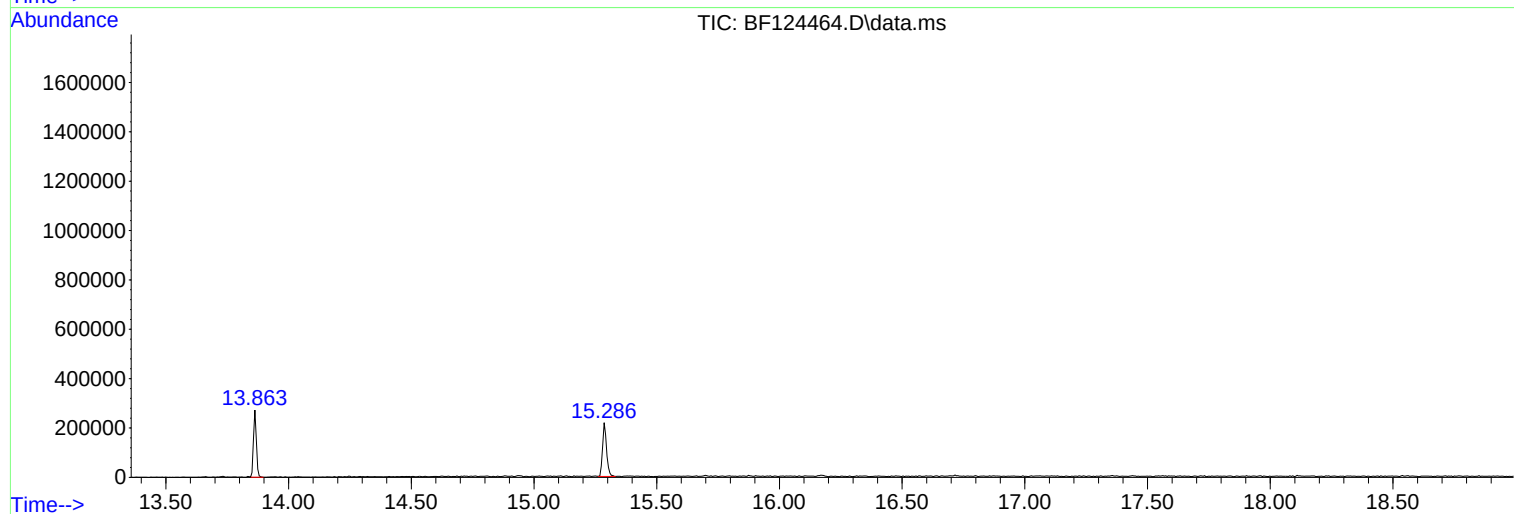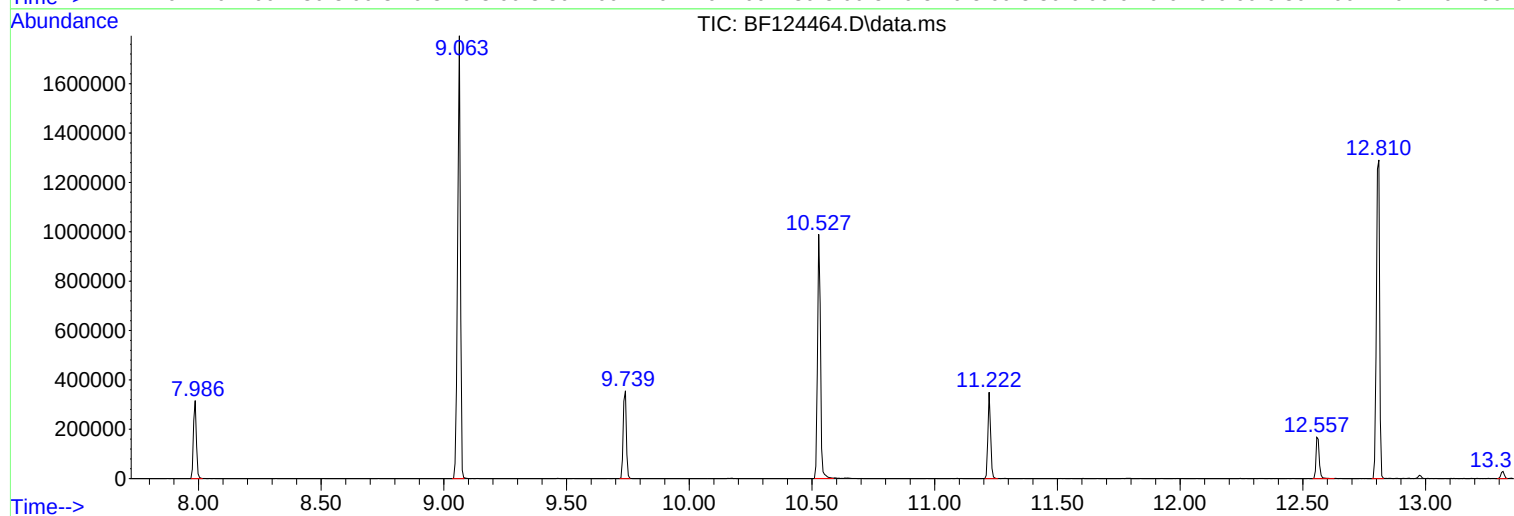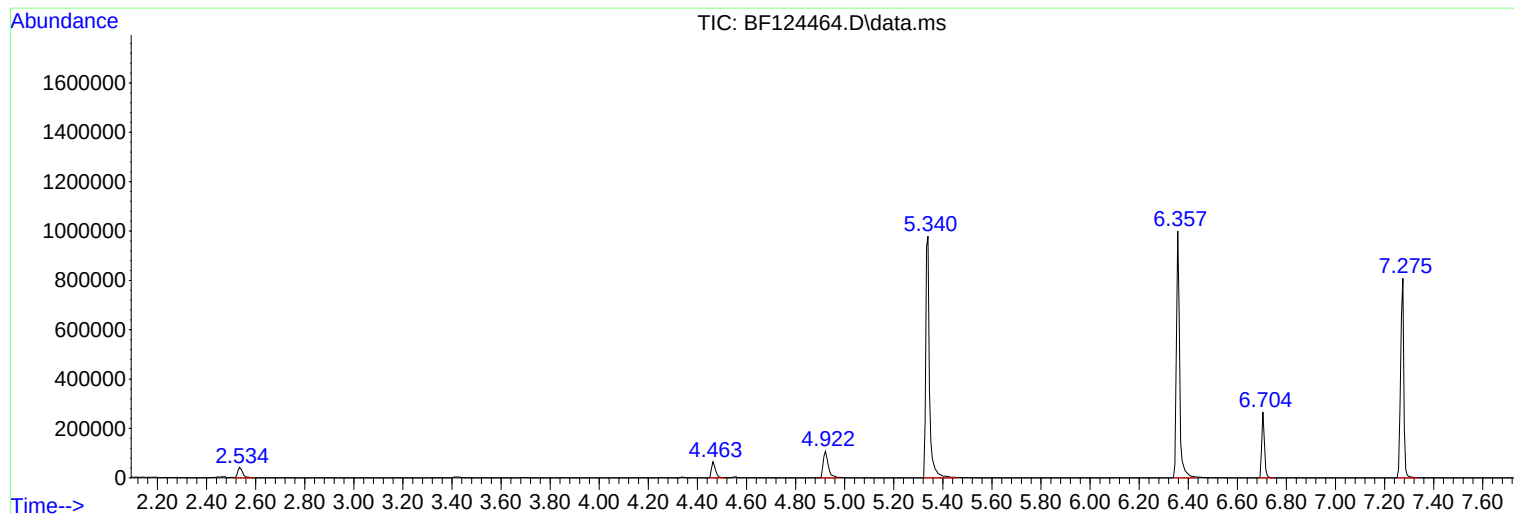

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124464.D
Acq On : 25 Jun 2021 21:55
Operator : JU/CG
Sample : M2829-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
15B-DUP-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124464.D
Acq On : 25 Jun 2021 21:55
Operator : JU/CG
Sample : M2829-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
15B-DUP-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------