

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
 Data File : BF124465.D
 Acq On : 25 Jun 2021 22:28
 Operator : JU/CG
 Sample : M2860-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ASH

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124465.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.563	78	81	89	rVB	50036	71619	5.22%	0.901%
2	4.469	401	405	413	rVB	95880	101360	7.39%	1.275%
3	4.922	478	482	491	rBV2	126099	203372	14.83%	2.558%
4	5.340	550	553	570	rBV	1081965	1012556	73.86%	12.735%
5	6.357	723	726	738	rBV	908389	881829	64.32%	11.091%
6	6.704	782	785	792	rBV	257127	190863	13.92%	2.400%
7	7.275	878	882	885	rBV	783435	701086	51.14%	8.818%
8	7.987	999	1003	1008	rBV	298604	245623	17.92%	3.089%
9	9.063	1181	1186	1189	rBV	1763374	1371004	100.00%	17.243%
10	9.734	1297	1300	1304	rBV	329325	289548	21.12%	3.642%
11	10.528	1431	1435	1447	rBV	994126	864309	63.04%	10.870%
12	11.222	1550	1553	1561	rBB	341365	272856	19.90%	3.432%
13	12.563	1778	1781	1788	rBV	57256	53563	3.91%	0.674%
14	12.810	1818	1823	1826	rBV	1362843	1230854	89.78%	15.481%
15	13.863	1998	2002	2007	rVB	252357	227177	16.57%	2.857%
16	15.286	2240	2244	2250	rBV	208831	233372	17.02%	2.935%




Sum of corrected areas: 7950991

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124465.D
Acq On : 25 Jun 2021 22:28
Operator : JU/CG
Sample : M2860-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ASH

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

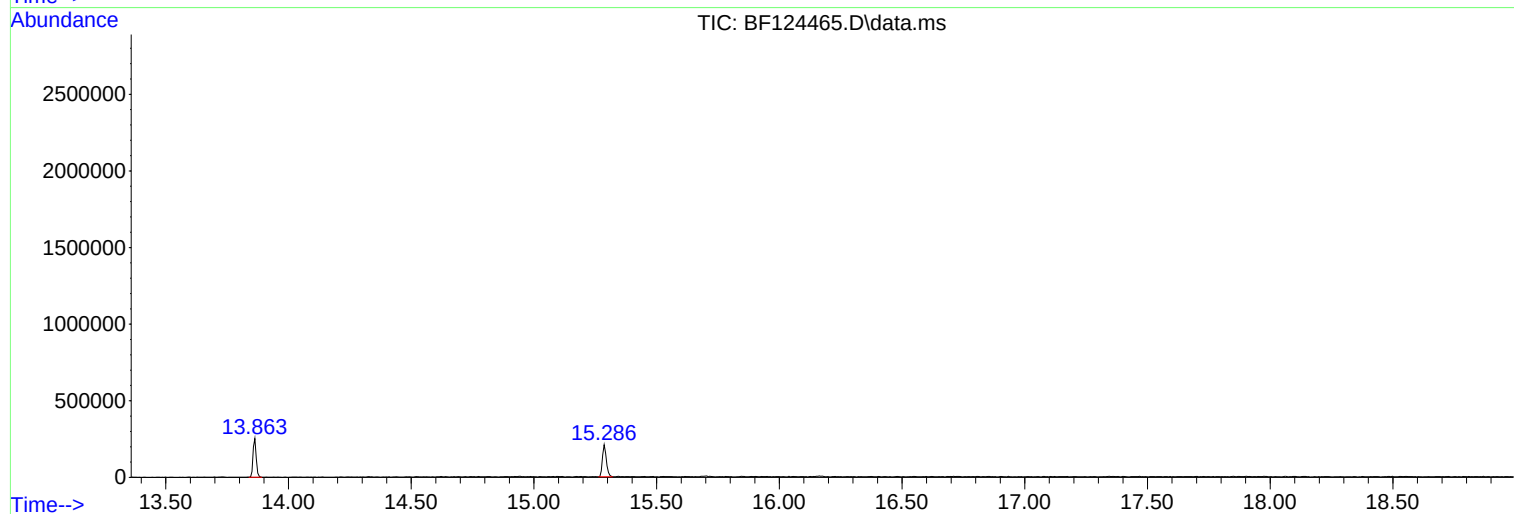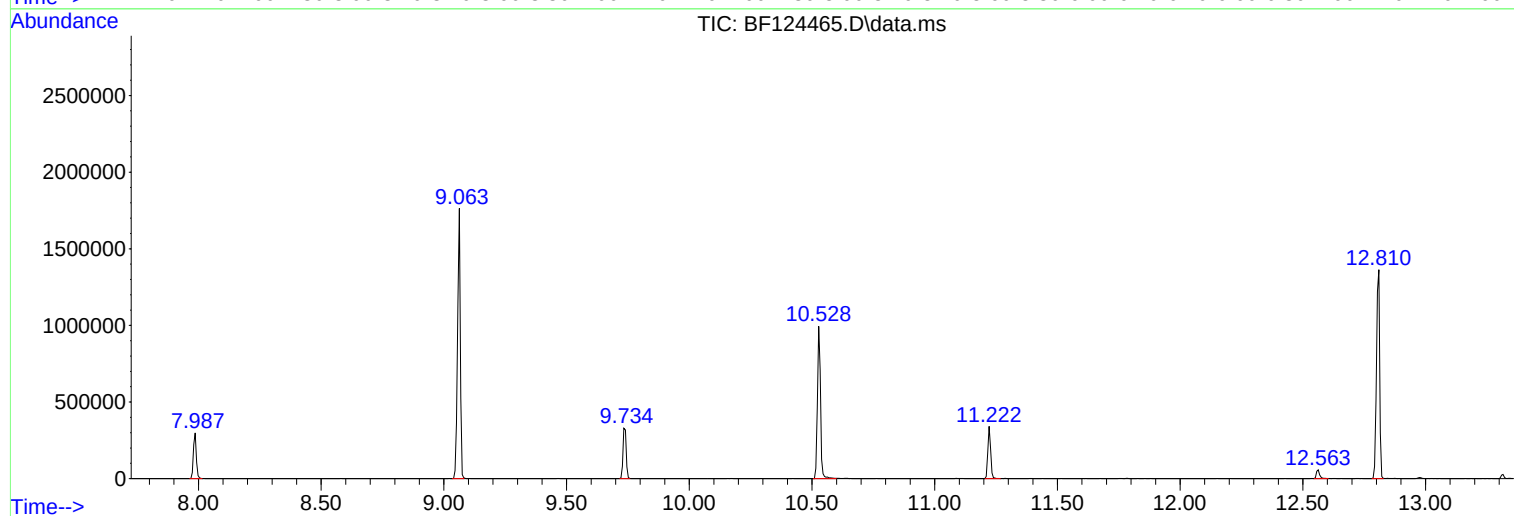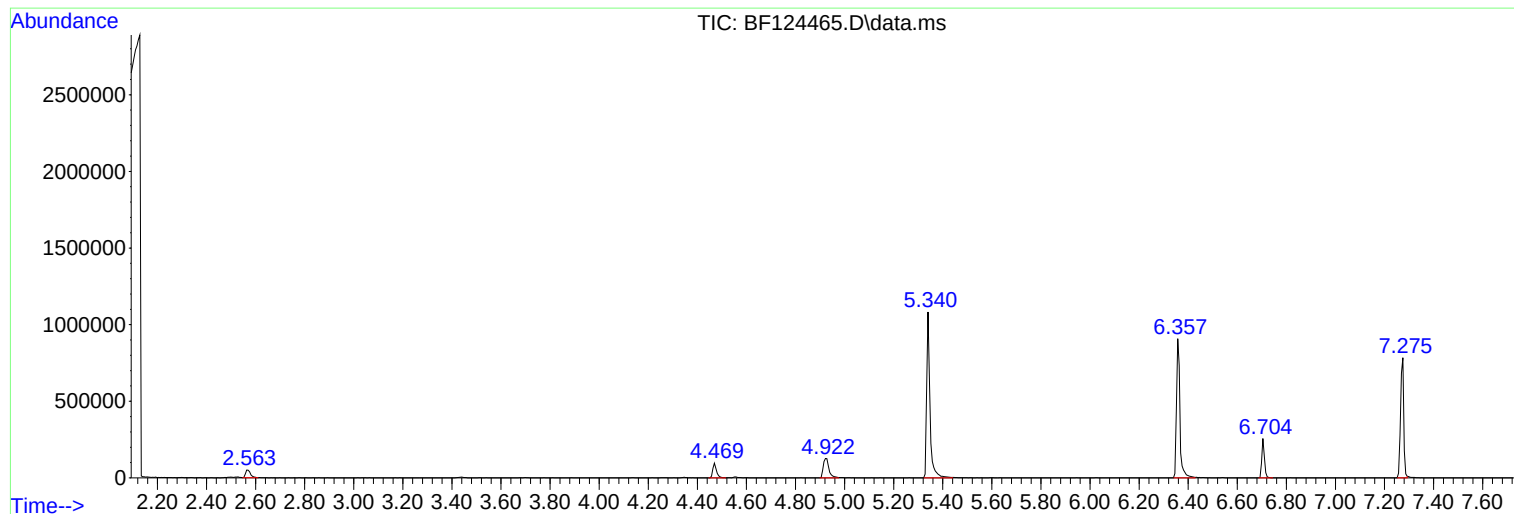

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124465.D
Acq On : 25 Jun 2021 22:28
Operator : JU/CG
Sample : M2860-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ASH

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124465.D
Acq On : 25 Jun 2021 22:28
Operator : JU/CG
Sample : M2860-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ASH

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------