

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
 Data File : BF124466.D
 Acq On : 25 Jun 2021 23:00
 Operator : JU/CG
 Sample : M2826-02 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LS-1(LIQUID-BLUE)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124466.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.669	82	99	103	rBV	3445498	10640643	100.00%	40.771%
2	3.157	167	182	183	rBV	72249	262811	2.47%	1.007%
3	4.010	323	327	331	rVB2	216788	288195	2.71%	1.104%
4	4.963	483	489	494	rVB	424605	735188	6.91%	2.817%
5	5.410	561	565	579	rVB3	69810	188089	1.77%	0.721%
6	5.528	581	585	589	rBV2	76783	107347	1.01%	0.411%
7	5.851	637	640	643	rBV	124294	111197	1.05%	0.426%
8	6.016	664	668	673	rBV	116776	108967	1.02%	0.418%
9	6.251	704	708	714	rVB	215740	244967	2.30%	0.939%
10	6.551	754	759	761	rBV	623581	584564	5.49%	2.240%
11	6.704	782	785	789	rVB	254830	194833	1.83%	0.747%
12	7.269	879	881	885	rBV	142106	118042	1.11%	0.452%
13	7.987	998	1003	1006	rVB	300466	244819	2.30%	0.938%
14	9.063	1181	1186	1189	rBV	264252	245549	2.31%	0.941%
15	9.145	1195	1200	1202	rBV2	112963	140492	1.32%	0.538%
16	9.604	1275	1278	1280	rBV4	88280	118396	1.11%	0.454%
17	9.645	1283	1285	1288	rVB3	168560	139353	1.31%	0.534%
18	9.675	1288	1290	1294	rBV	212602	204026	1.92%	0.782%
19	9.716	1294	1297	1299	rBV3	135391	164346	1.54%	0.630%
20	9.739	1299	1301	1305	rVB	301712	242987	2.28%	0.931%
21	9.998	1343	1345	1348	rBV2	131670	140854	1.32%	0.540%
22	10.104	1361	1363	1367	rBV5	98960	132769	1.25%	0.509%
23	10.145	1367	1370	1372	rBV2	245768	200850	1.89%	0.770%
24	10.181	1373	1376	1378	rBV	329907	295011	2.77%	1.130%
25	10.398	1411	1413	1417	rVB	178111	170040	1.60%	0.652%
26	10.657	1454	1457	1458	rBV	438830	495485	4.66%	1.899%
27	11.104	1531	1533	1535	rBV	396355	322562	3.03%	1.236%
28	11.133	1536	1538	1542	rVB2	290149	255648	2.40%	0.980%
29	11.233	1552	1555	1558	rBV	302984	321747	3.02%	1.233%
30	11.469	1593	1595	1596	rBV	264078	210214	1.98%	0.805%
31	11.798	1649	1651	1654	rVB	480068	354721	3.33%	1.359%
32	12.204	1717	1720	1725	rBV	1039394	1143714	10.75%	4.382%
33	12.575	1781	1783	1789	rVB	398056	378040	3.55%	1.449%
34	13.116	1872	1875	1883	rVB	856508	1148816	10.80%	4.402%
35	13.880	2003	2005	2009	rVB	292190	261528	2.46%	1.002%
36	14.021	2026	2029	2036	rBV	1102544	1357166	12.75%	5.200%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124466.D
Acq On : 25 Jun 2021 23:00
Operator : JU/CG
Sample : M2826-02 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-1(LIQUID-BLUE)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.298	2074	2076	2082	rVB	323672	353168	3.32%	1.353%
38	14.863	2168	2172	2180	rVB	1010406	1482446	13.93%	5.680%
39	15.239	2233	2236	2239	rVB5	130076	159564	1.50%	0.611%
40	15.304	2245	2247	2255	rVB	237919	322565	3.03%	1.236%
41	15.921	2346	2352	2362	rVB2	434418	1018572	9.57%	3.903%
42	16.333	2417	2422	2432	rBV9	104979	264561	2.49%	1.014%
43	17.527	2616	2625	2629	rBV10	73647	223594	2.10%	0.857%




Sum of corrected areas: 26098446

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124466.D
Acq On : 25 Jun 2021 23:00
Operator : JU/CG
Sample : M2826-02 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-1(LIQUID-BLUE)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

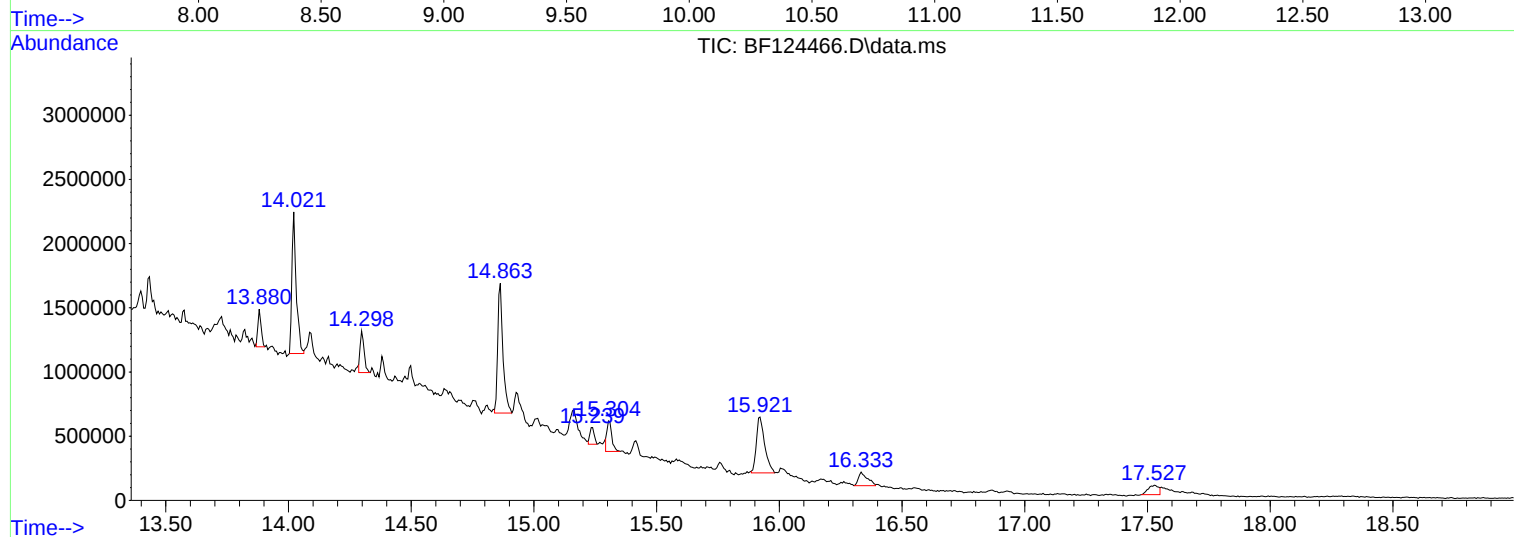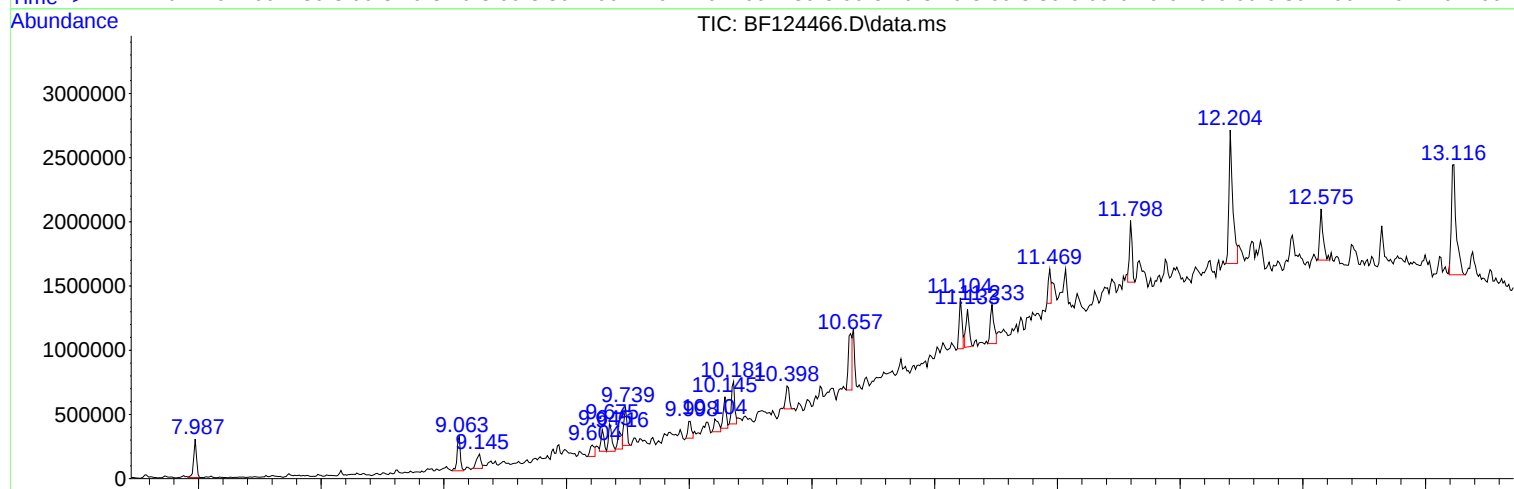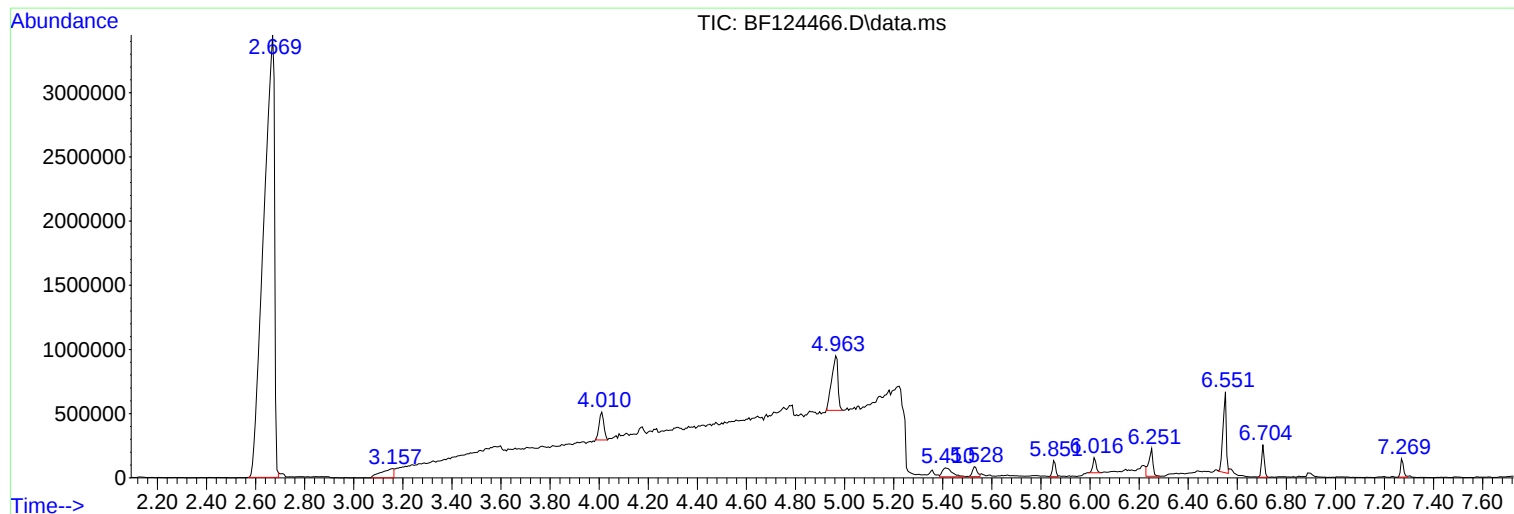

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124466.D
Acq On : 25 Jun 2021 23:00
Operator : JU/CG
Sample : M2826-02 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-1(LIQUID-BLUE)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124466.D
Acq On : 25 Jun 2021 23:00
Operator : JU/CG
Sample : M2826-02 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LS-1(LIQUID-BLUE)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc