
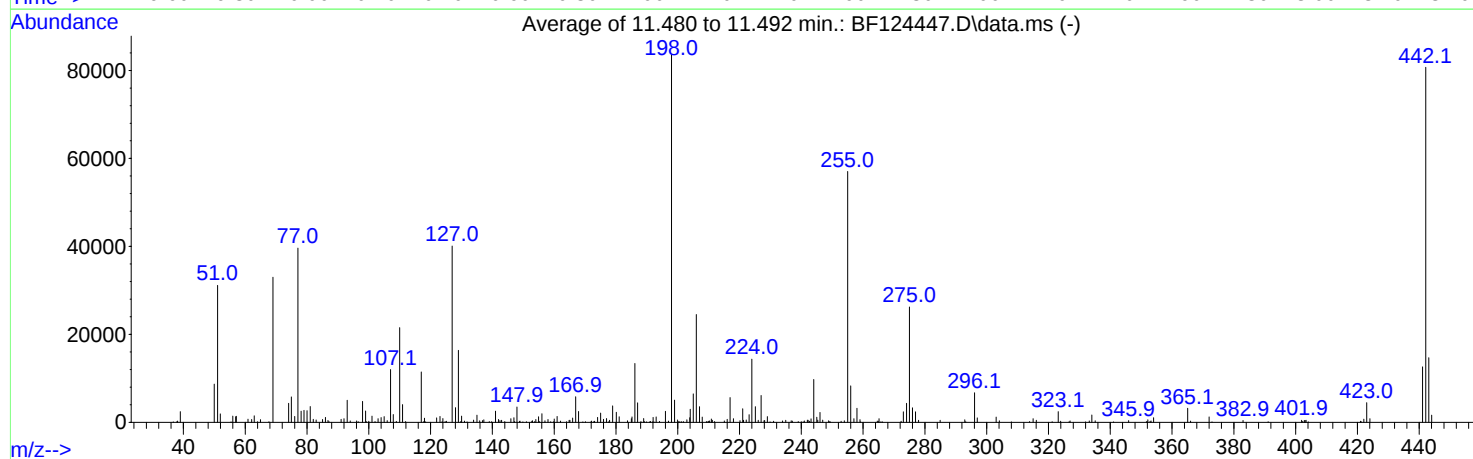


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
 Data File : BF124447.D
 Acq On : 25 Jun 2021 12:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 28 16:01:42 2021

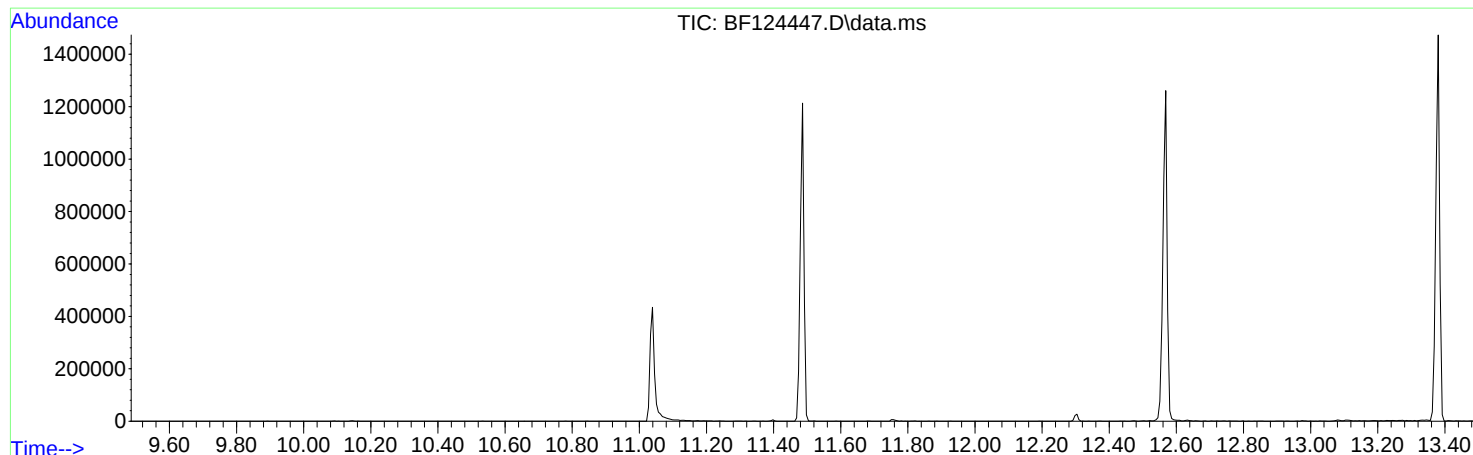




AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	31146	PASS
68	69	0.00	2	0.5	151	PASS
69	198	0.00	100	39.4	32977	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	40089	PASS
197	198	0.00	2	0.4	296	PASS
198	198	100	100	100.0	83624	PASS
199	198	5	9	6.0	5052	PASS
275	198	10	60	31.4	26244	PASS
365	198	1	100	3.8	3189	PASS
441	198	0.01	100	15.1	12633	PASS
442	442	50	100	100.0	80699	PASS
443	442	15	24	18.2	14680	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
 Data File : BF124447.D
 Acq On : 25 Jun 2021 12:18
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 25 13:19:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 18:48:27 2021
 Response via : Initial Calibration

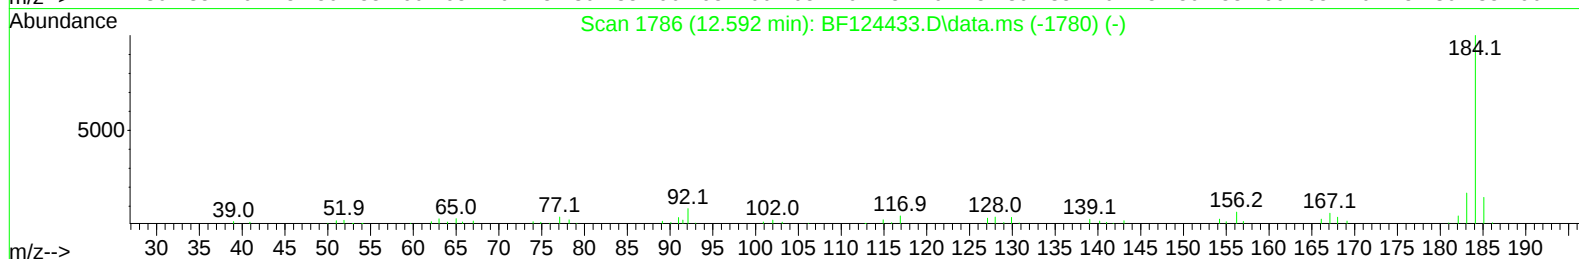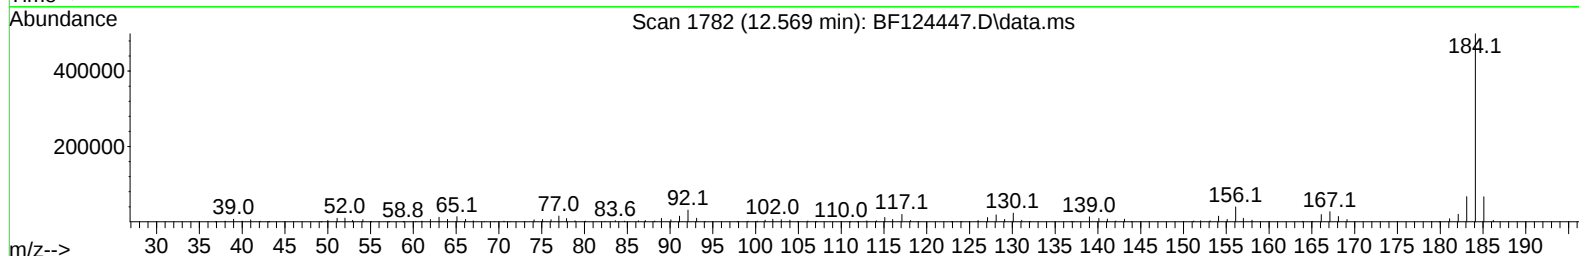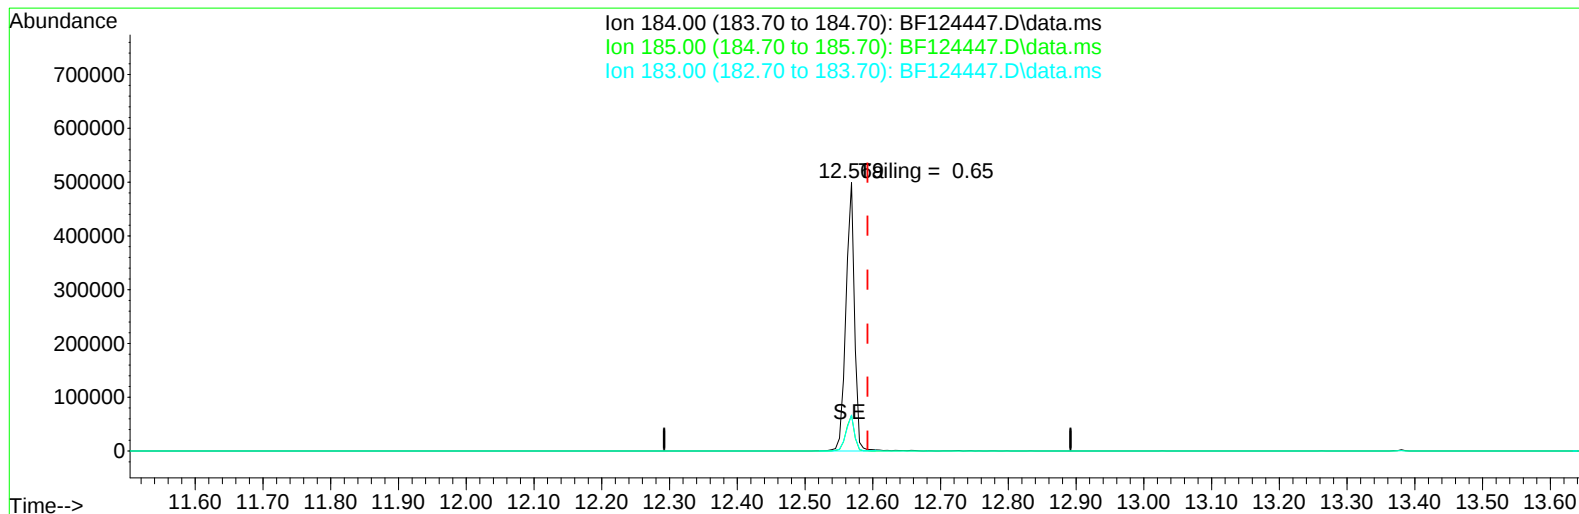

TIC: BF124447.D\data.ms

(77) Benzidine

12.569min (-0.024) 0.00 ng




response 440460

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.30
183.00	9.80	13.44#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062521\
Data File : BF124447.D
Acq On : 25 Jun 2021 12:18
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 25 13:19:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 18:48:27 2021
Response via : Initial Calibration

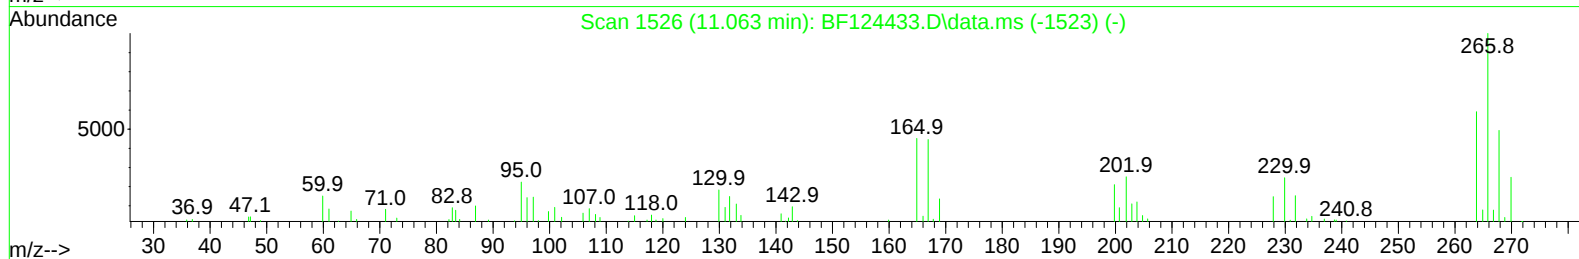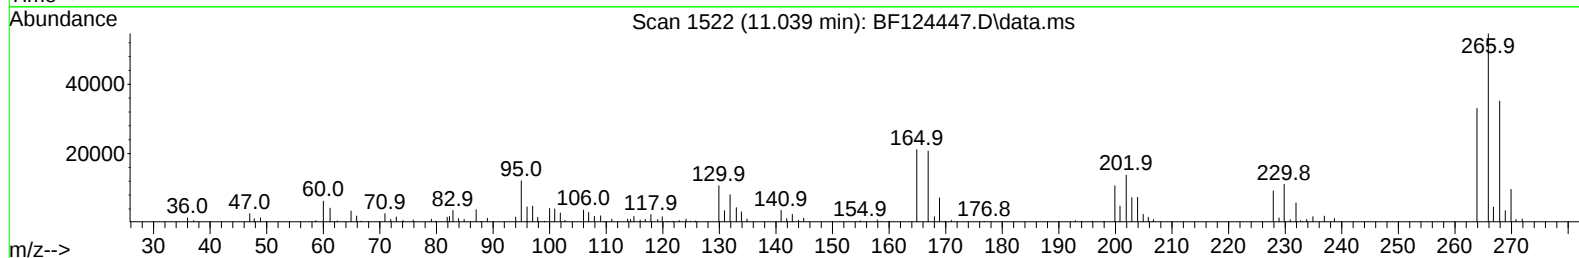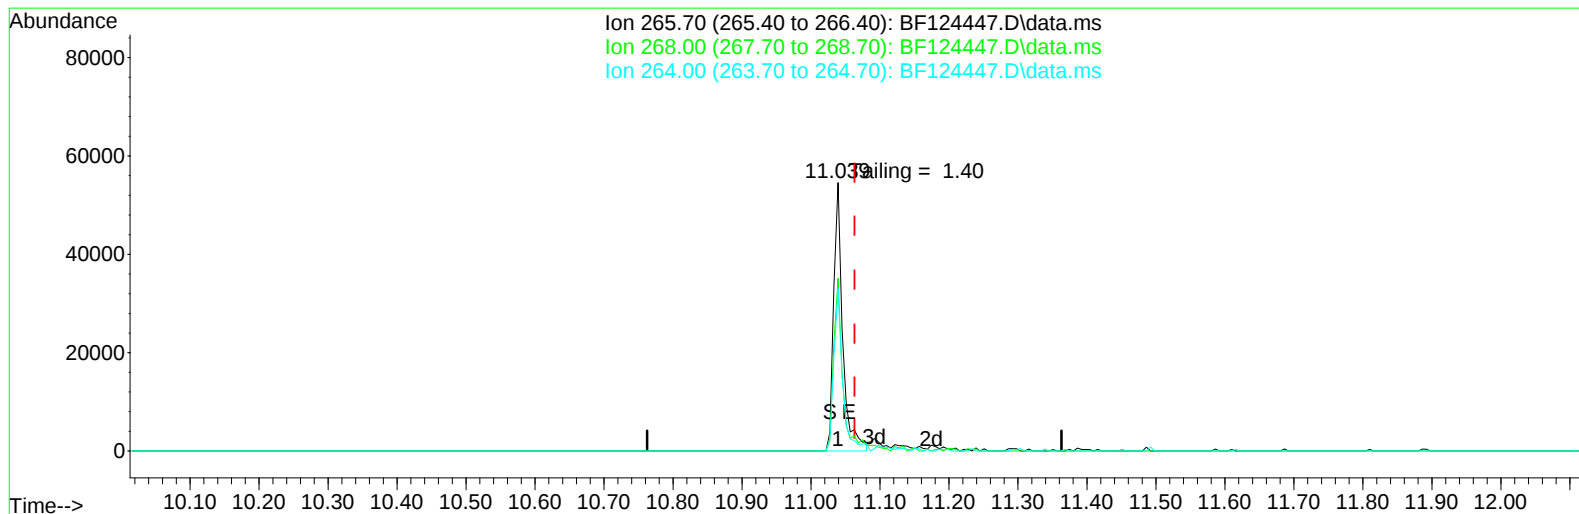

TIC: BF124447.D\data.ms

(70) Pentachlorophenol (C)

11.039min (-0.024) 68752.69 ng

response 49682

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.37
264.00	65.70	60.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/25/2021	BNA_F	<u>BF124447.D</u>
Compound Name	Response	Retention Time
DDT	220791	13.38
DDD	1695	13.08
DDE	255	12.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1950	222741	0.88