
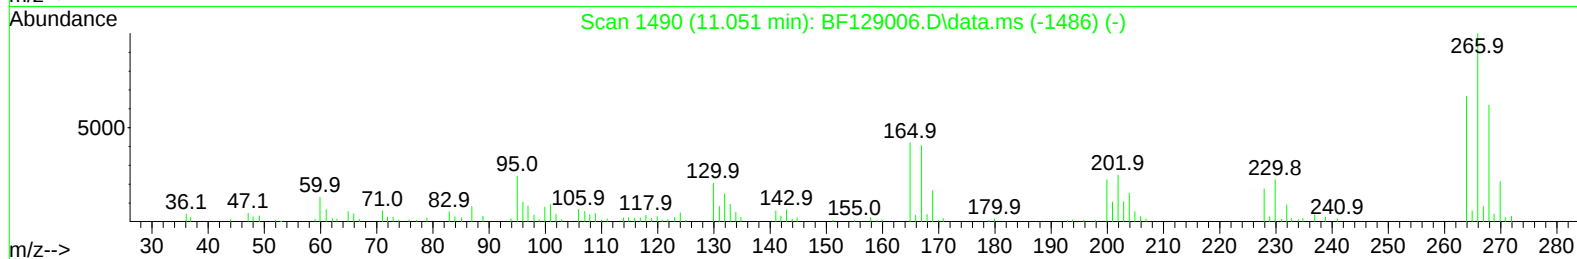
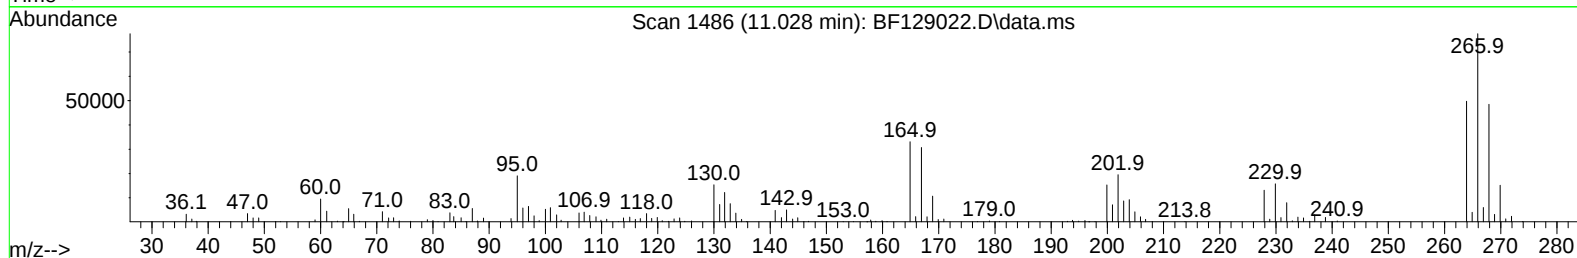


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062722\
Data File : BF129022.D
Acq On : 27 Jun 2022 10:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 07:03:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 28 06:51:48 2022
Response via : Initial Calibration

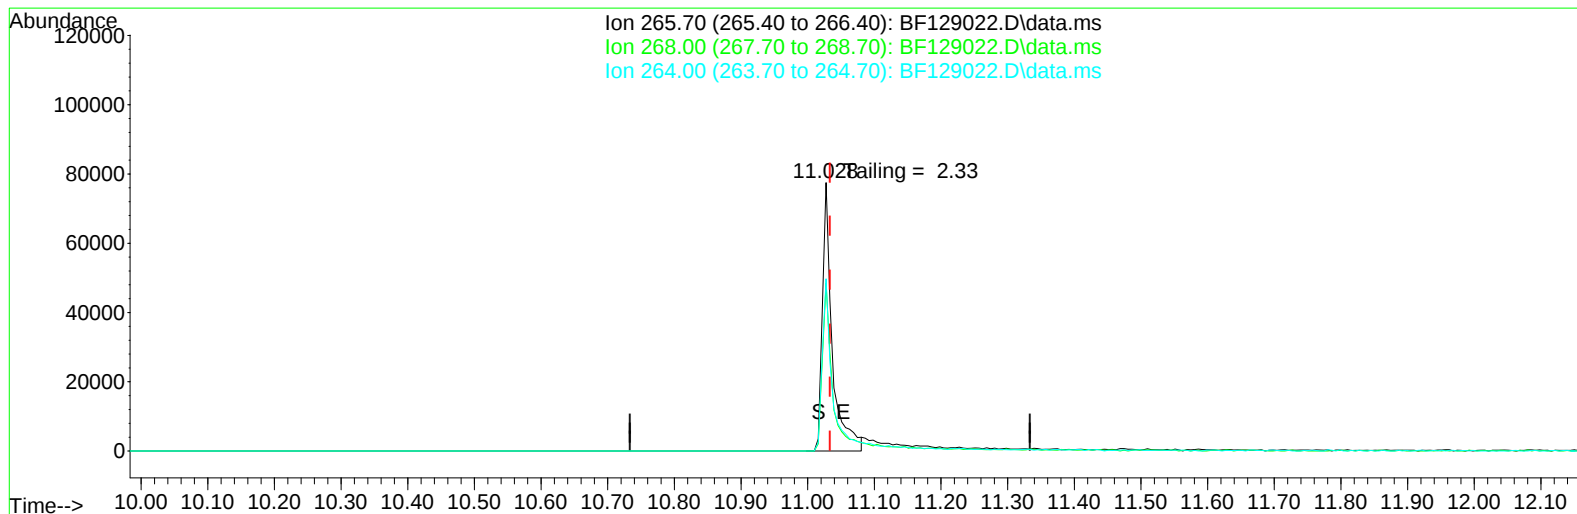

TIC: BF129022.D\data.ms

(70) Pentachlorophenol (C)




11.028min (-0.006) 491591.91 ng

response 90871

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.57
264.00	61.80	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062722\
 Data File : BF129022.D
 Acq On : 27 Jun 2022 10:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 07:03:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 28 06:51:48 2022
 Response via : Initial Calibration

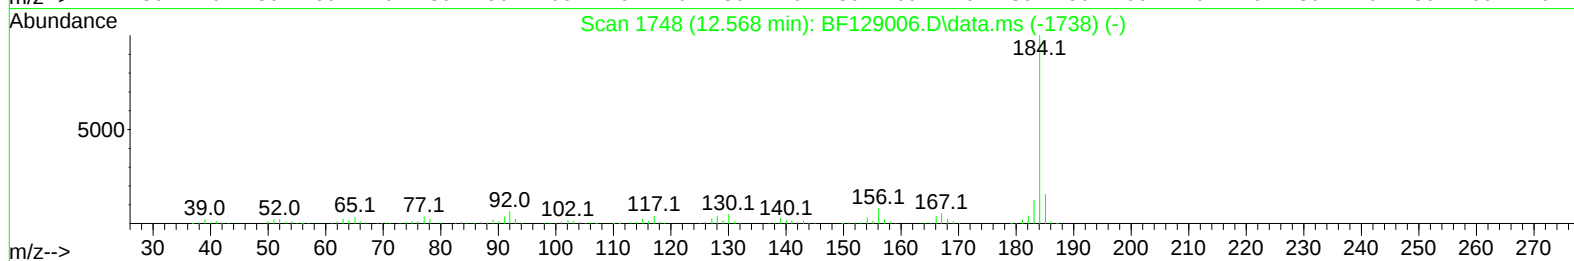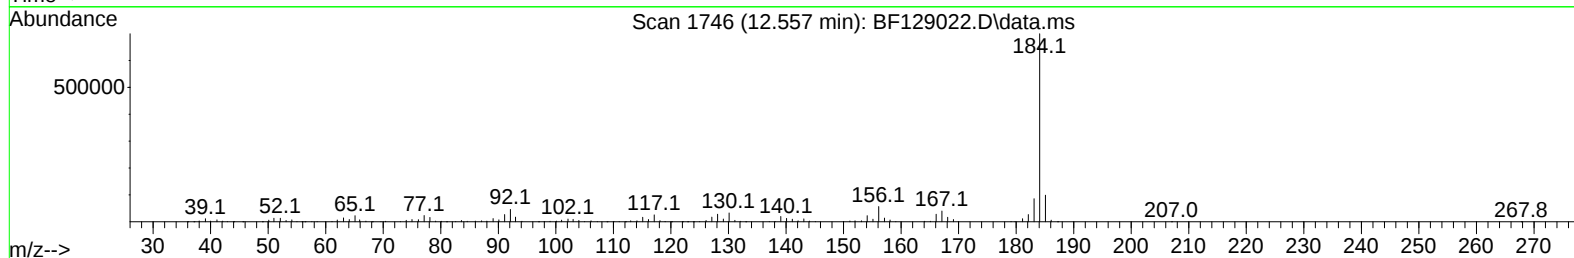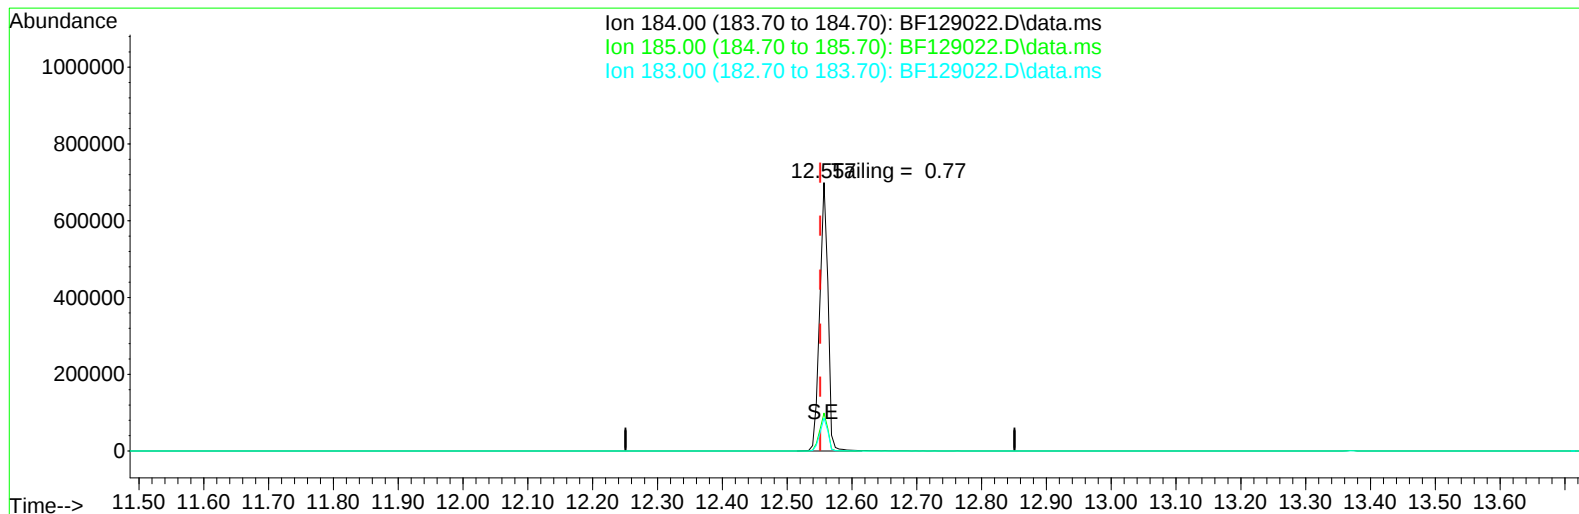

TIC: BF129022.D\data.ms

(77) Benzidine

12.557min (+ 0.006) 0.00 ng

response 625319

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.12
183.00	11.60	12.25
0.00	0.00	0.00