
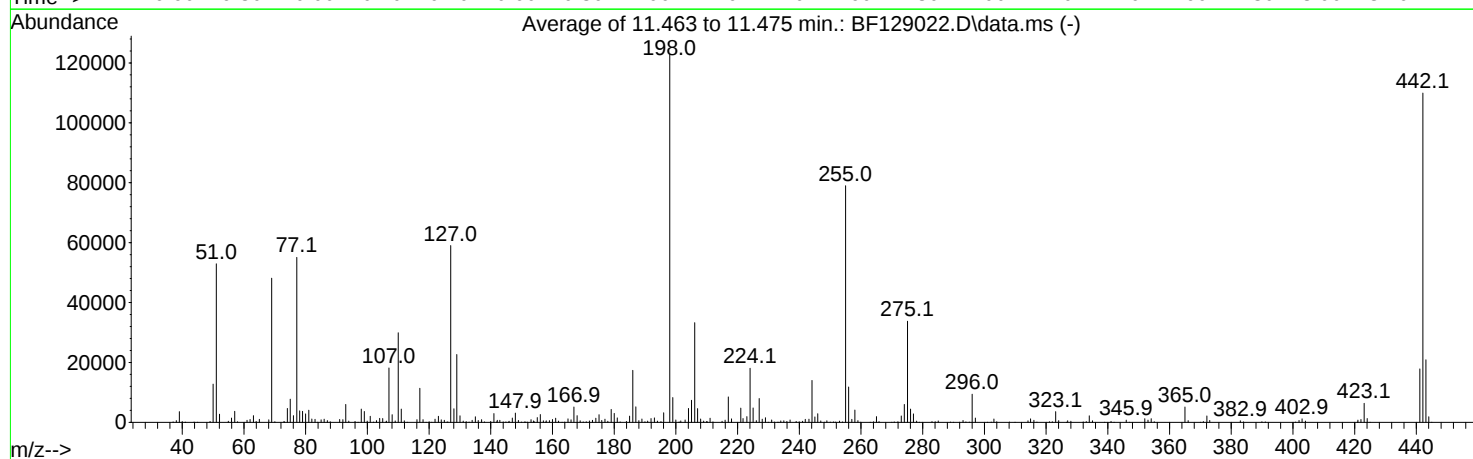


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062722\
 Data File : BF129022.D
 Acq On : 27 Jun 2022 10:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 29 16:19:25 2022

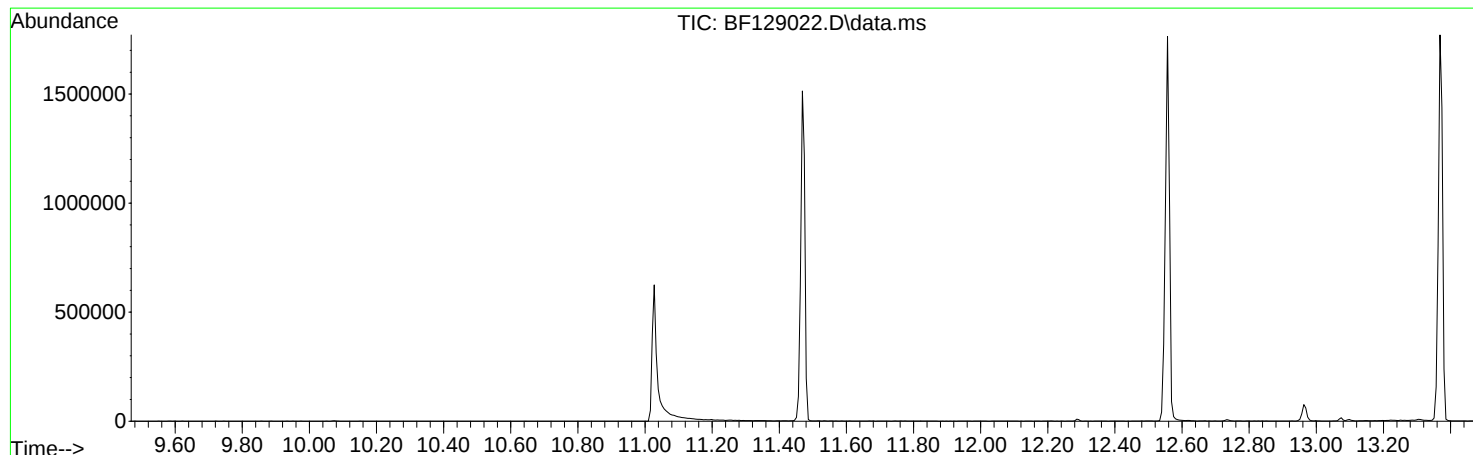




AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	52936	PASS
68	69	0.00	2	1.8	857	PASS
69	198	0.00	100	39.2	48112	PASS
70	69	0.00	2	0.5	222	PASS
127	198	10	80	48.1	59035	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	122808	PASS
199	198	5	9	6.8	8295	PASS
275	198	10	60	27.5	33742	PASS
365	198	1	100	4.2	5143	PASS
441	198	0.01	100	14.5	17821	PASS
442	442	50	100	100.0	109947	PASS
443	442	15	24	19.0	20909	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062722\
 Data File : BF129022.D
 Acq On : 27 Jun 2022 10:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 28 07:03:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 28 06:51:48 2022
 Response via : Initial Calibration

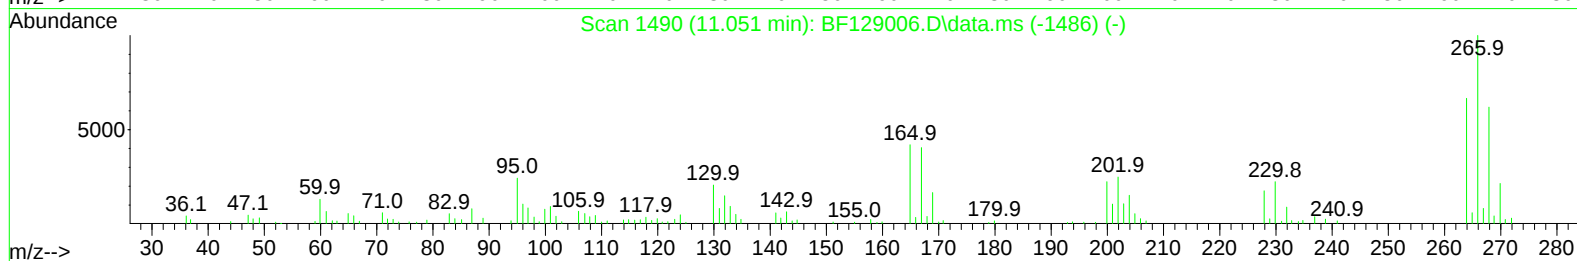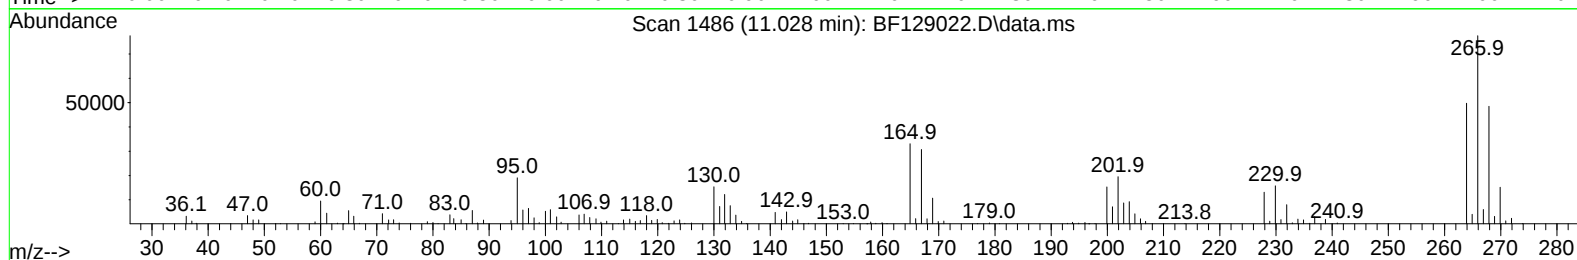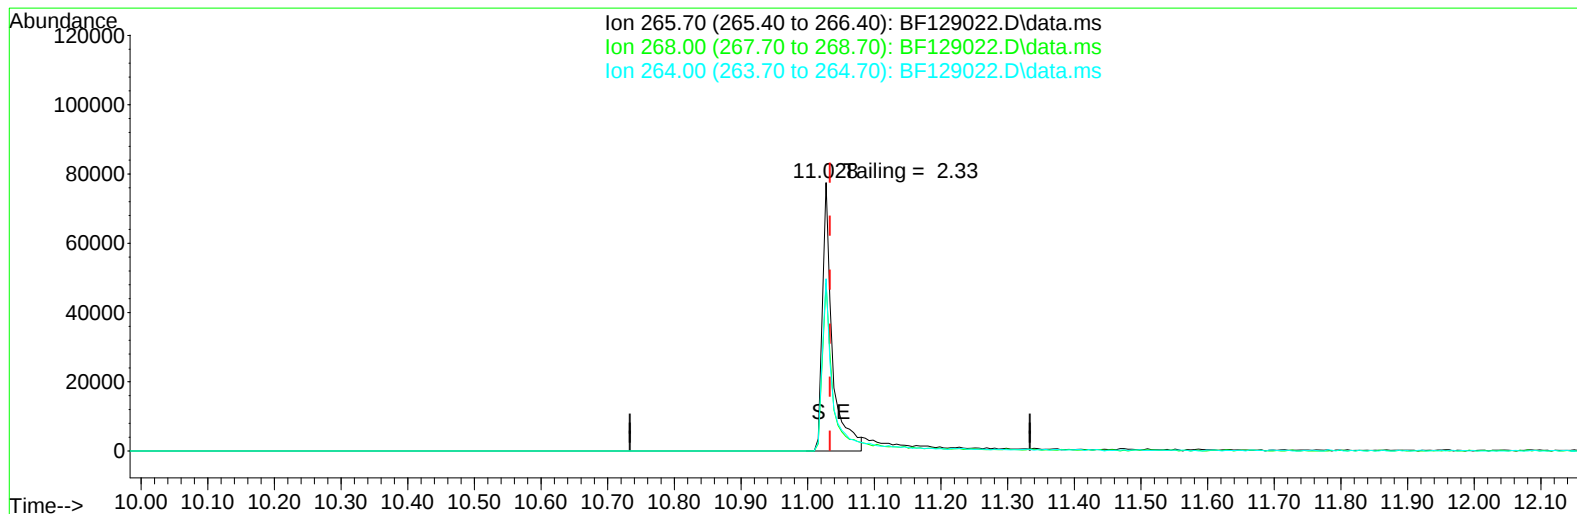

TIC: BF129022.D\data.ms

(70) Pentachlorophenol (C)

11.028min (-0.006) 491591.91 ng




response 90871

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.57
264.00	61.80	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062722\
 Data File : BF129022.D
 Acq On : 27 Jun 2022 10:40
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 28 07:03:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 28 06:51:48 2022
 Response via : Initial Calibration

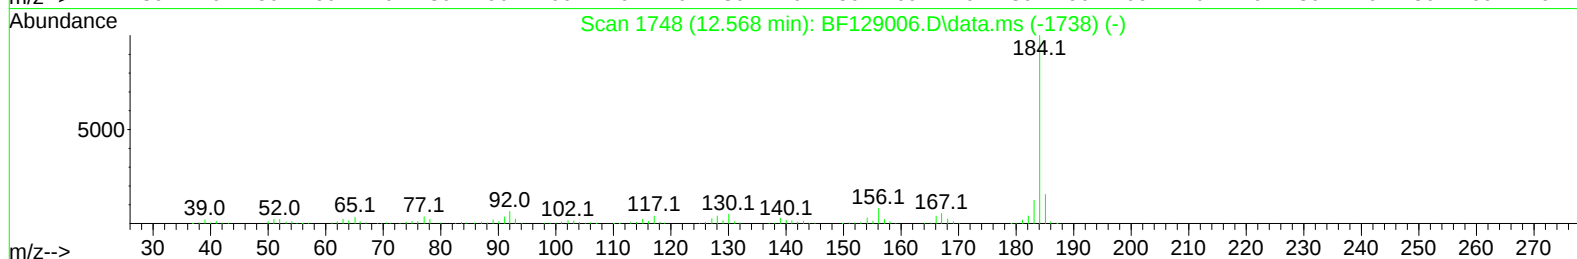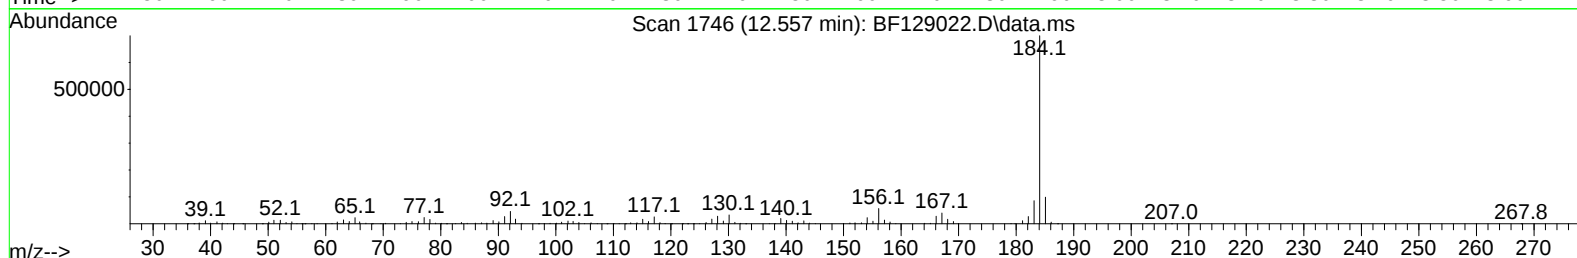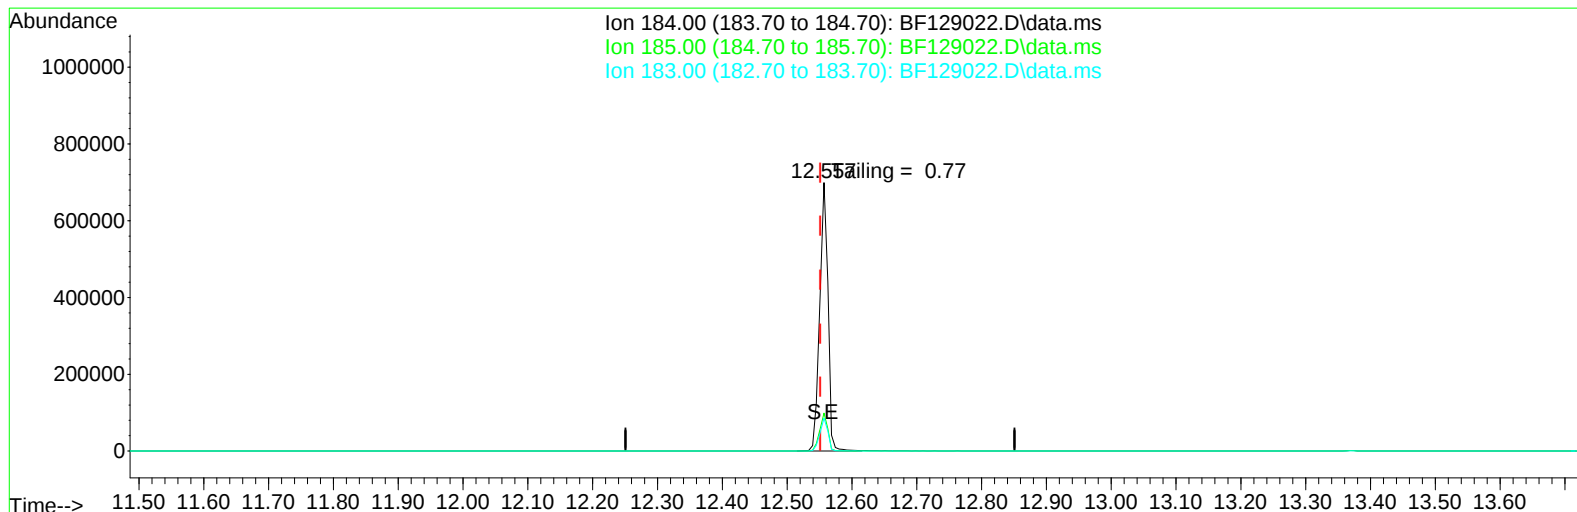

TIC: BF129022.D\data.ms

(77) Benzidine

12.557min (+ 0.006) 0.00 ng

response 625319

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.12
183.00	11.60	12.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/27/2022	BNA_F	<u>BF129022.D</u>
Compound Name	Response	Retention Time
DDT	305690	13.36
DDD	2894	13.07
DDE	1152	12.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4046	309736	1.31

Instrument :
BNA_F
ClientSampleId :
DFTPP