
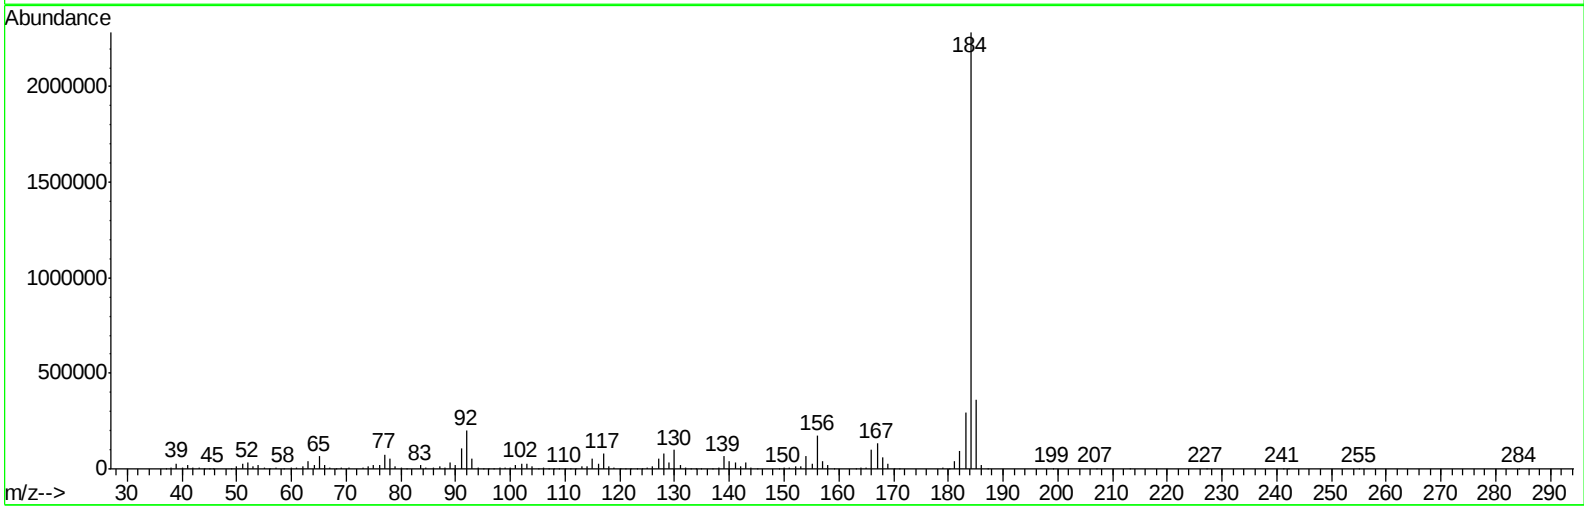


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062819\
Data File : BF115265.D
Acq On : 28 Jun 2019 7:45
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 06:26:14 2019
Quant Method : Z:\SV0ASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 05:26:43 2019
Response via : Initial Calibration

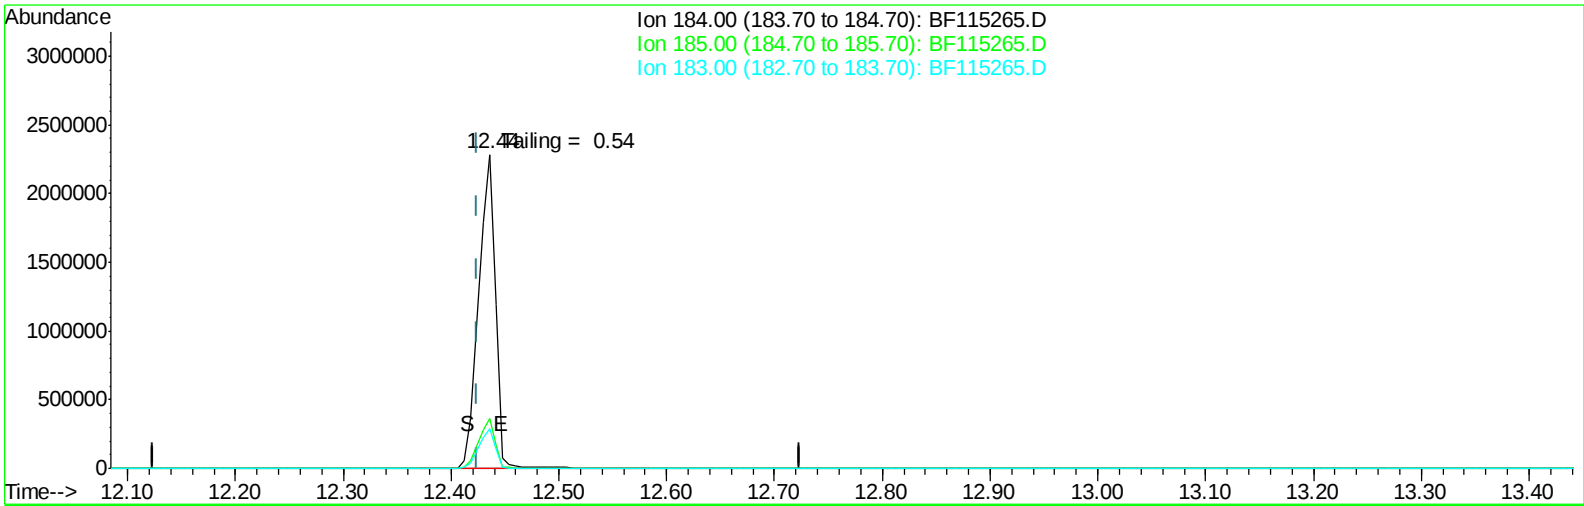

TIC: BF115265.D

(77) Benzidine



12.436min (+0.012) 1408.67ng

response 2471246

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.79
183.00	12.00	12.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF062819\
Data File : BF115265.D
Acq On : 28 Jun 2019 7:45
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 06:26:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 05:26:43 2019
Response via : Initial Calibration

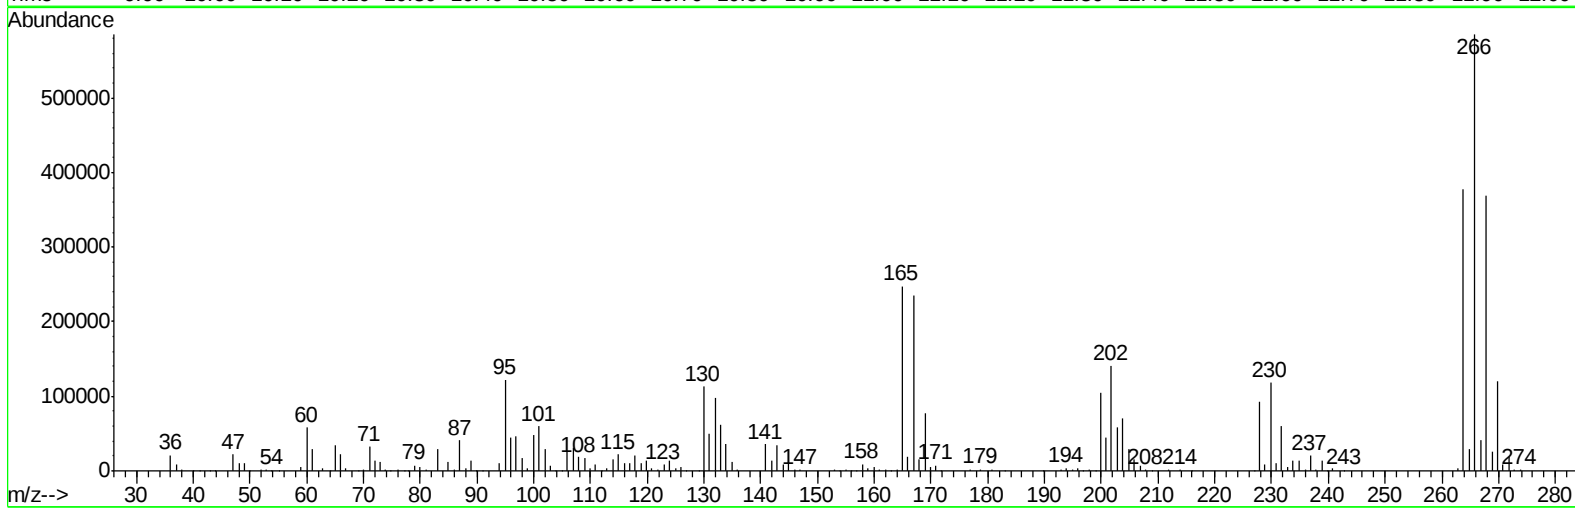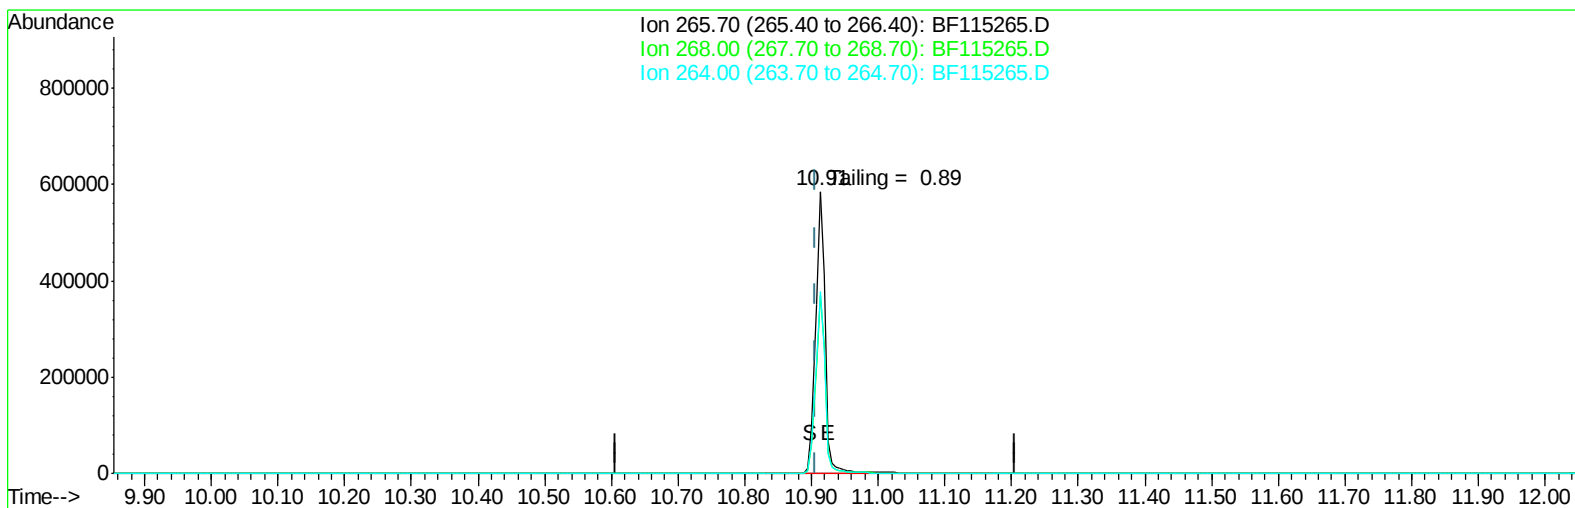

TIC: BF115265.D

(70) Pentachlorophenol (C)

10.913min (+0.006) 3209.57ng

response 569887

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	62.97
264.00	61.60	64.47
0.00	0.00	0.00