

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
 Data File : BF115267.D
 Acq On : 28 Jun 2019 8:38
 Operator : HP/JU
 Sample : PB120890BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120890BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.207	550	556	559	rBV	5178162	5599168	72.16%	9.502%
2	6.242	726	732	735	rBV	4893836	5793439	74.67%	9.832%
3	6.372	748	754	757	rBV	5698509	5962227	76.84%	10.118%
4	6.601	789	793	796	rBV	1622206	1453125	18.73%	2.466%
5	6.754	815	819	823	rBV	5063817	4923968	63.46%	8.356%
6	7.160	882	888	891	rBV	3558576	3856068	49.70%	6.544%
7	7.878	1005	1010	1014	rBV	2055555	1883799	24.28%	3.197%
8	8.960	1188	1194	1197	rBV	7091790	7311193	94.23%	12.407%
9	9.625	1302	1307	1311	rBV2	2550776	2183547	28.14%	3.706%
10	10.407	1435	1440	1444	rBV	4195915	4528396	58.36%	7.685%
11	11.095	1553	1557	1561	rBV	2515756	2374805	30.61%	4.030%
12	12.689	1822	1828	1831	rBV	6844993	7759109	100.00%	13.167%
13	13.718	1998	2003	2006	rBV	2381667	2289494	29.51%	3.885%
14	14.812	2186	2189	2193	rVB	86114	92888	1.20%	0.158%
15	15.083	2230	2235	2239	rBV	2051100	2314665	29.83%	3.928%
16	15.148	2242	2246	2250	rVB	118743	147308	1.90%	0.250%
17	15.524	2306	2310	2317	rVB3	170567	296972	3.83%	0.504%
18	15.965	2381	2385	2390	rVB	96710	156081	2.01%	0.265%


Sum of corrected areas: 58926252

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115267.D
Acq On : 28 Jun 2019 8:38
Operator : HP/JU
Sample : PB120890BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120890BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

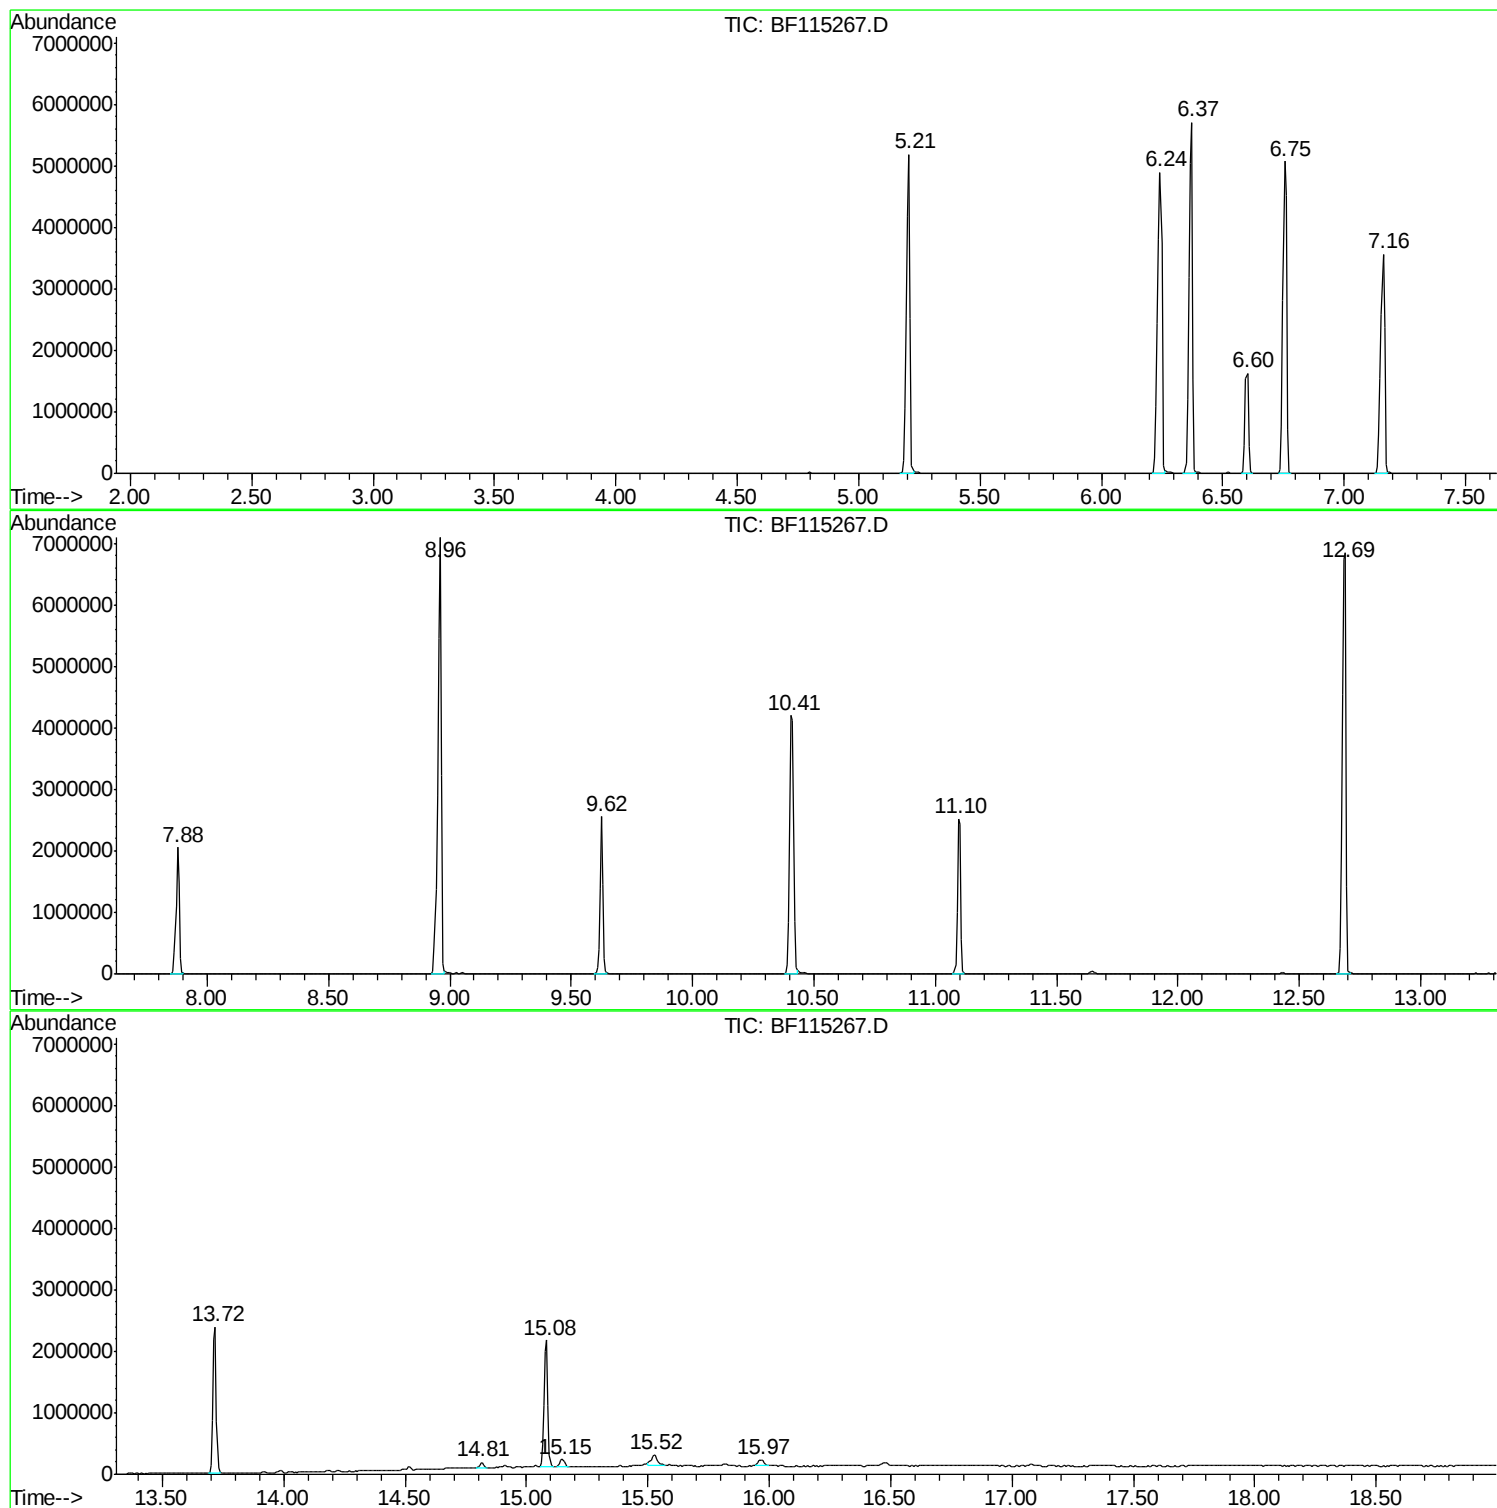

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115267.D
Acq On : 28 Jun 2019 8:38
Operator : HP/JU
Sample : PB120890BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120890BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.37	82.06 ng	5962230	1,4-Dichlorobenzene-d4	6.60

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	16
3		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

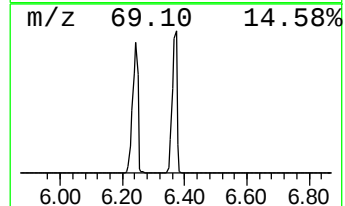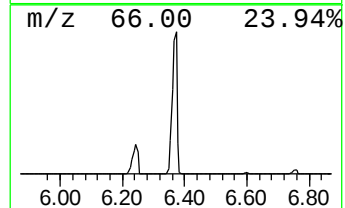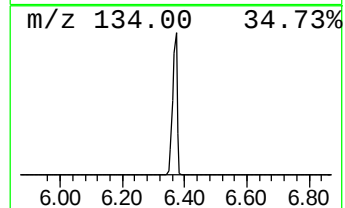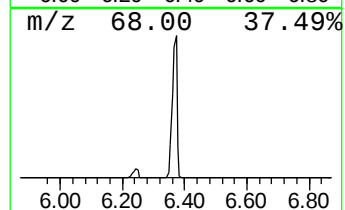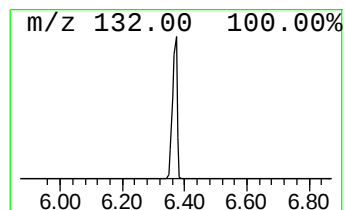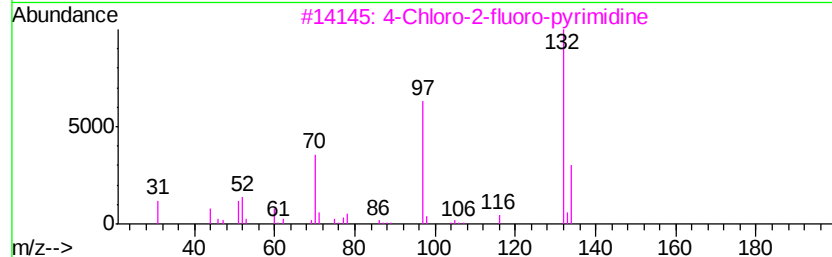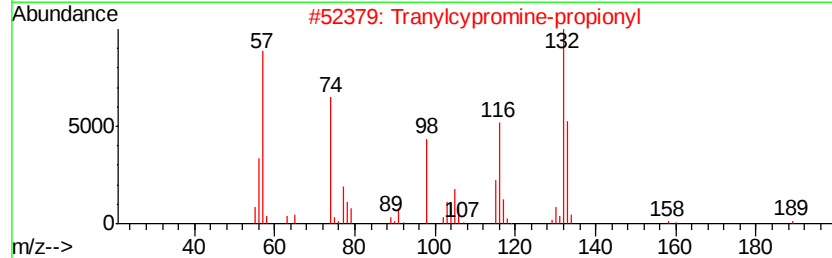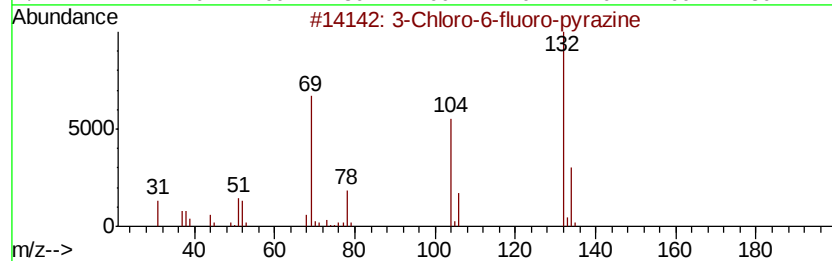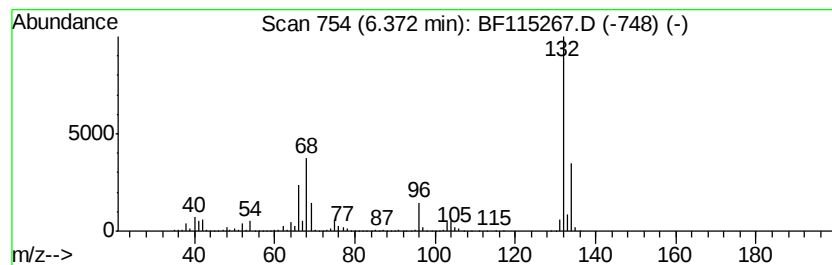

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115267.D
Acq On : 28 Jun 2019 8:38
Operator : HP/JU
Sample : PB120890BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120890BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Hexadecane Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.52	2.57 ng	296972	Perylene-d12	15.08

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Hexadecane	226	C16H34	000544-76-3	91
2		Heneicosane	296	C21H44	000629-94-7	87
3		Eicosane	282	C20H42	000112-95-8	86
4		Pentacosane	352	C25H52	000629-99-2	86
5		Octacosane	394	C28H58	000630-02-4	86

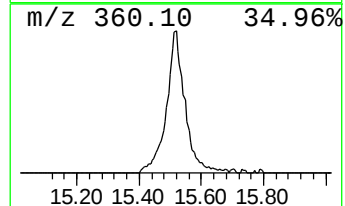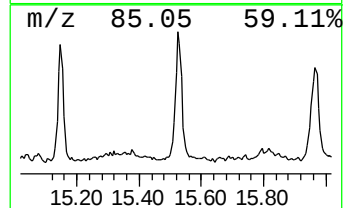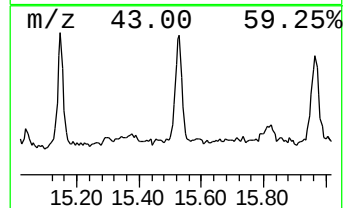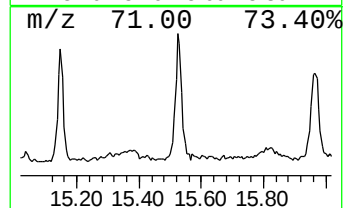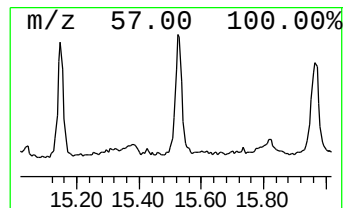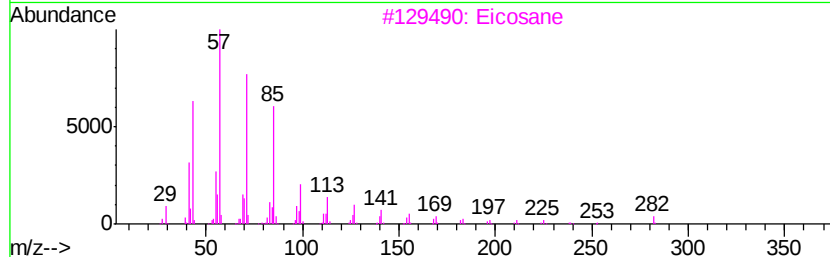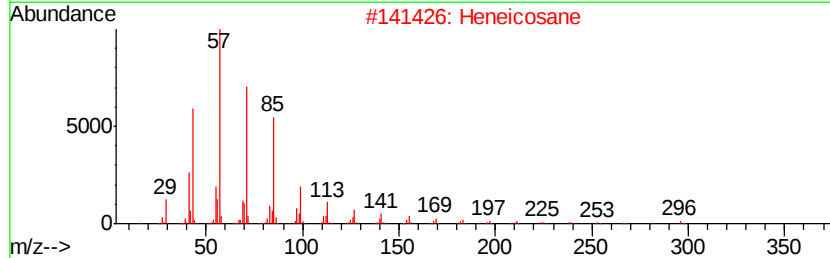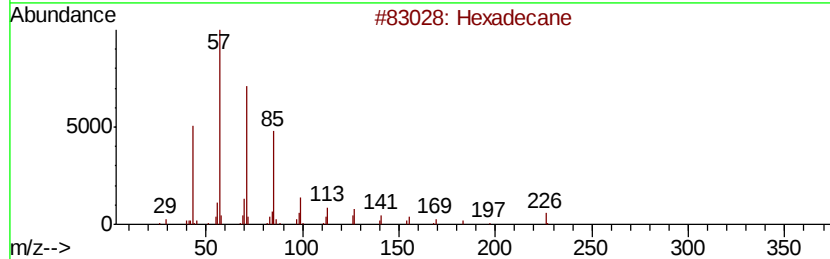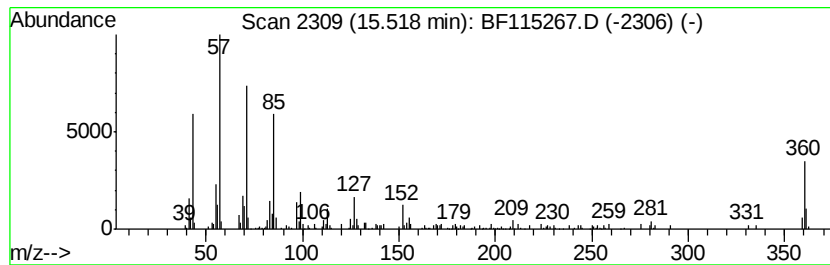

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
Data File : BF115267.D
Acq On : 28 Jun 2019 8:38
Operator : HP/JU
Sample : PB120890BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120890BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.37	6.37	82.1	ng	5962230	1	6.60	1453130	20.0
Hexadecane	15.52	2.6	ng	296972	6	15.08	2314670	20.0