

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
 Data File : BF115273.D
 Acq On : 28 Jun 2019 11:35
 Operator : HP/JU
 Sample : PB120961BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120961BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.201	550	555	559	rBV	4569755	5324609	68.66%	9.540%
2	6.242	725	732	735	rBV	4950168	5409813	69.76%	9.693%
3	6.366	748	753	757	rBV	5171875	5744243	74.07%	10.292%
4	6.595	789	792	796	rBV	1586178	1330784	17.16%	2.384%
5	6.754	815	819	822	rBV	5076619	4713628	60.78%	8.445%
6	7.160	882	888	891	rBV	3533177	3680532	47.46%	6.594%
7	7.878	1005	1010	1013	rBV	1973213	1706484	22.01%	3.057%
8	8.960	1188	1194	1197	rBV	6625947	7101256	91.57%	12.723%
9	9.625	1302	1307	1316	rBV	2313564	2055653	26.51%	3.683%
10	10.407	1434	1440	1443	rBV	4400892	4482051	57.80%	8.030%
11	11.095	1553	1557	1561	rBV	2632407	2227388	28.72%	3.991%
12	12.683	1822	1827	1830	rBV	6955412	7754654	100.00%	13.894%
13	13.713	1998	2002	2006	rBV	2306765	2084379	26.88%	3.735%
14	15.077	2229	2234	2239	rBV	1814563	2098601	27.06%	3.760%
15	15.148	2243	2246	2253	rVB	70286	99244	1.28%	0.178%


Sum of corrected areas: 55813319

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115273.D
Acq On : 28 Jun 2019 11:35
Operator : HP/JU
Sample : PB120961BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120961BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

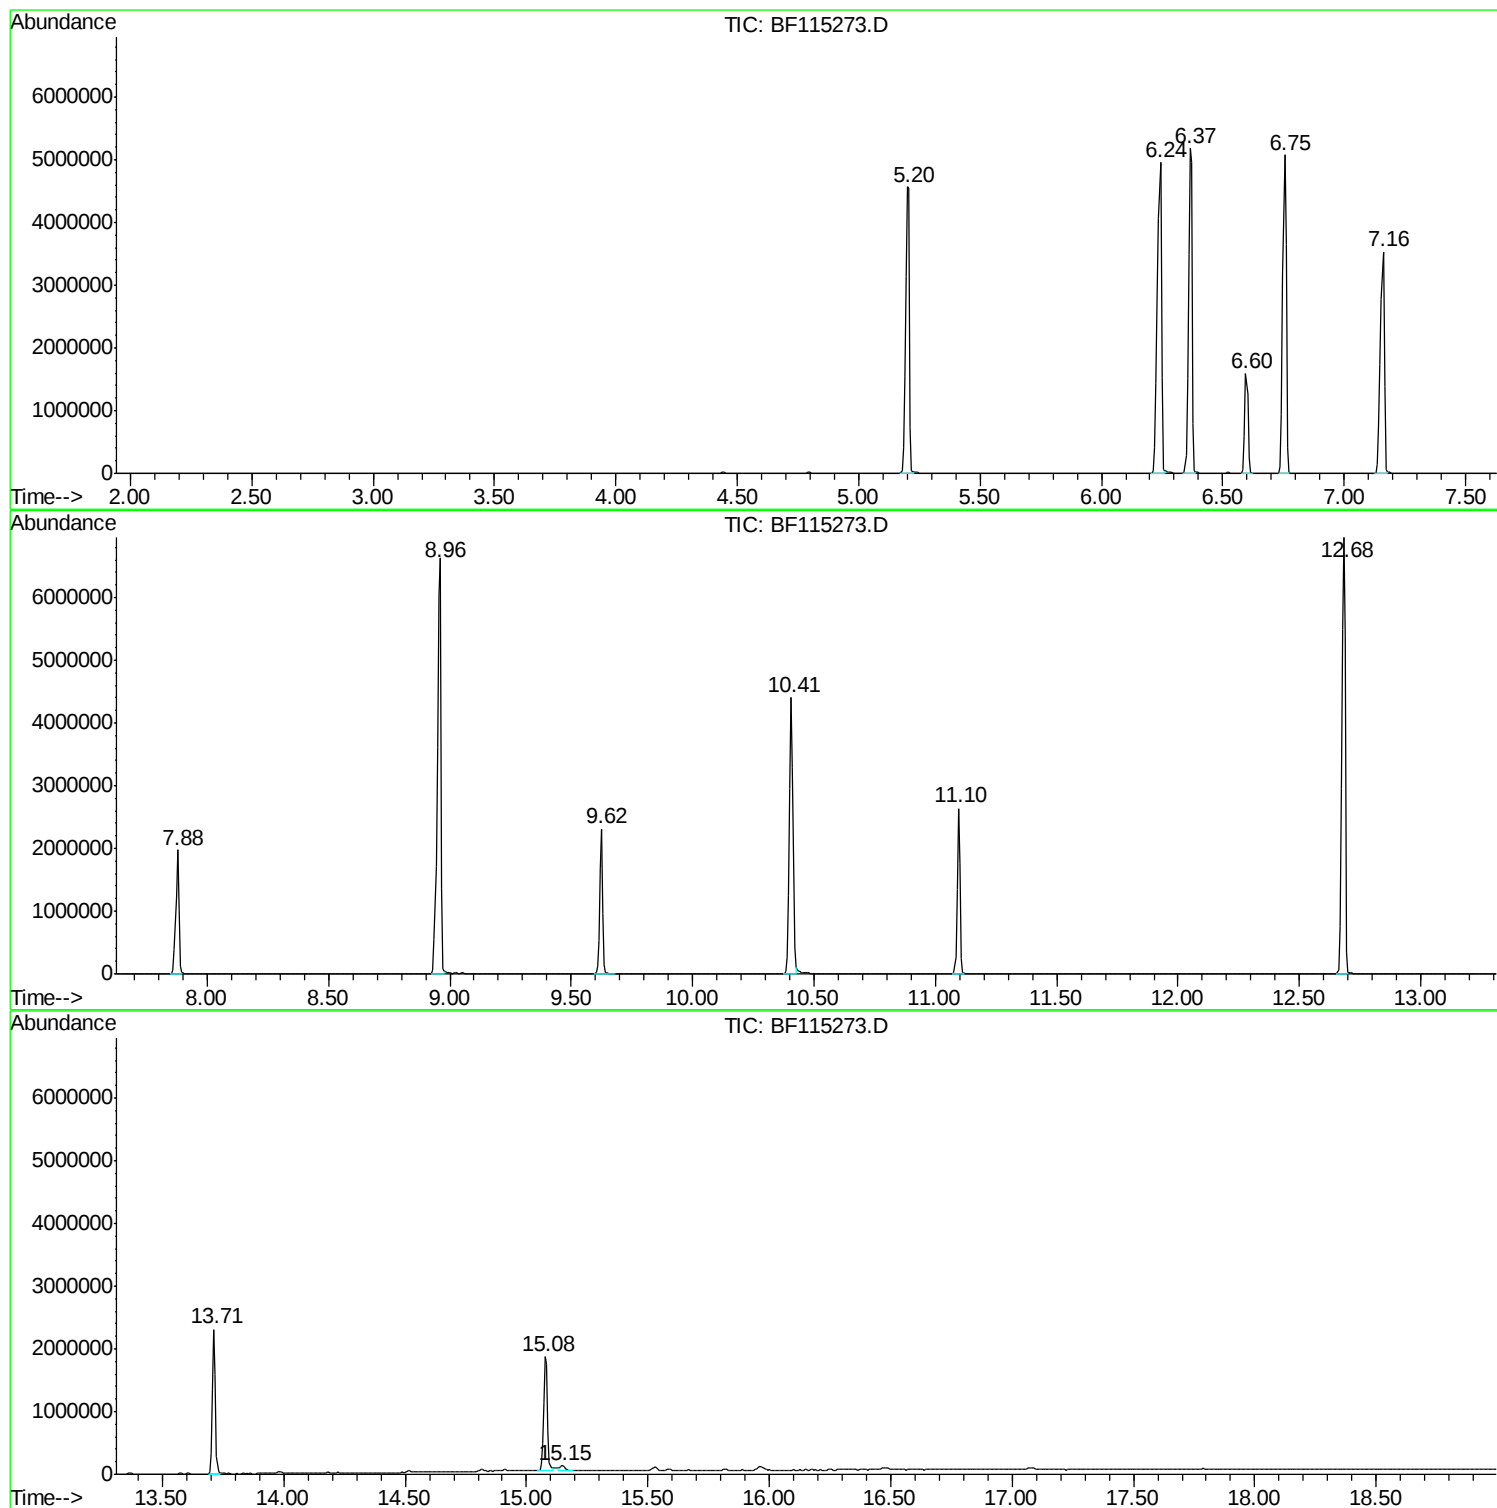

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115273.D
Acq On : 28 Jun 2019 11:35
Operator : HP/JU
Sample : PB120961BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120961BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.37	86.33 ng	5744240	1,4-Dichlorobenzene-d4	6.60

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

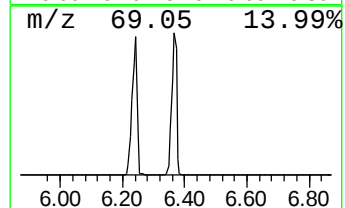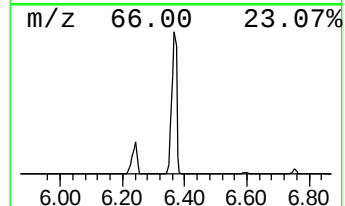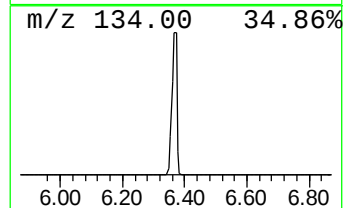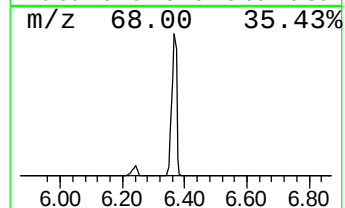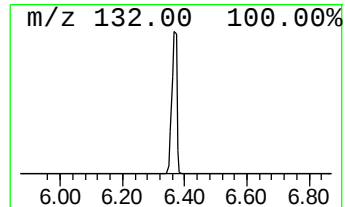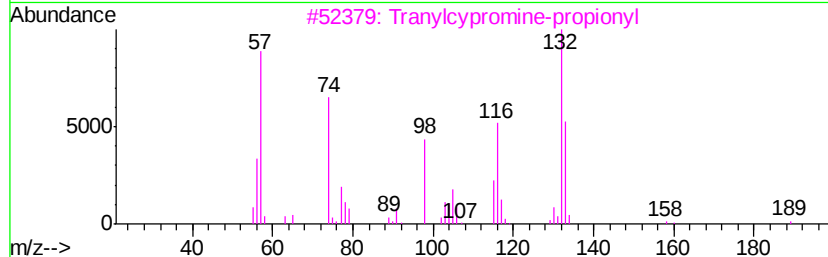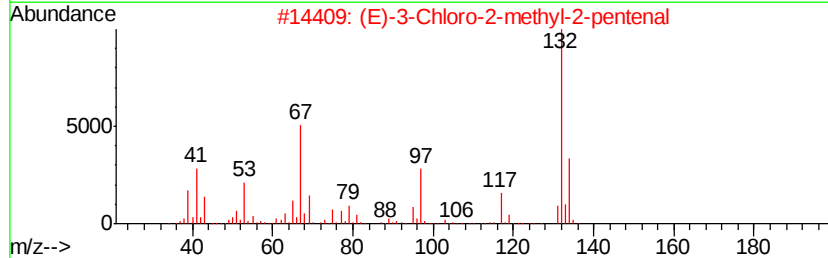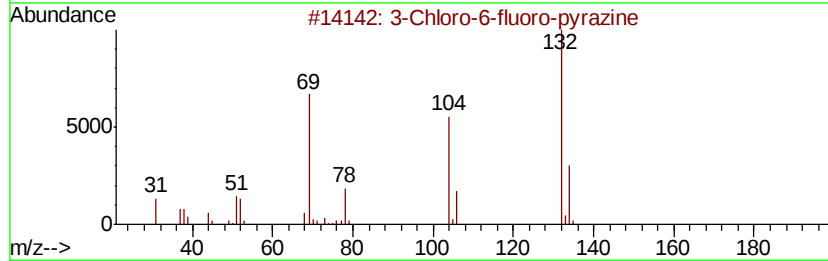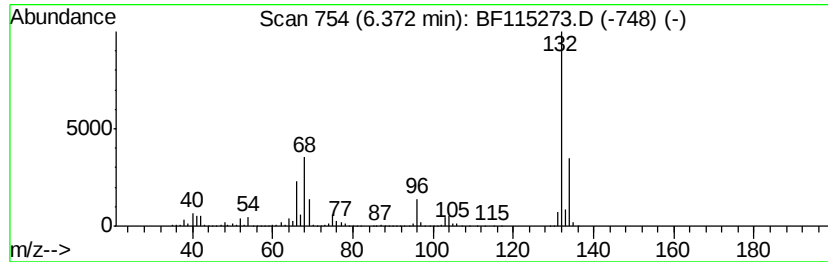

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
Data File : BF115273.D
Acq On : 28 Jun 2019 11:35
Operator : HP/JU
Sample : PB120961BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120961BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.37	6.37	86.3	ng	5744240	1	6.60	1330780	20.0