

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
 Data File : BF115275.D
 Acq On : 28 Jun 2019 12:28
 Operator : HP/JU
 Sample : PB120979BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120979BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.201	550	555	558	rBV	4576279	5144784	72.08%	9.745%
2	6.242	725	732	735	rBV	4778112	5168708	72.41%	9.791%
3	6.366	748	753	757	rBV	5148885	5535638	77.55%	10.486%
4	6.595	789	792	796	rBV	1559263	1286067	18.02%	2.436%
5	6.754	815	819	822	rBV	5020527	4509185	63.17%	8.541%
6	7.160	882	888	891	rBV	3474310	3499208	49.02%	6.628%
7	7.878	1005	1010	1013	rBV	1841134	1633800	22.89%	3.095%
8	8.954	1188	1193	1197	rBV	6195666	6757170	94.67%	12.800%
9	9.624	1302	1307	1317	rBV	2104174	1919161	26.89%	3.635%
10	10.407	1434	1440	1443	rBV	4343318	4068530	57.00%	7.707%
11	11.095	1553	1557	1560	rBV	2501273	2060257	28.86%	3.903%
12	12.683	1822	1827	1830	rBV	6812590	7137912	100.00%	13.521%
13	13.712	1998	2002	2006	rBV	2242103	1964374	27.52%	3.721%
14	15.083	2230	2235	2240	rBV	1819197	2030961	28.45%	3.847%
15	15.154	2244	2247	2255	rVB4	52873	75751	1.06%	0.143%


Sum of corrected areas: 52791506

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115275.D
Acq On : 28 Jun 2019 12:28
Operator : HP/JU
Sample : PB120979BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120979BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

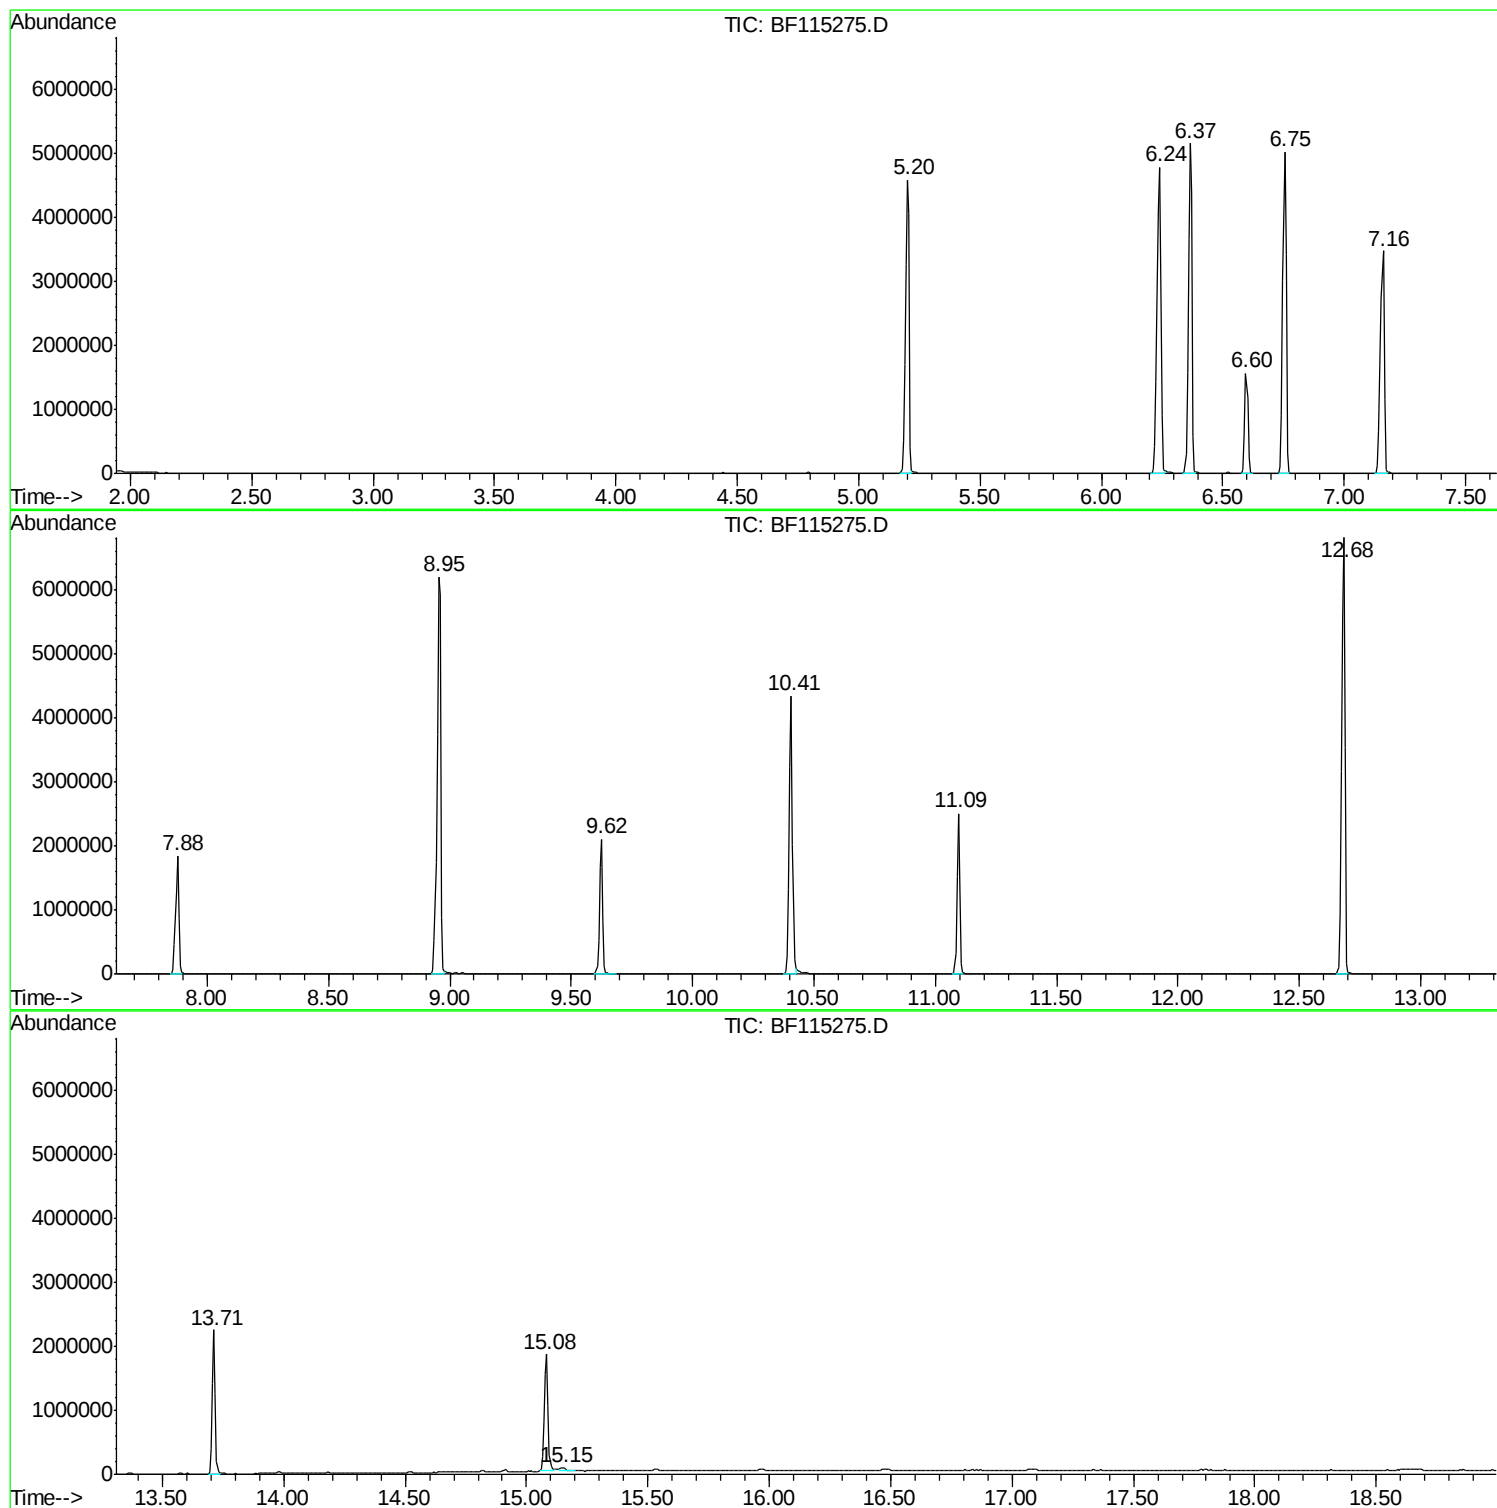

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115275.D
Acq On : 28 Jun 2019 12:28
Operator : HP/JU
Sample : PB120979BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120979BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.37	86.09 ng	5535640	1,4-Dichlorobenzene-d4	6.60

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		Xenon	132	Xe	007440-63-3	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

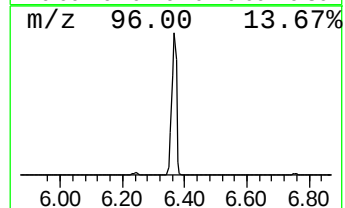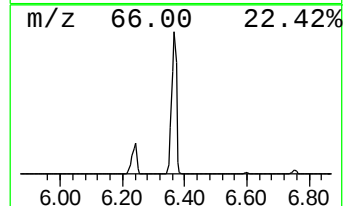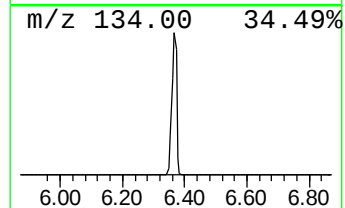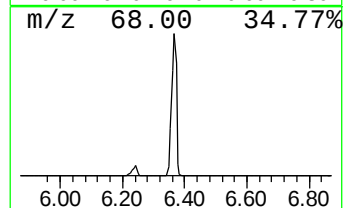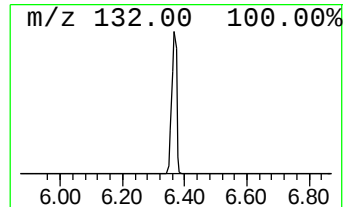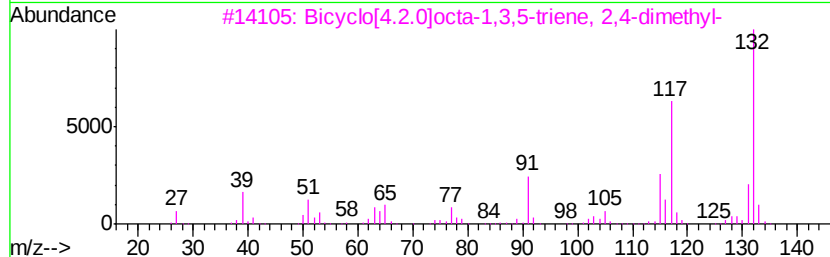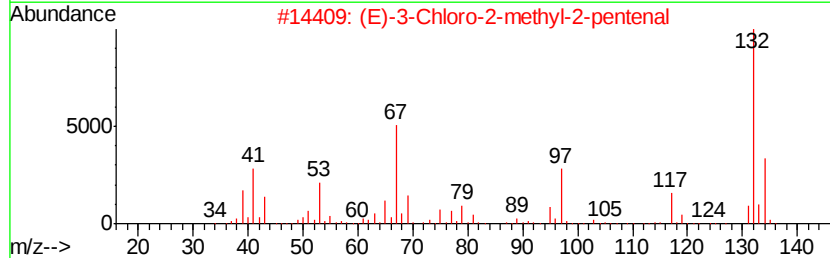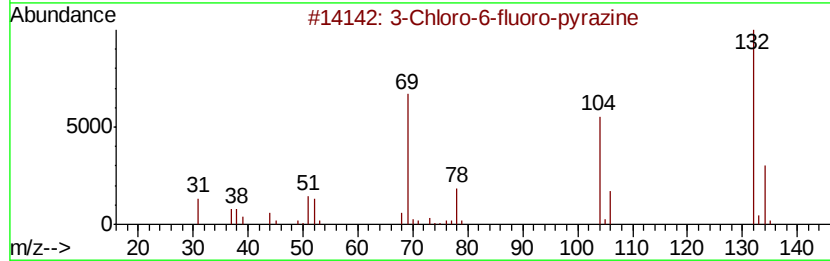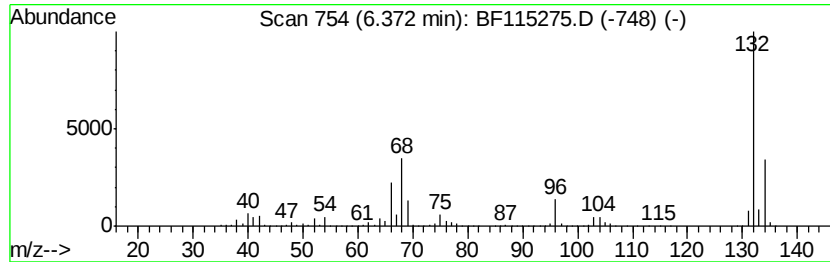

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
Data File : BF115275.D
Acq On : 28 Jun 2019 12:28
Operator : HP/JU
Sample : PB120979BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120979BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.37	6.37	86.1	ng	5535640	1	6.60	1286070	20.0