

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
 Data File : BF115278.D
 Acq On : 28 Jun 2019 13:47
 Operator : HP/JU
 Sample : PB120984BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120984BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.201	550	555	558	rBV	4607352	5148136	71.79%	9.487%
2	6.242	725	732	735	rBV	4801848	5233484	72.98%	9.644%
3	6.366	748	753	756	rBV	5339035	5495012	76.63%	10.126%
4	6.595	789	792	796	rBV	1817493	1501660	20.94%	2.767%
5	6.754	815	819	822	rBV	5032444	4511181	62.91%	8.313%
6	7.160	882	888	891	rBV	3497904	3477731	48.50%	6.409%
7	7.877	1005	1010	1013	rBV	2187227	1931823	26.94%	3.560%
8	8.954	1188	1193	1197	rBV	6144971	6693016	93.33%	12.334%
9	9.624	1301	1307	1316	rBV	2446180	2222656	30.99%	4.096%
10	10.407	1434	1440	1443	rBV	4240892	4050187	56.48%	7.464%
11	11.095	1553	1557	1560	rBV	2829699	2326363	32.44%	4.287%
12	12.683	1822	1827	1830	rBV	6869360	7171200	100.00%	13.215%
13	13.712	1998	2002	2006	rBV	2548561	2209466	30.81%	4.072%
14	15.077	2229	2234	2240	rBV	1883161	2294311	31.99%	4.228%


Sum of corrected areas: 54266226

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115278.D
Acq On : 28 Jun 2019 13:47
Operator : HP/JU
Sample : PB120984BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120984BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

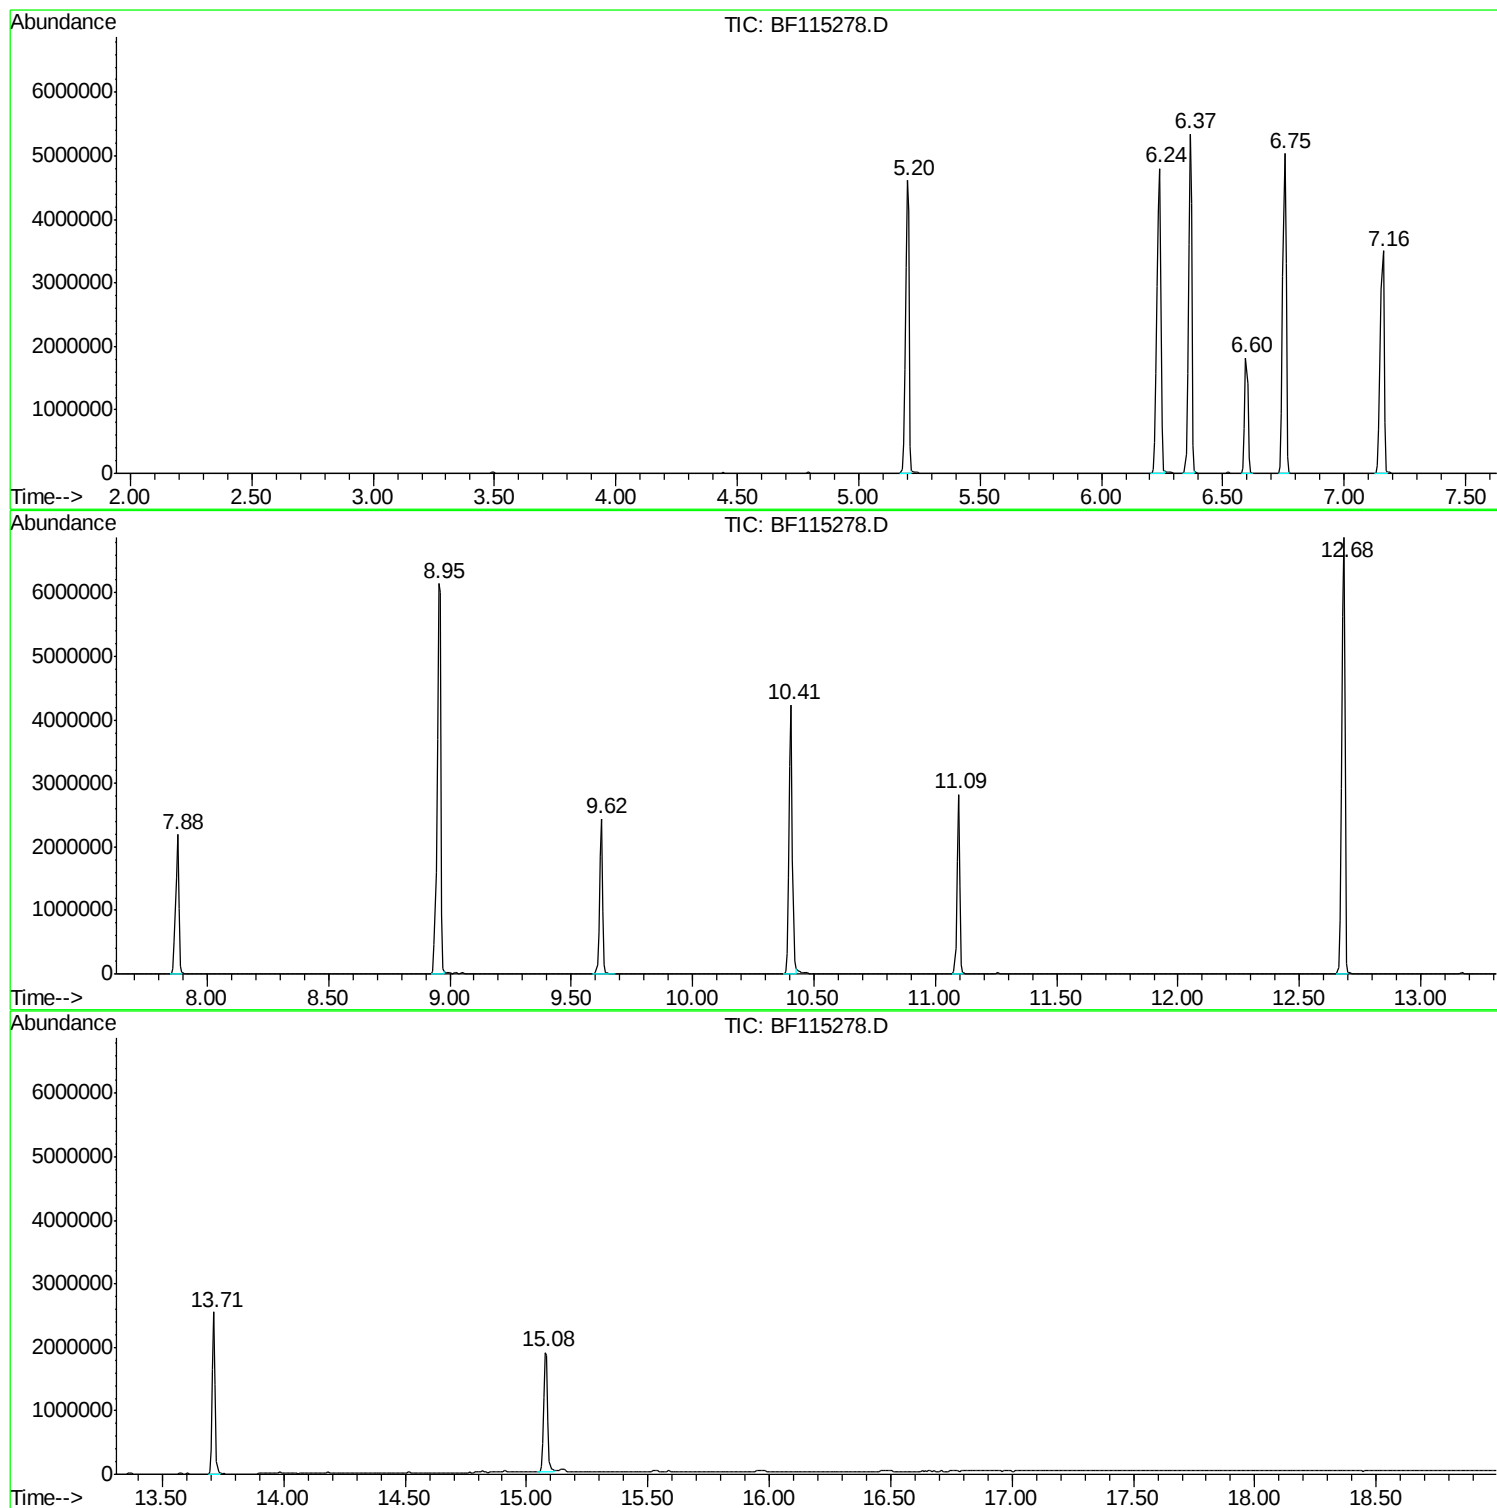

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115278.D
Acq On : 28 Jun 2019 13:47
Operator : HP/JU
Sample : PB120984BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120984BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.37	73.19 ng	5495010	1,4-Dichlorobenzene-d4	6.60

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

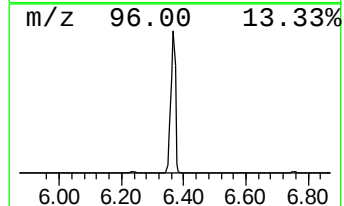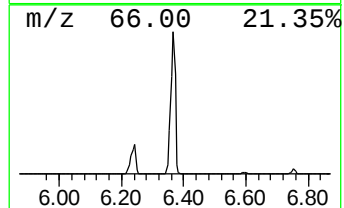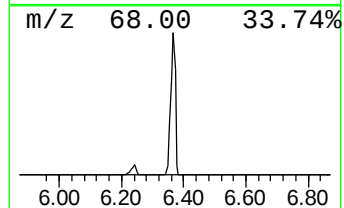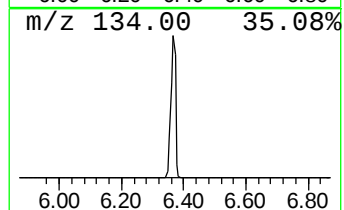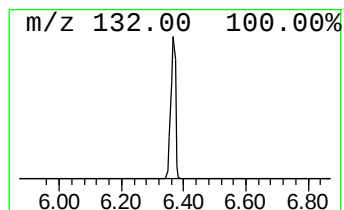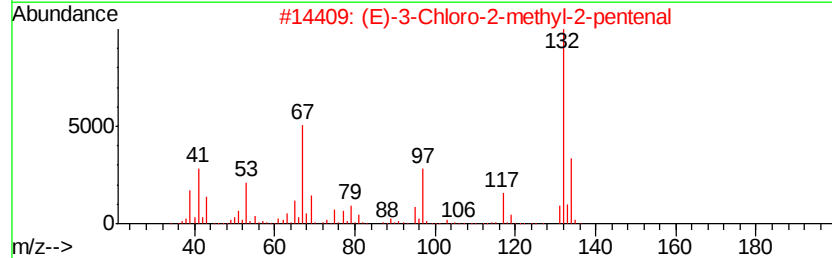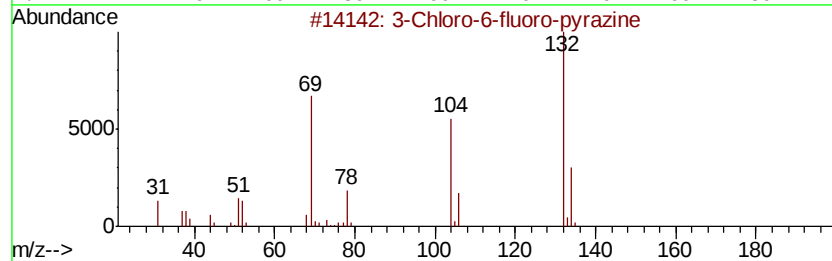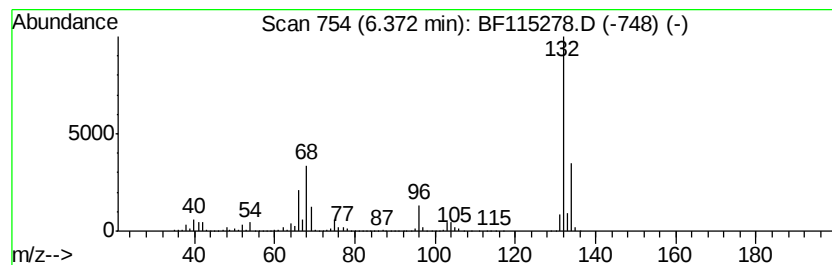

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
Data File : BF115278.D
Acq On : 28 Jun 2019 13:47
Operator : HP/JU
Sample : PB120984BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120984BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.37	6.37	73.2	ng	5495010	1	6.60	1501660	20.0