

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
 Data File : BF115280.D
 Acq On : 28 Jun 2019 14:40
 Operator : HP/JU
 Sample : PB120920BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB120920BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.201	549	555	558	rBV	4838028	5155459	75.16%	9.816%
2	6.242	725	732	734	rBV	4753164	5243295	76.44%	9.983%
3	6.366	748	753	756	rBV	5348288	5496484	80.13%	10.465%
4	6.595	789	792	796	rBV	1634879	1323007	19.29%	2.519%
5	6.754	815	819	822	rBV	5105191	4513496	65.80%	8.593%
6	7.160	882	888	891	rBV	3302050	3507018	51.13%	6.677%
7	7.877	1005	1010	1013	rBV	1920195	1695622	24.72%	3.228%
8	8.954	1188	1193	1197	rBV	6258687	6692405	97.56%	12.742%
9	9.624	1302	1307	1321	rVB	2043401	1964682	28.64%	3.741%
10	10.407	1435	1440	1443	rBV	4196908	3970407	57.88%	7.559%
11	11.095	1553	1557	1560	rBV	2490408	2064210	30.09%	3.930%
12	12.683	1822	1827	1830	rBV	6562247	6859522	100.00%	13.060%
13	13.712	1998	2002	2005	rBV	2237063	1946198	28.37%	3.705%
14	15.077	2228	2234	2243	rBV	1694416	2091230	30.49%	3.982%


Sum of corrected areas: 52523035

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115280.D
Acq On : 28 Jun 2019 14:40
Operator : HP/JU
Sample : PB120920BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120920BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

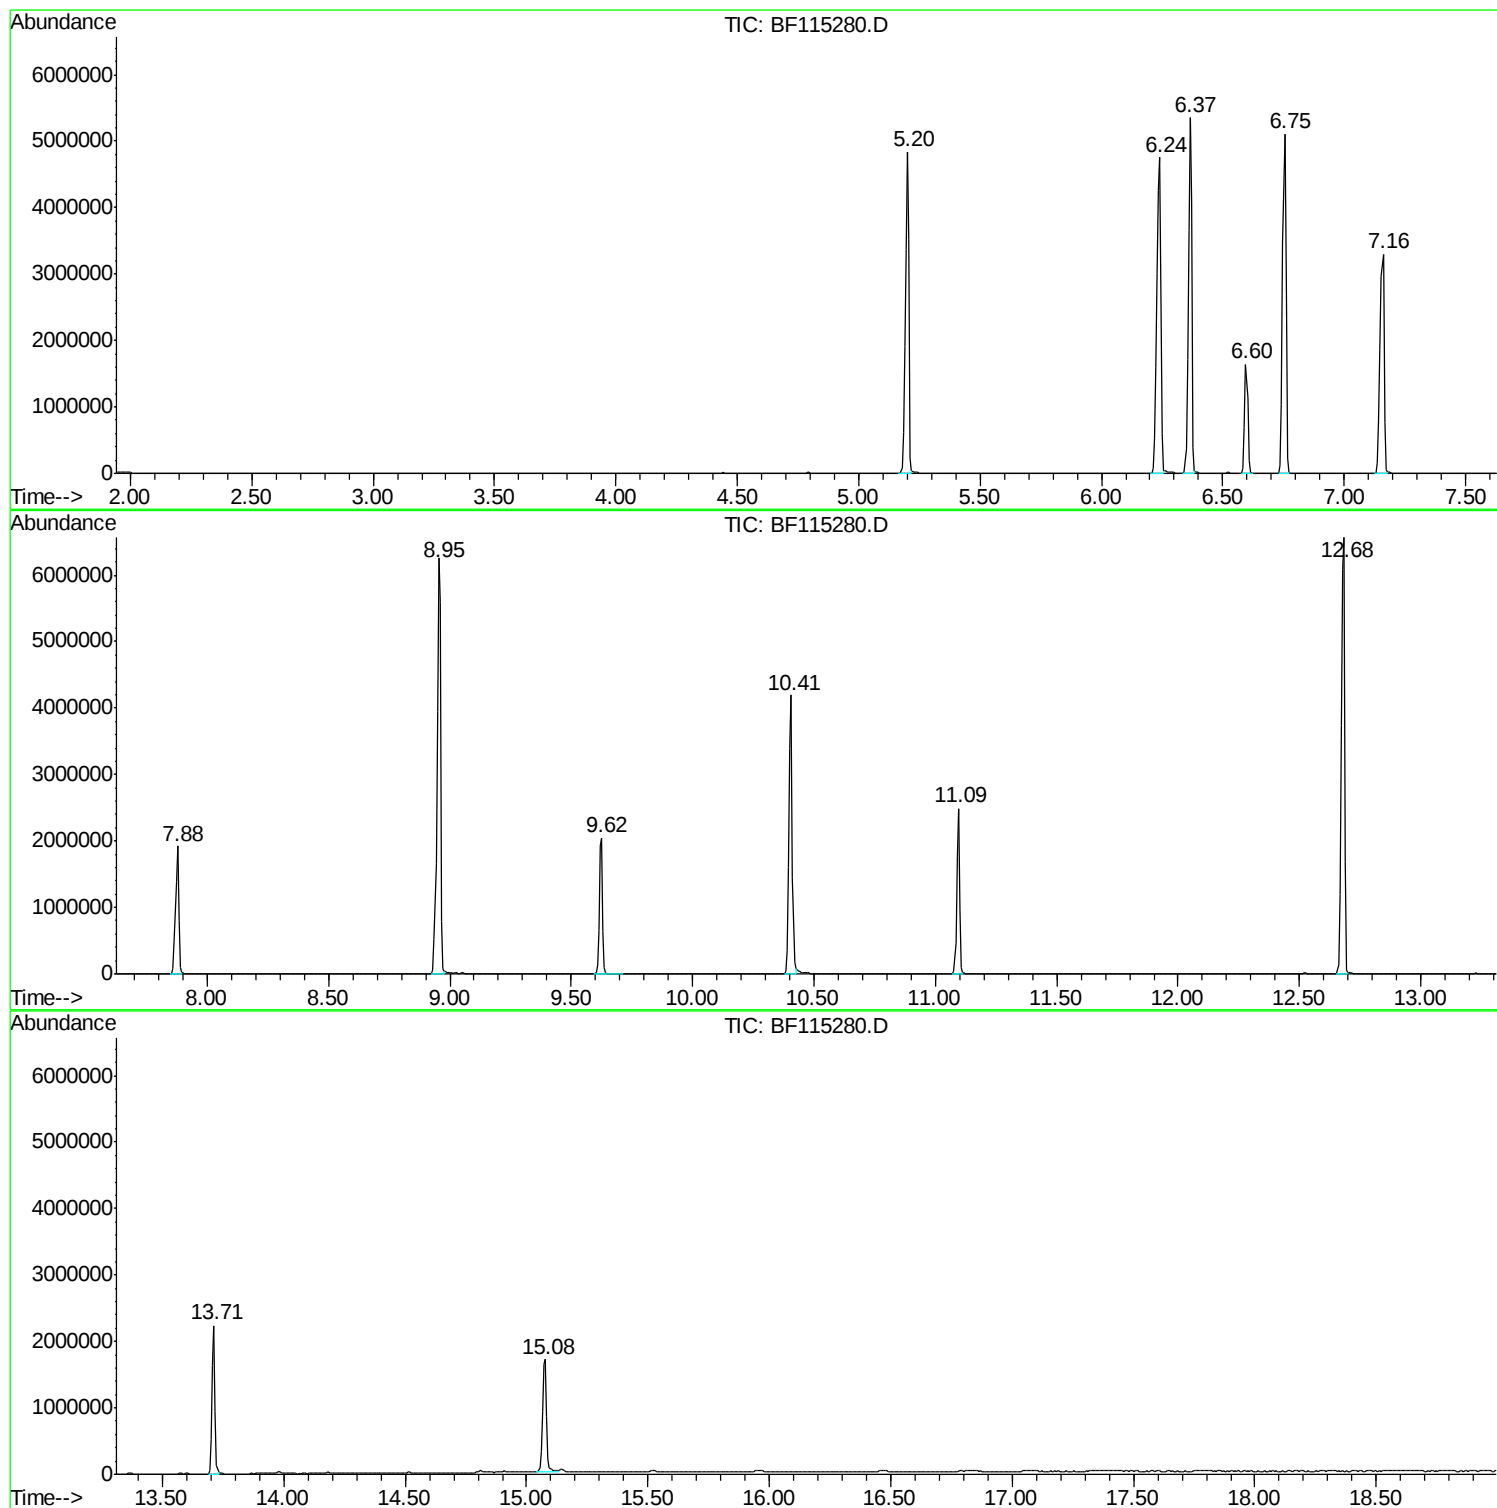

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062819\
Data File : BF115280.D
Acq On : 28 Jun 2019 14:40
Operator : HP/JU
Sample : PB120920BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120920BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.37	83.09 ng	5496480	1,4-Dichlorobenzene-d4	6.60

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

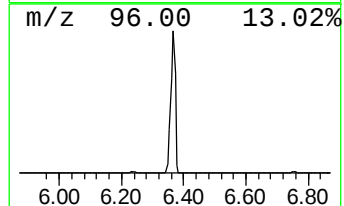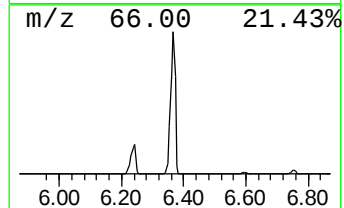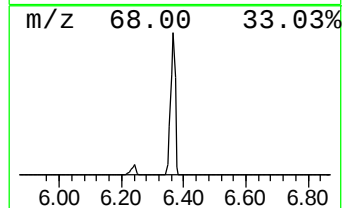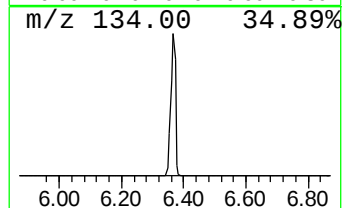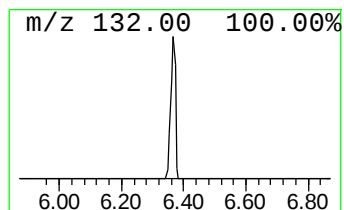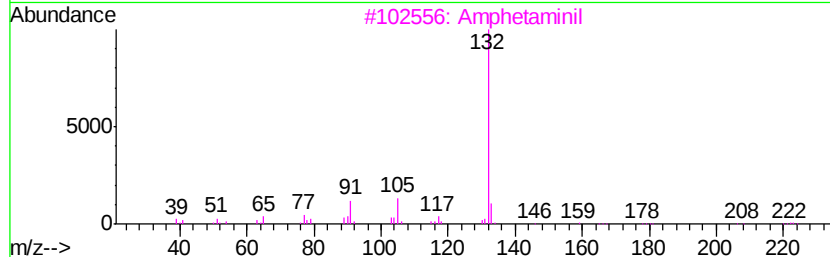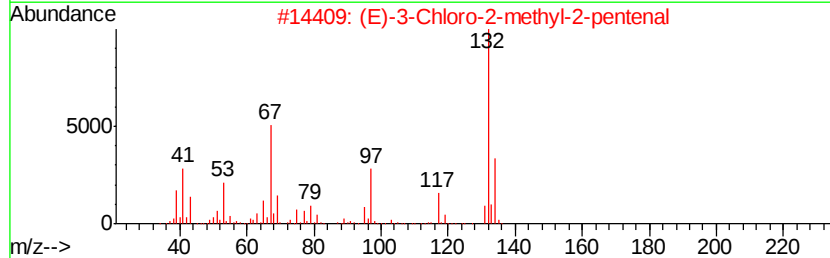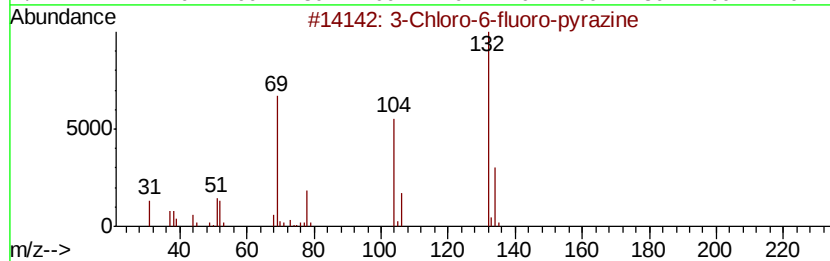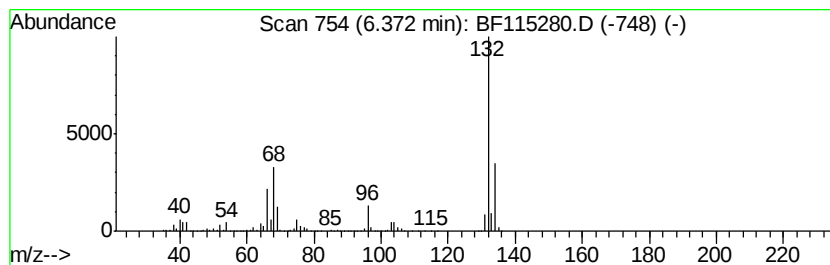

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
Data File : BF115280.D
Acq On : 28 Jun 2019 14:40
Operator : HP/JU
Sample : PB120920BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB120920BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.37	6.37	83.1	ng	5496480	1	6.60	1323010	20.0