


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
Data File : BF115265.D
Acq On : 28 Jun 2019 7:45
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 28 05:26:43 2019

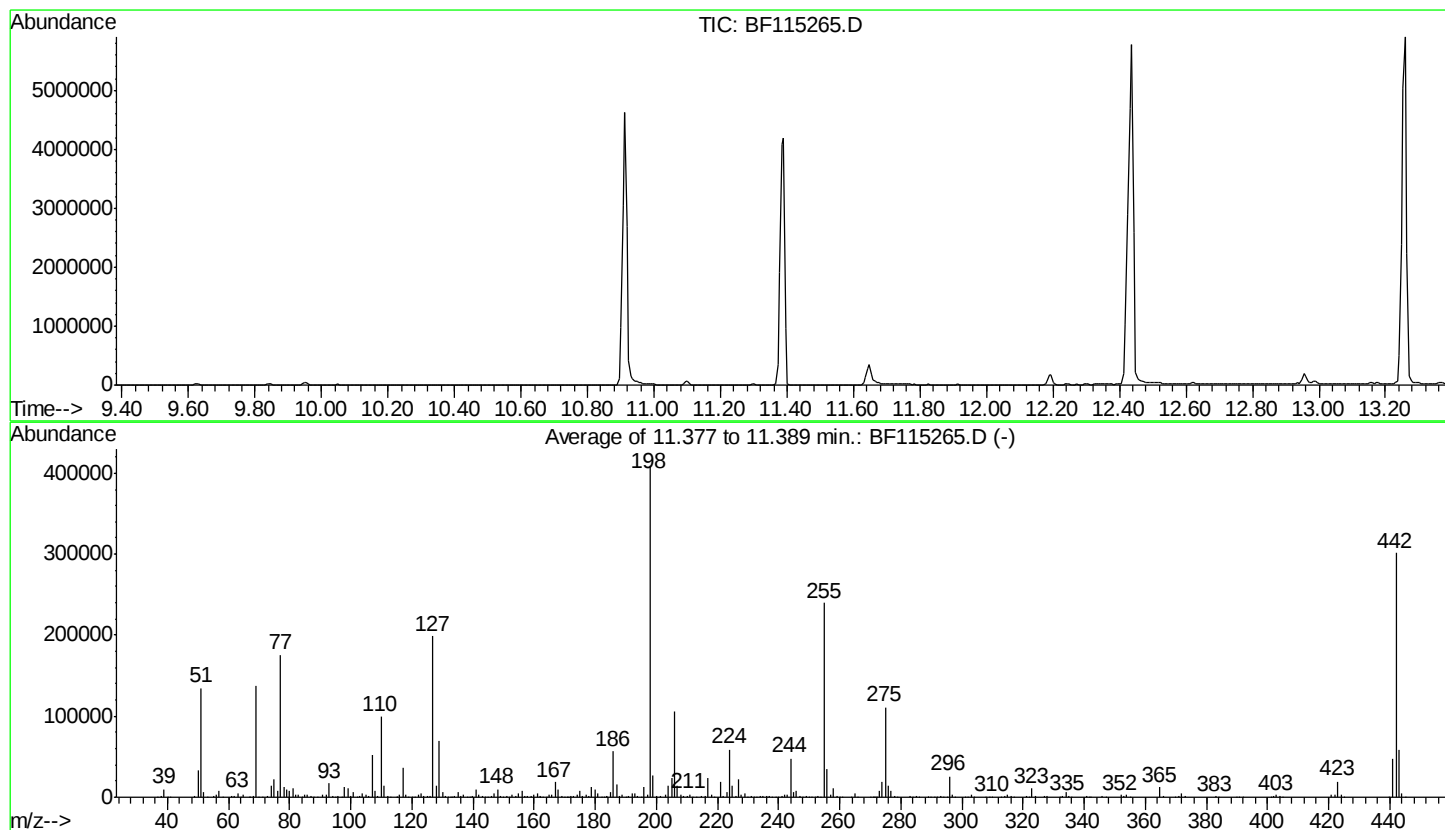

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	134624	PASS
68	69	0.00	2	1.7	2275	PASS
69	198	0.00	100	33.6	137688	PASS
70	69	0.00	2	0.5	710	PASS
127	198	10	80	48.5	198693	PASS
197	198	0.00	2	0.6	2559	PASS
198	198	100	100	100.0	409301	PASS
199	198	5	9	6.7	27348	PASS
275	198	10	60	27.0	110645	PASS
365	198	1	100	3.0	12378	PASS
441	198	0.01	100	11.7	47938	PASS
442	198	50	100	73.6	301210	PASS
443	442	15	24	19.3	58269	PASS