


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF062819\
 Data File : BF115282.D
 Acq On : 28 Jun 2019 15:33
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 05:26:43 2019

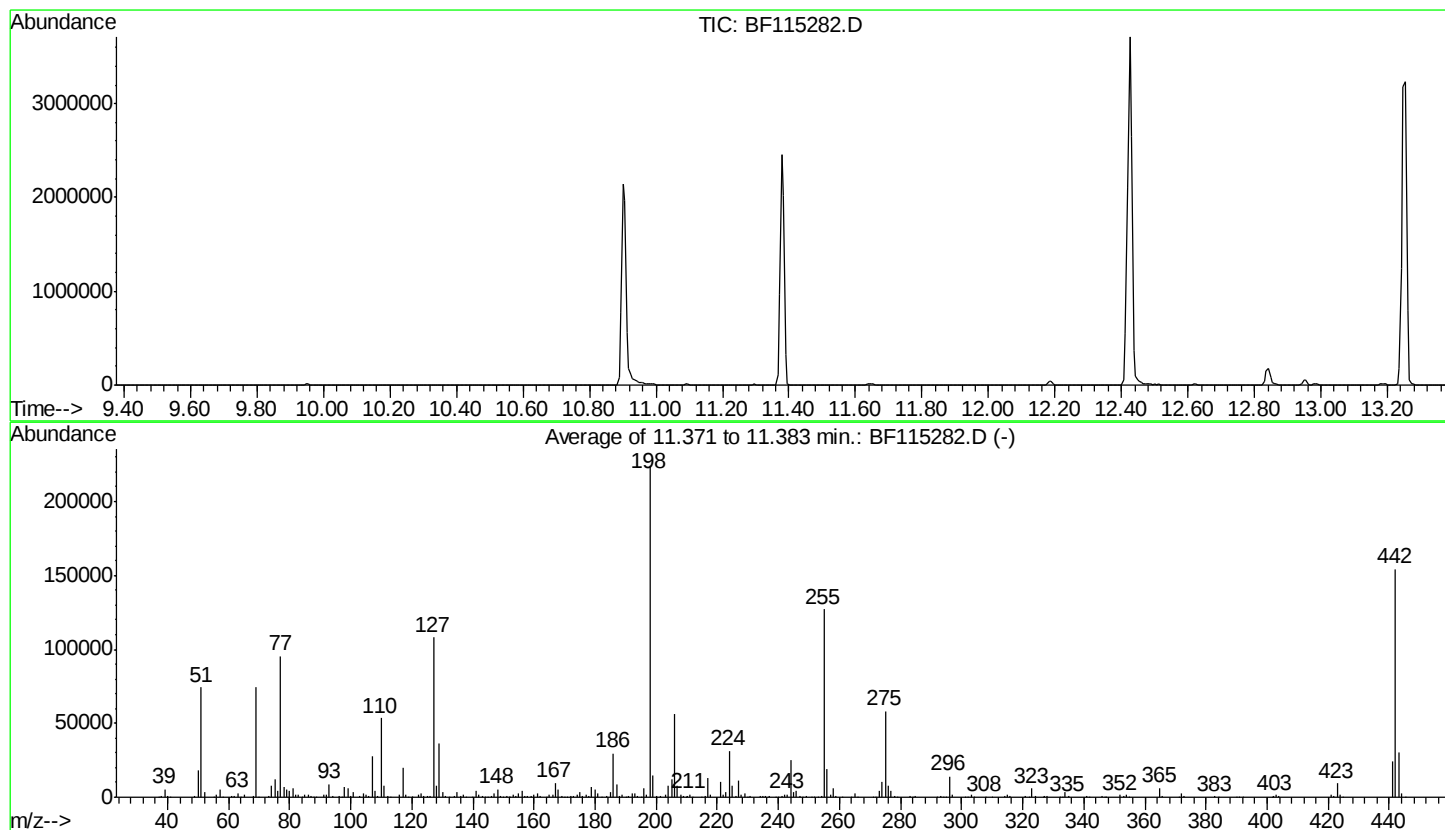

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	74416	PASS
68	69	0.00	2	1.6	1213	PASS
69	198	0.00	100	33.1	74149	PASS
70	69	0.00	2	0.6	422	PASS
127	198	10	80	48.3	108197	PASS
197	198	0.00	2	0.6	1388	PASS
198	198	100	100	100.0	224240	PASS
199	198	5	9	6.8	15152	PASS
275	198	10	60	25.9	58157	PASS
365	198	1	100	2.8	6254	PASS
441	198	0.01	100	10.6	23875	PASS
442	198	50	100	68.8	154170	PASS
443	442	15	24	19.5	30083	PASS