
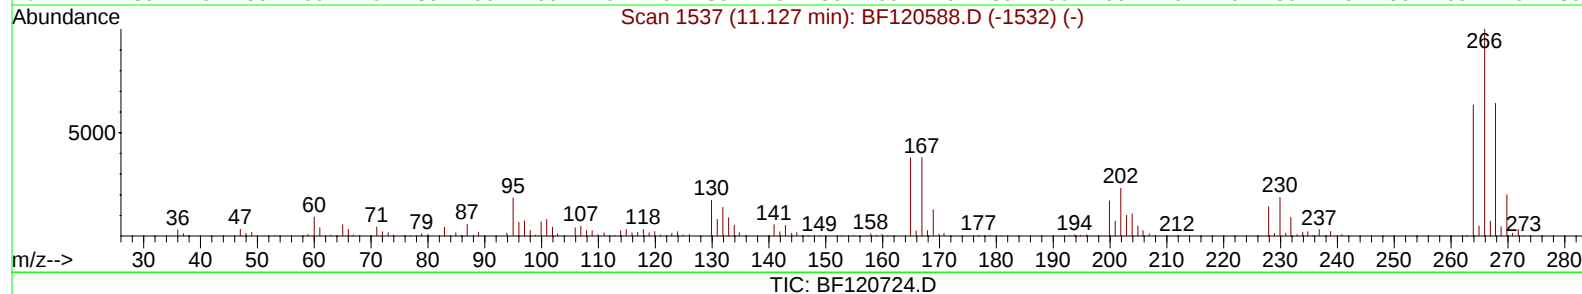
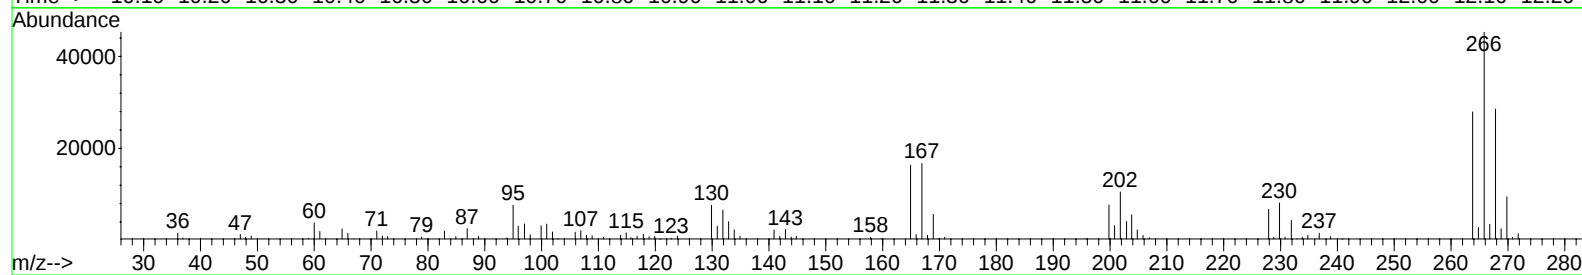


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062920\
Data File : BF120724.D
Acq On : 29 Jun 2020 13:01
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 18:51:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 29 15:30:14 2020
Response via : Initial Calibration

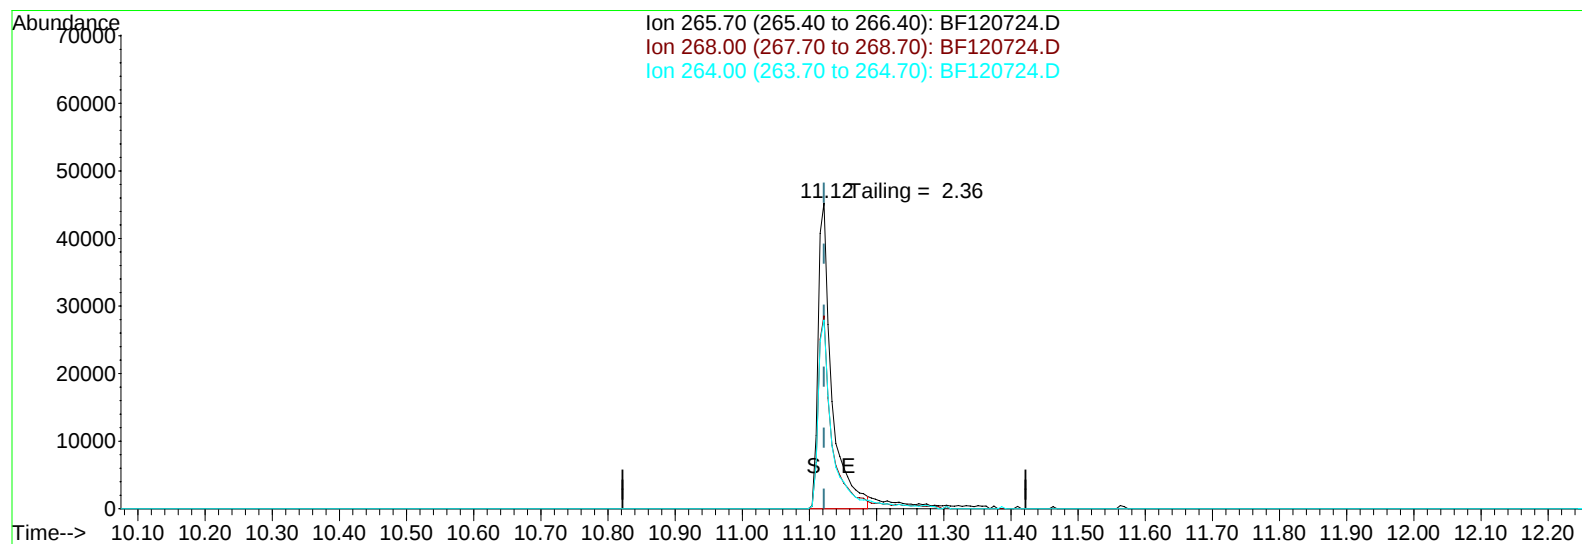

(70) Pentachlorophenol (C)




11.122min (-0.000) 30822.15ng

response 68165

Ion	Exp%	Act%
265.70	100	100
268.00	64.70	63.07
264.00	64.10	61.68
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062920\
 Data File : BF120724.D
 Acq On : 29 Jun 2020 13:01
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 18:51:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 29 15:30:14 2020
 Response via : Initial Calibration

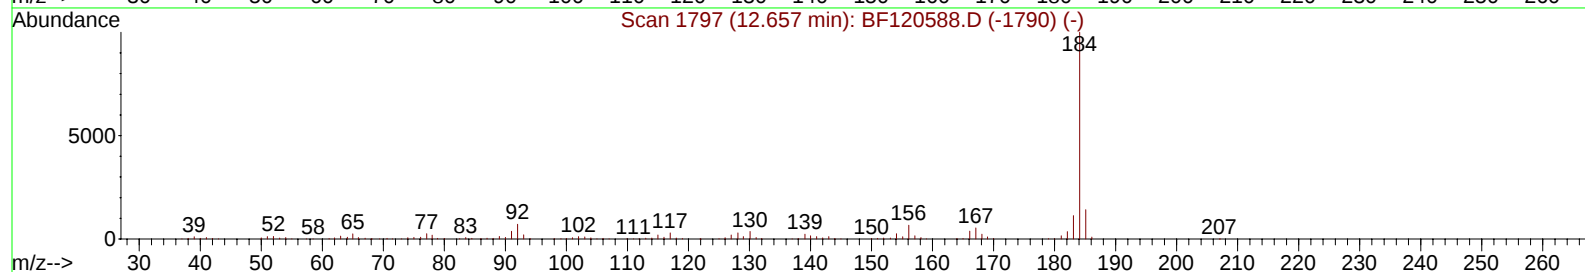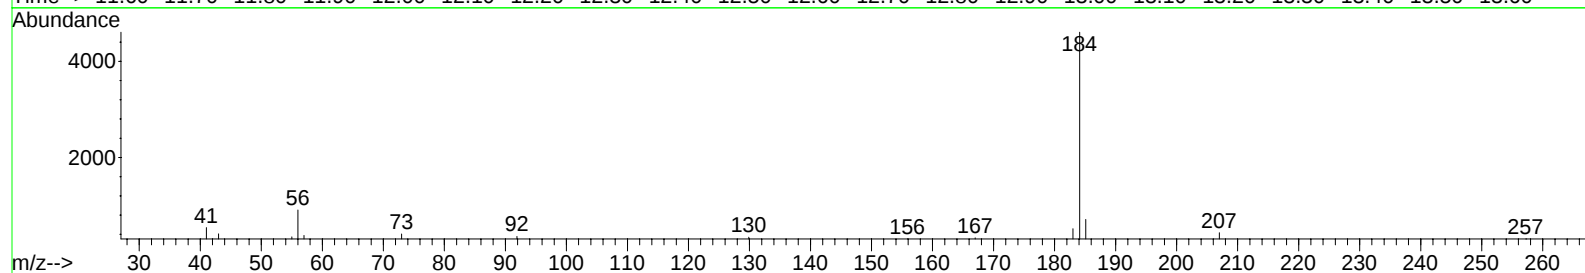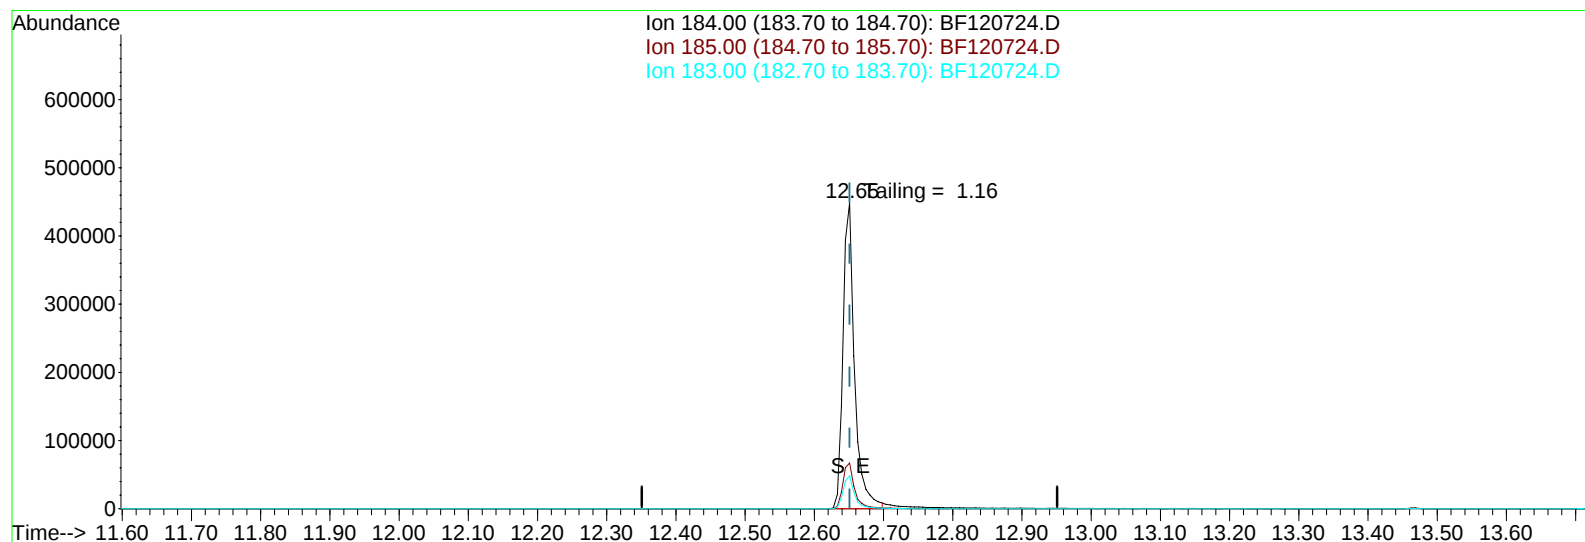

(77) Benzidine

12.710min (+0.059) 0.00ng m

response 1626

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	20.60#
183.00	10.70	8.85
0.00	0.00	0.00