

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062920\
 Data File : BF120746.D
 Acq On : 29 Jun 2020 23:57
 Operator : JU/CG
 Sample : L3114-02RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VNJ-242RE

Quant Time: Jun 30 03:19:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 29 15:30:14 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	148845	20.00	ng	0.00
21) Naphthalene-d8	8.08	136	230851	20.00	ng	0.00
39) Acenaphthene-d10	9.83	164	120319	20.00	ng	0.00
64) Phenanthrene-d10	11.32	188	217031	20.00	ng	0.00
76) Chrysene-d12	13.96	240	171857	20.00	ng	0.00
86) Perylene-d12	15.40	264	332215	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	883454	101.76	ng	0.08
7) Phenol-d6	6.50	99	823165	76.13	ng	0.08
23) Nitrobenzene-d5	7.36	82	404669	97.98	ng	0.00
42) 2,4,6-Tribromophenol	10.63	330	197377	141.10	ng	0.02
45) 2-Fluorobiphenyl	9.16	172	822409	104.58	ng	0.00
79) Terphenyl-d14	12.91	244	849456	109.18	ng	0.01
Target Compounds						
50) Dimethylphthalate	9.55	163	92775	10.706	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF062920\
Data File : BF120746.D
Acq On : 29 Jun 2020 23:57
Operator : JU/CG
Sample : L3114-02RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VNJ-242RE

Quant Time: Jun 30 03:19:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 29 15:30:14 2020
Response via : Initial Calibration

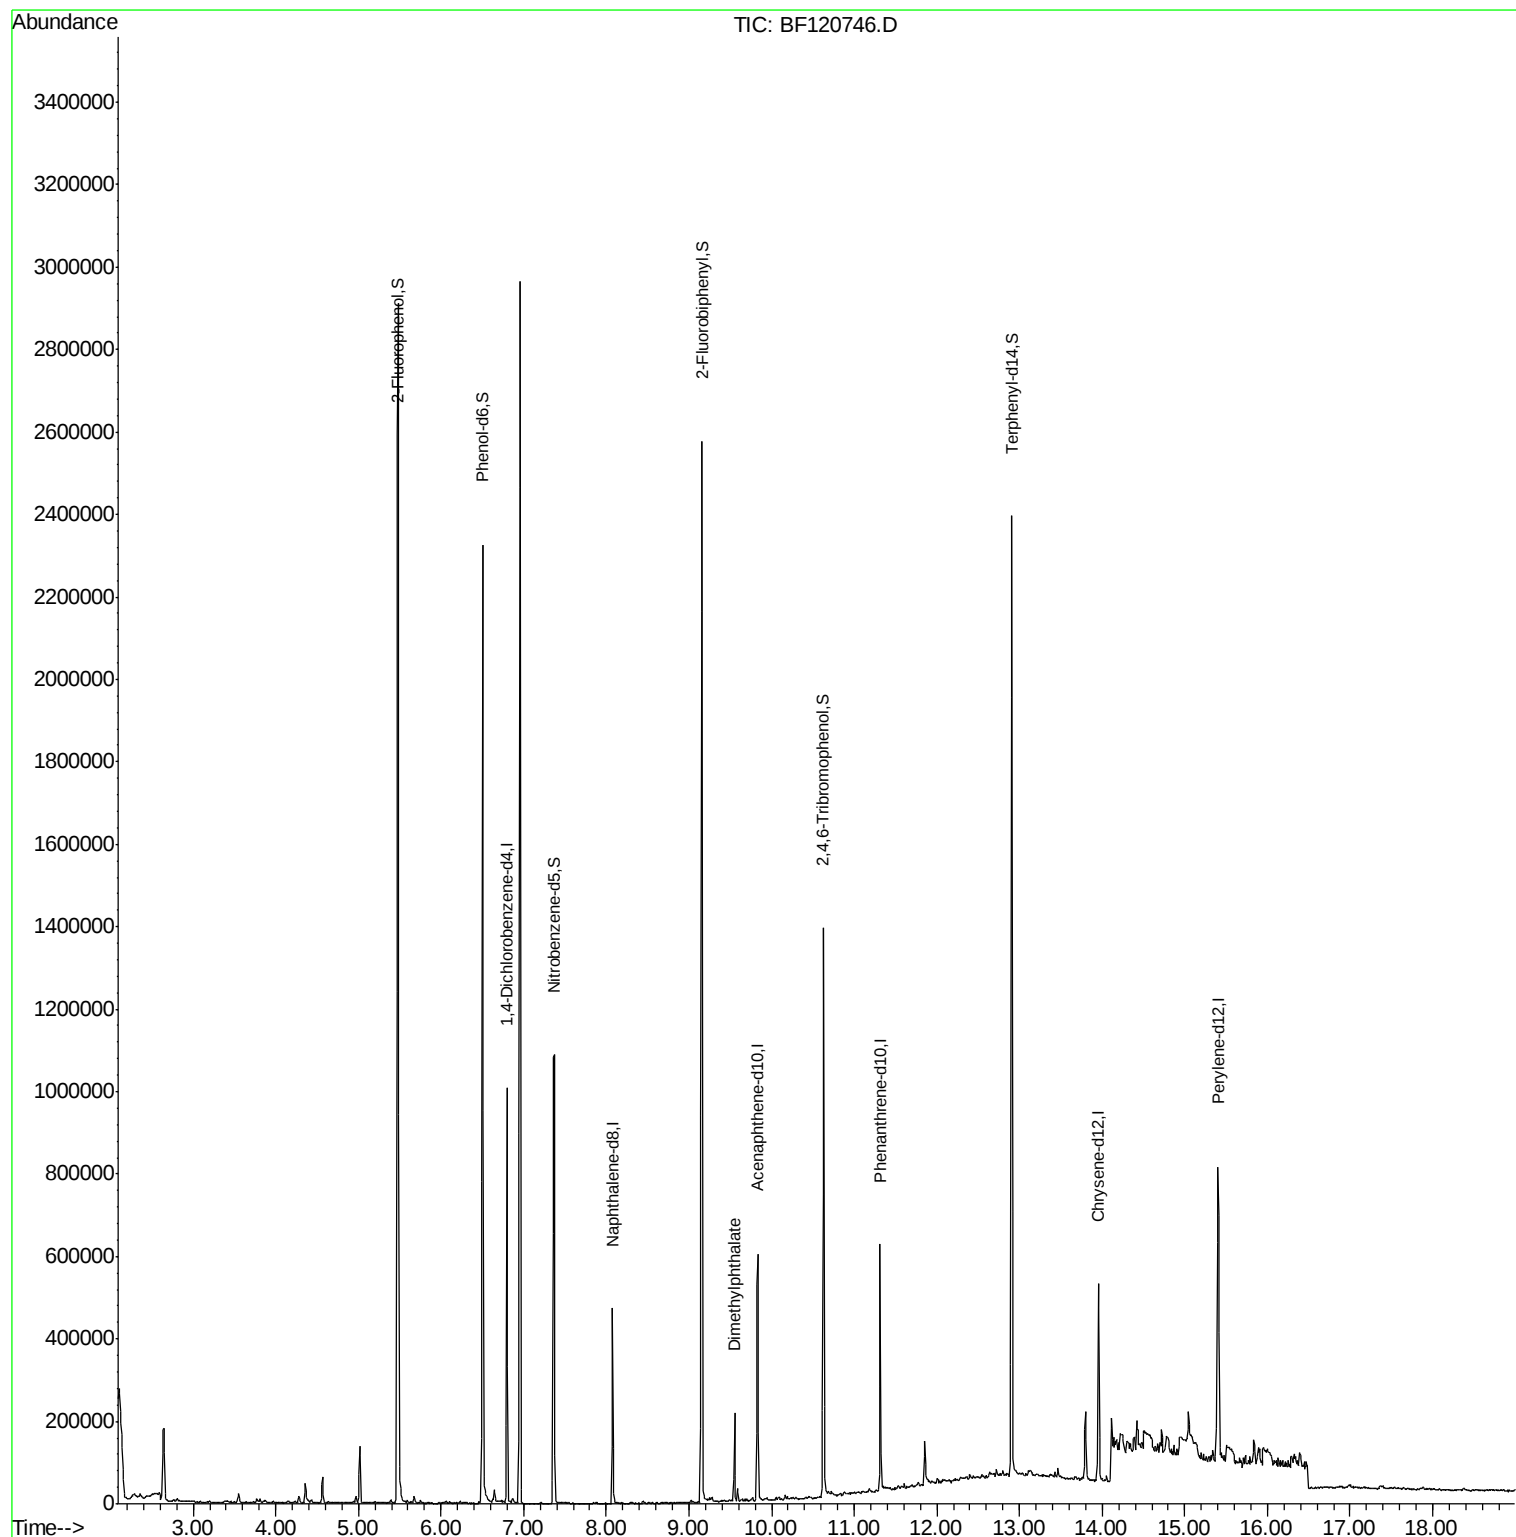

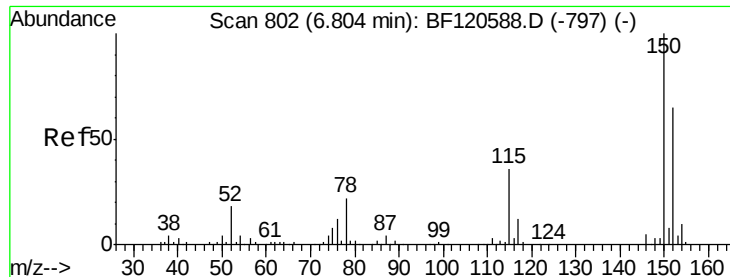


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.80 min Scan# 801
Delta R.T. 0.01 min
Lab File: BF120746.D
Acq: 29 Jun 2020 23:57

Instrument :
BNA_F
ClientSampleId :
VNJ-242RE

Tot Ion:152 Resp: 148845
Ion Ratio Lower Upper
152 100
150 154.7 124.6 187.0
115 57.1 44.2 66.4

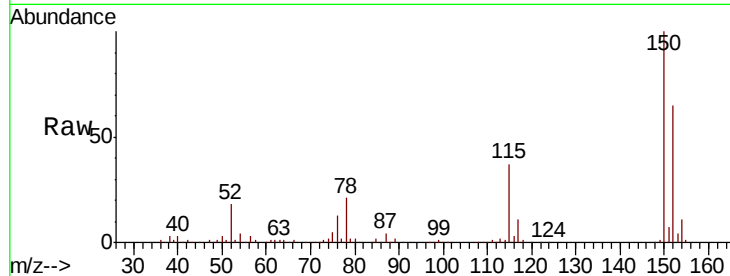


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

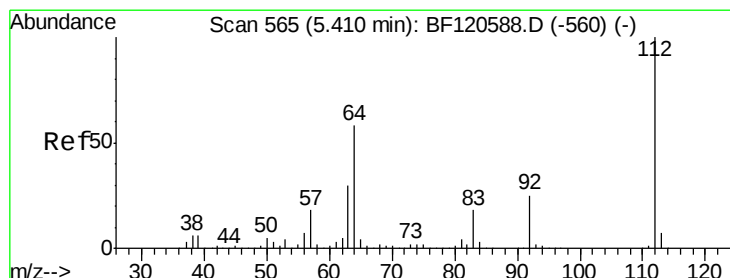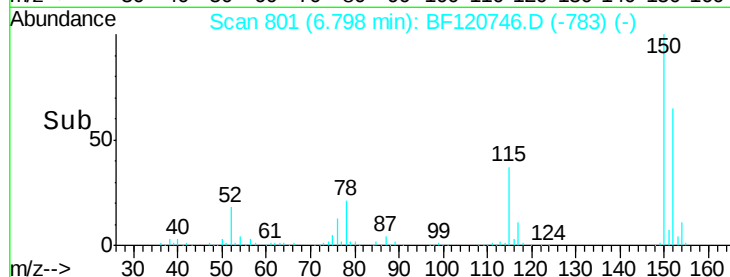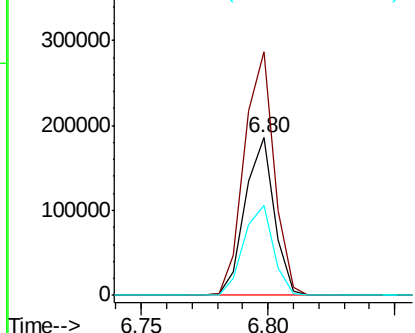



#5


2-Fluorophenol
Concen: 101.760 ng
RT: 5.48 min Scan# 577
Delta R.T. 0.08 min
Lab File: BF120746.D
Acq: 29 Jun 2020 23:57

Tgt Ion:112 Resp: 883454
Ion Ratio Lower Upper
112 100
64 54.4 42.2 63.2
63 28.5 21.7 32.5

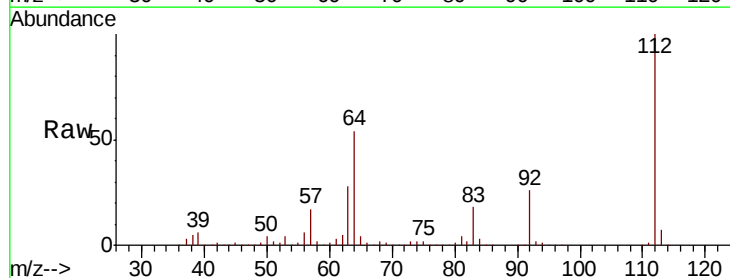

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

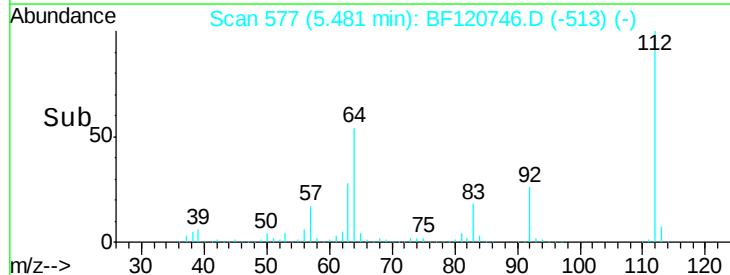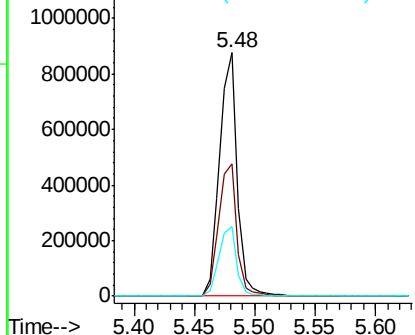

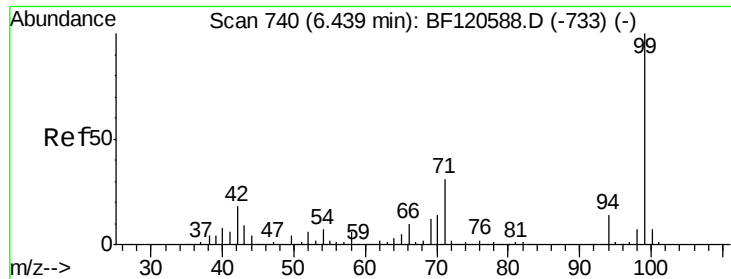

#7

Phenol-d6

Concen: 76.126 ng

RT: 6.50 min Scan# 751

Delta R.T. 0.08 min

Lab File: BF120746.D

Acq: 29 Jun 2020 23:57

Instrument :

BNA_F

ClientSampled :

VNJ-242RE


Tot Ion: 99 Resp: 823165

Ion Ratio Lower Upper




99 100

42 17.9 14.2 21.4

71 34.1 25.4 38.2

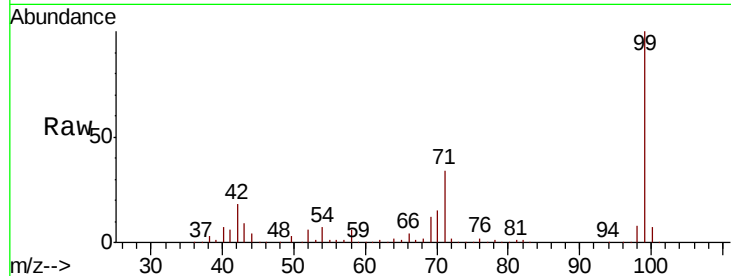

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

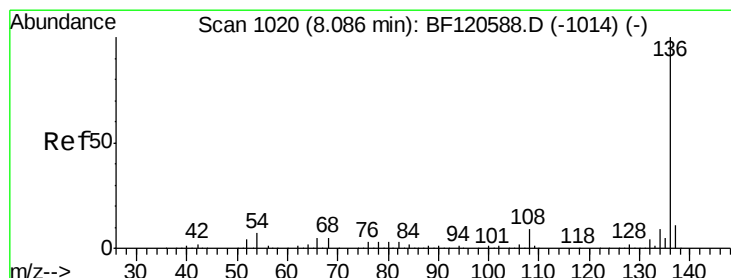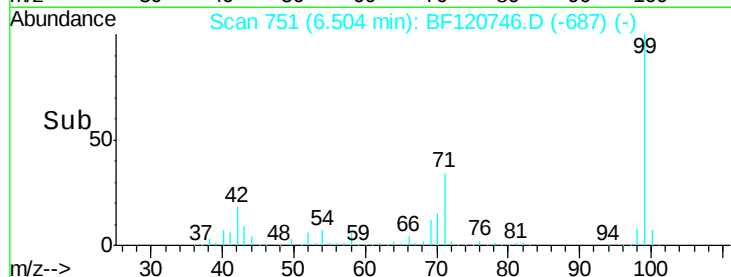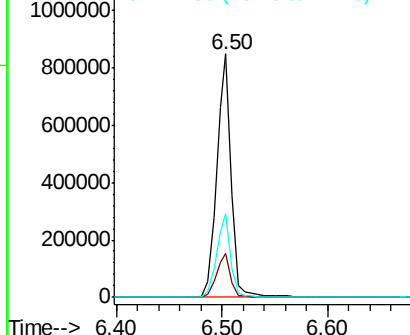

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.08 min Scan# 1019

Delta R.T. 0.01 min

Lab File: BF120746.D

Acq: 29 Jun 2020 23:57

Tgt Ion: 136 Resp: 230851


Ion Ratio Lower Upper

136 100



137 10.9 8.6 12.8


54 5.5 5.3 7.9

68 4.3 4.3 6.5#

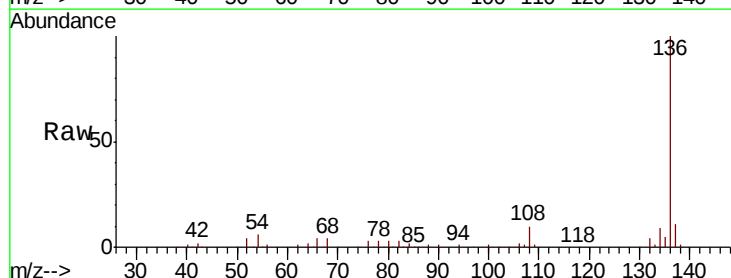

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



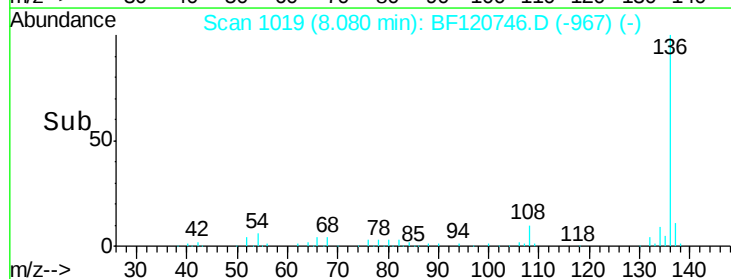
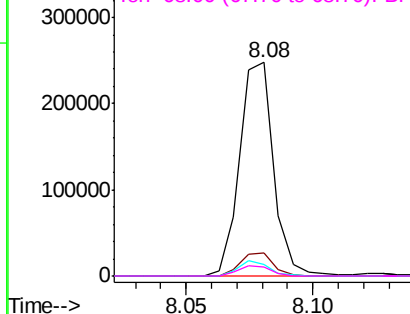


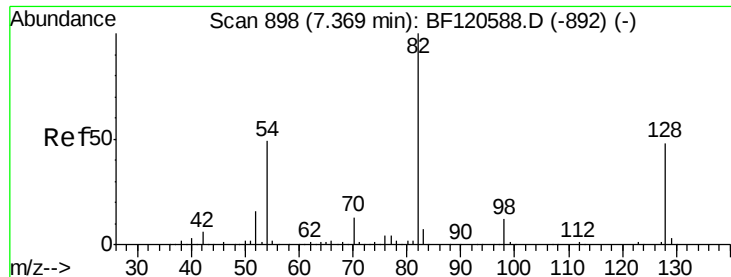

#23
Nitrobenzene-d5
Concen: 97.984 ng
RT: 7.36 min Scan# 897
Delta R.T. 0.01 min
Lab File: BF120746.D
Acq: 29 Jun 2020 23:57




Instrument :
BNA_F
ClientSampleId :
VNJ-242RE


Tot Ion	82	Resp	404669
Ion Ratio	100	Lower	Upper
128	44.2	38.1	57.1
54	49.3	38.8	58.2

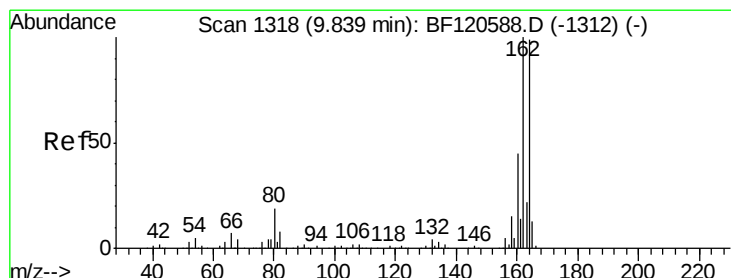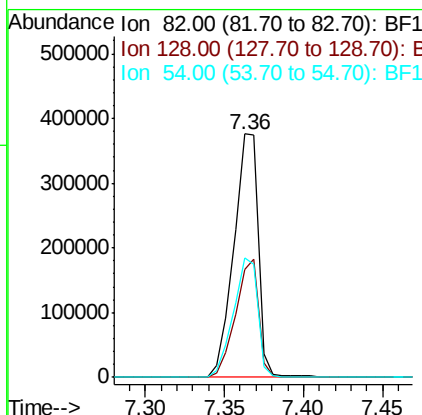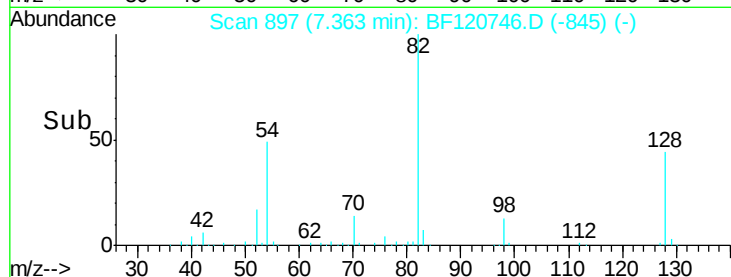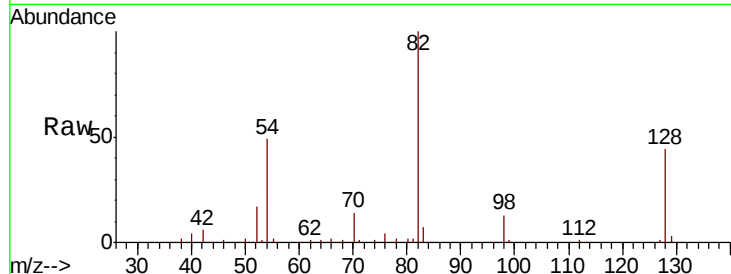

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.83 min Scan# 1317
Delta R.T. 0.01 min
Lab File: BF120746.D
Acq: 29 Jun 2020 23:57

Tgt Ion	164	Resp	120319
Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td>	100	Lower	Upper
162	103.3	81.4	122.0
160	45.7	36.6	55.0


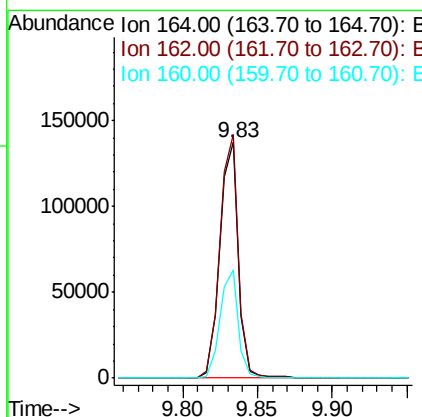
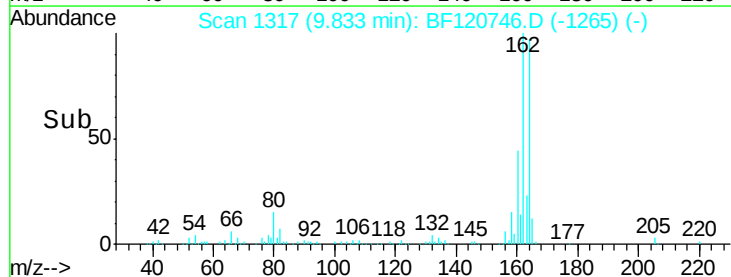
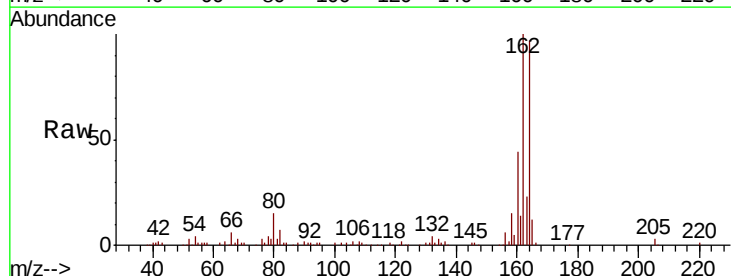


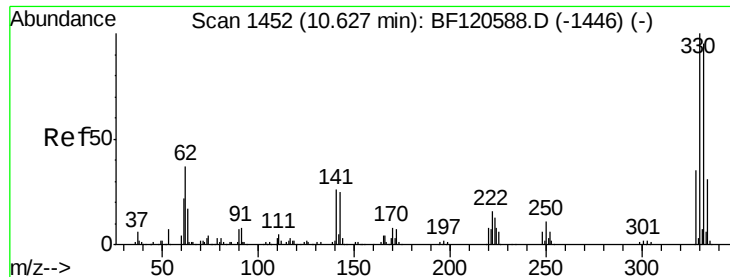

#42
 2,4,6-Tribromophenol
 Concen: 141.097 ng
 RT: 10.63 min Scan# 1453
 Delta R.T. 0.02 min
 Lab File: BF120746.D
 Acq: 29 Jun 2020 23:57




Instrument :
 BNA_F
 ClientSampled :
 VNJ-242RE


Tot Ion	Ratio	Lower	Upper
330	100		
332	94.8	76.4	114.6
141	30.6	23.0	34.6

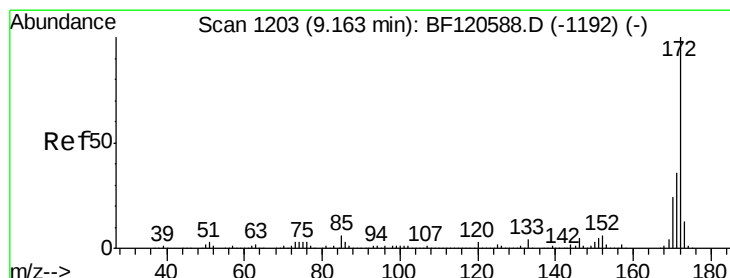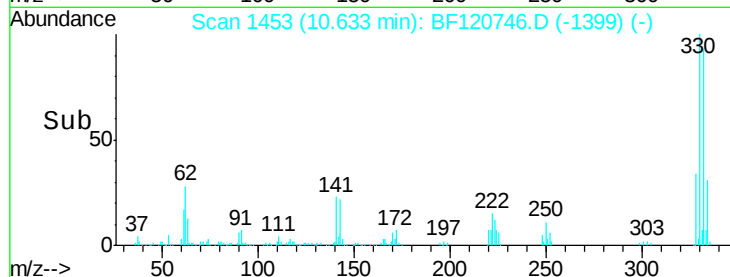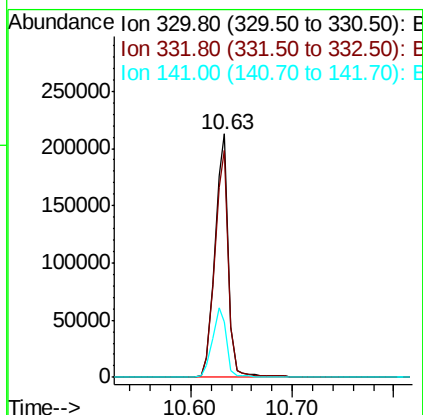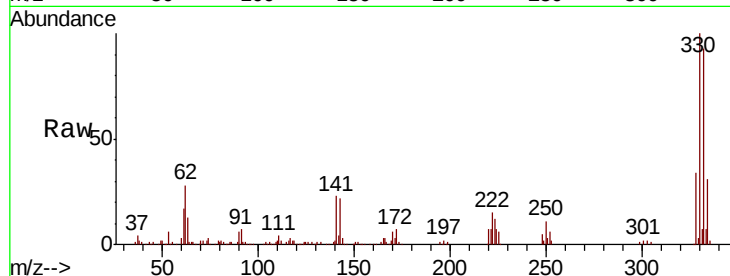

#45
 2-Fluorobiphenyl
 Concen: 104.578 ng
 RT: 9.16 min Scan# 1202
 Delta R.T. 0.01 min
 Lab File: BF120746.D
 Acq: 29 Jun 2020 23:57

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	28.6	43.0
170	23.5	19.1	28.7

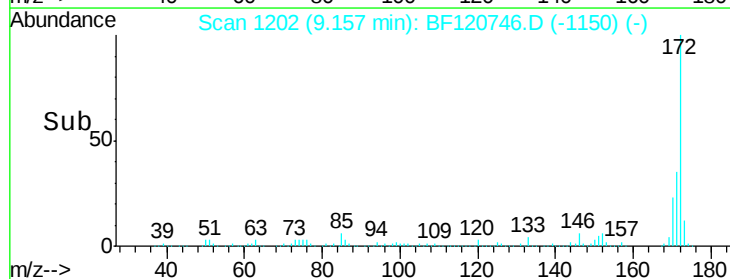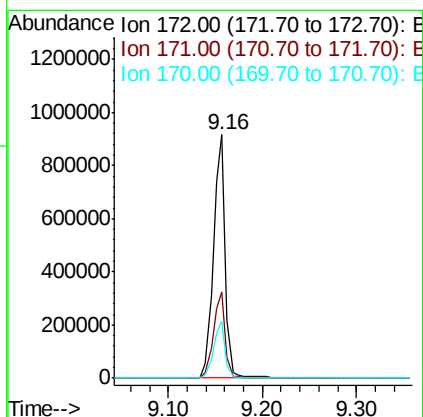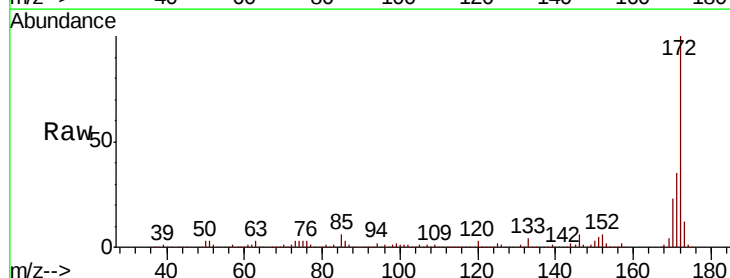

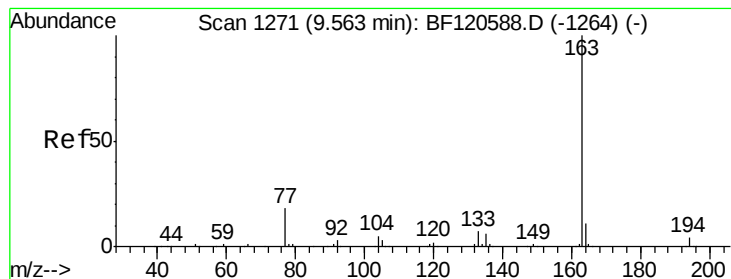

#50

Dimethylphthalate

Concen: 10.706 ng

RT: 9.55 min Scan# 1269

Delta R.T. -0.00 min

Lab File: BF120746.D

Acq: 29 Jun 2020 23:57

Instrument :

BNA_F

ClientSampleId :

VNJ-242RE


Tot Ion:163 Resp: 92775

Ion Ratio Lower Upper

163 100

194 3.8 3.0 4.6




164 9.8 8.2 12.2

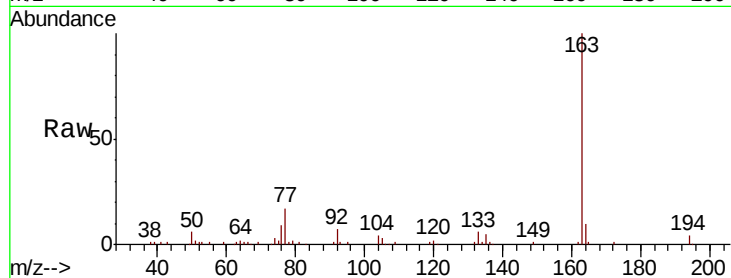

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

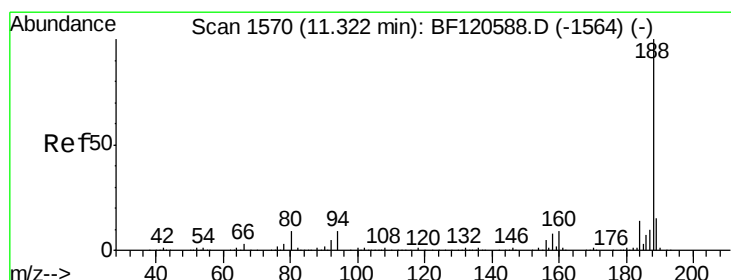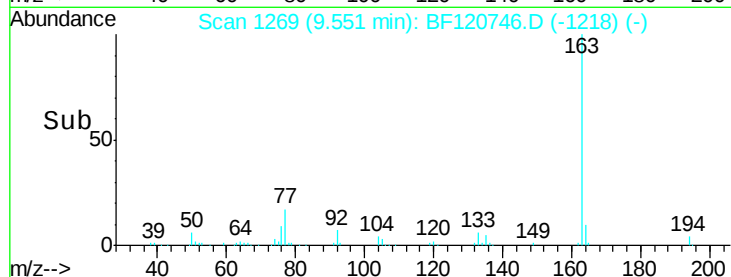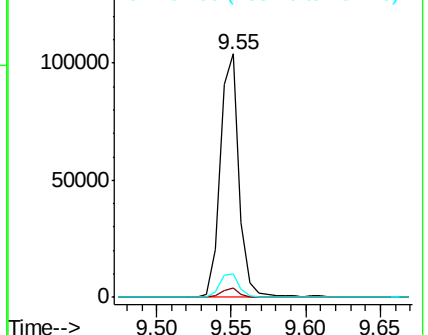

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.32 min Scan# 1569

Delta R.T. 0.01 min

Lab File: BF120746.D

Acq: 29 Jun 2020 23:57


Tgt Ion:188 Resp: 217031

Ion Ratio Lower Upper

188 100

94 8.1 7.5 11.3



80 9.0 7.7 11.5

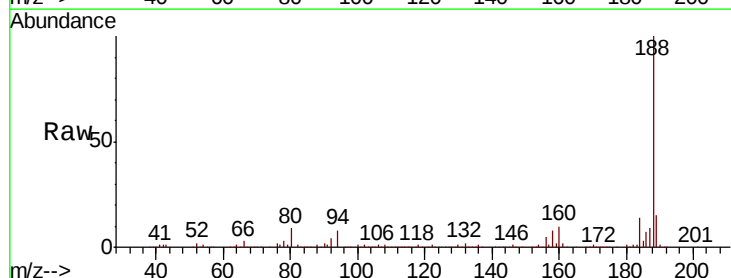


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1



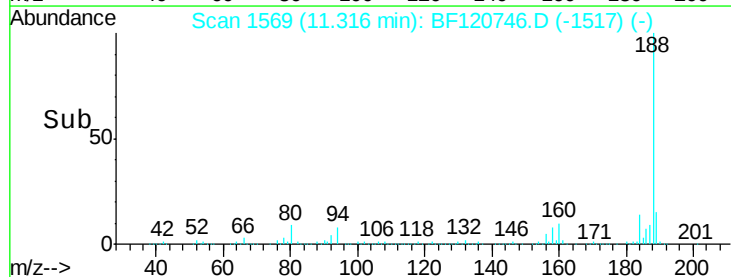
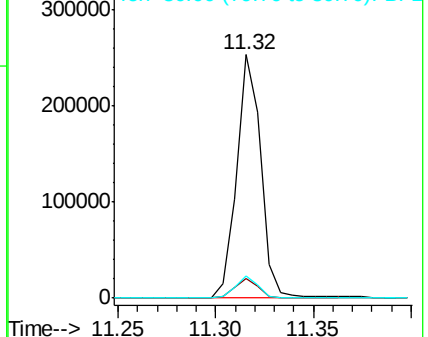


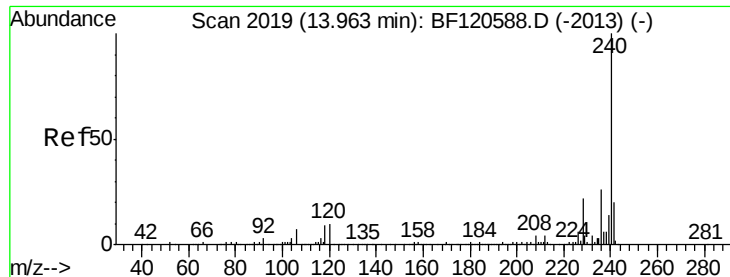

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.96 min Scan# 2018
 Delta R.T. -0.00 min
 Lab File: BF120746.D
 Acq: 29 Jun 2020 23:57




Instrument :
 BNA_F
 ClientSampleID :
 VNJ-242RE


Tot Ion:240 Resp: 171857
 Ion Ratio Lower Upper
 240 100
 120 10.2 7.6 11.4
 236 24.7 21.0 31.4

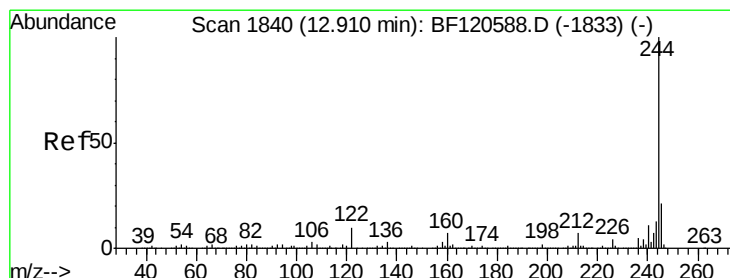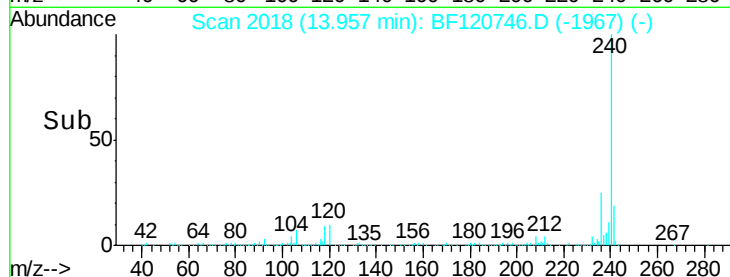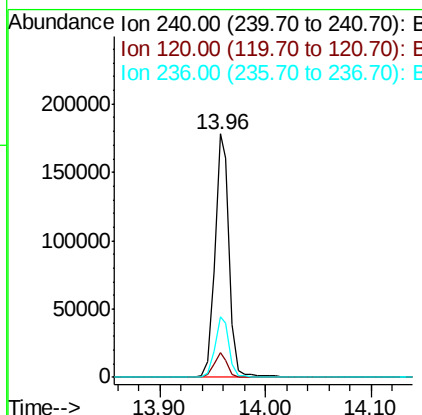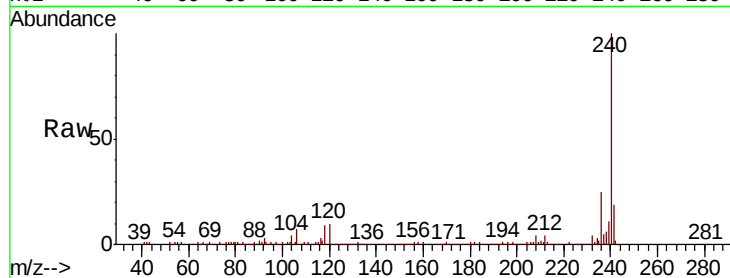

#79
 Terphenyl-d14
 Concen: 109.181 ng
 RT: 12.91 min Scan# 1840
 Delta R.T. 0.01 min
 Lab File: BF120746.D
 Acq: 29 Jun 2020 23:57

Tgt Ion:244 Resp: 849456
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.6 8.4
 122 9.8 8.8 13.2

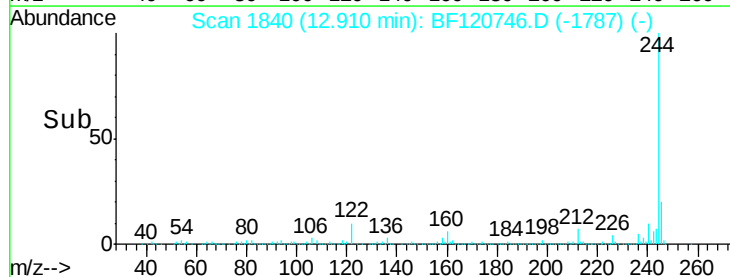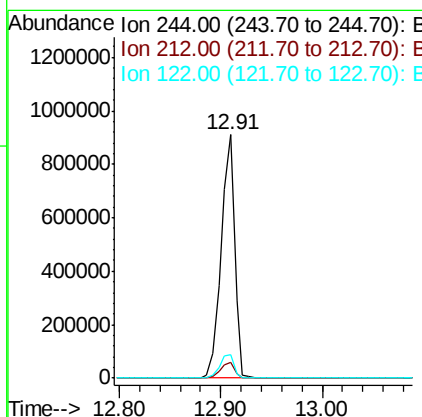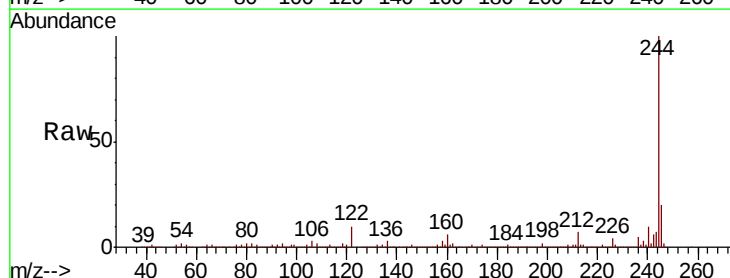


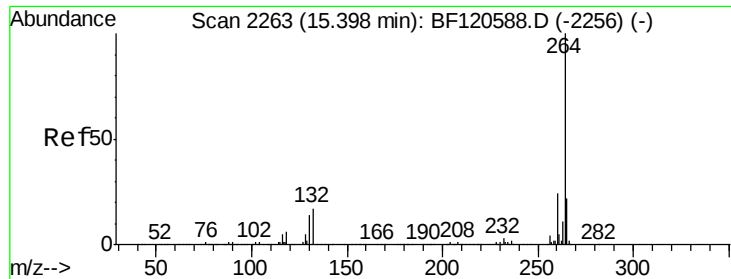

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.40 min Scan# 2264
Delta R.T. 0.01 min
Lab File: BF120746.D
Acq: 29 Jun 2020 23:57

Instrument :
BNA_F
ClientSampleId :
VNJ-242RE

Tot Ion:	264	Resp:	332215
Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.4	29.2
265	21.8	17.4	26.0

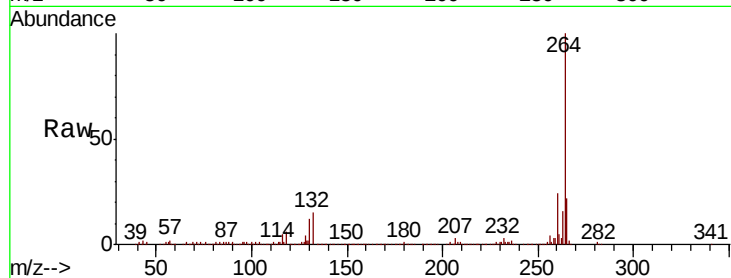

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

