


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF062920\
 Data File : BF120724.D
 Acq On : 29 Jun 2020 13:01
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 29 15:30:14 2020

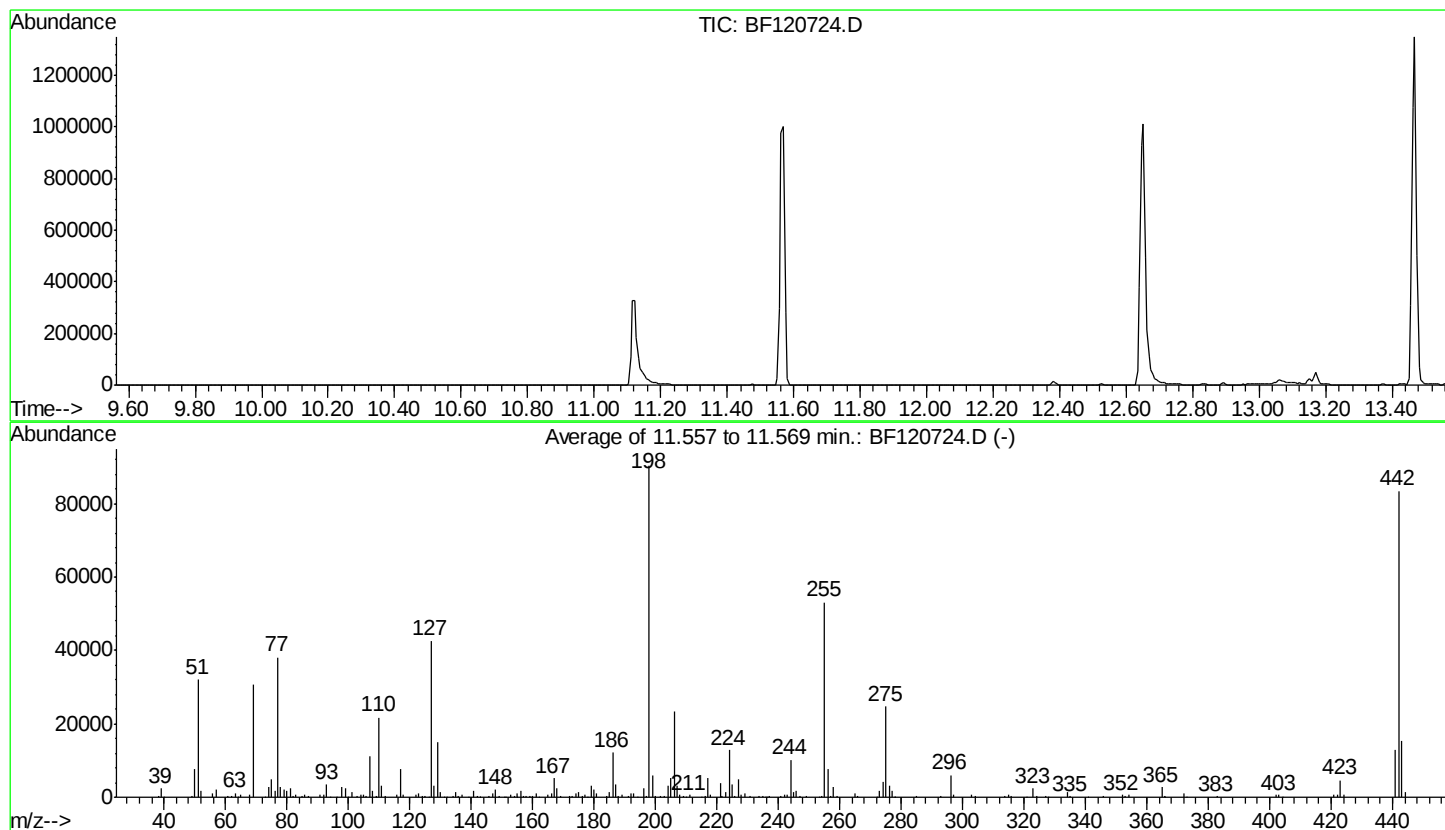

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	32080	PASS
68	69	0.00	2	1.9	565	PASS
69	198	0.00	100	33.8	30536	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.2	42600	PASS
197	198	0.00	2	0.2	219	PASS
198	198	100	100	100.0	90338	PASS
199	198	5	9	6.6	5986	PASS
275	198	10	60	27.3	24694	PASS
365	198	1	100	2.9	2651	PASS
441	198	0.01	100	14.4	13046	PASS
442	198	50	100	92.4	83486	PASS
443	442	15	24	18.4	15348	PASS