
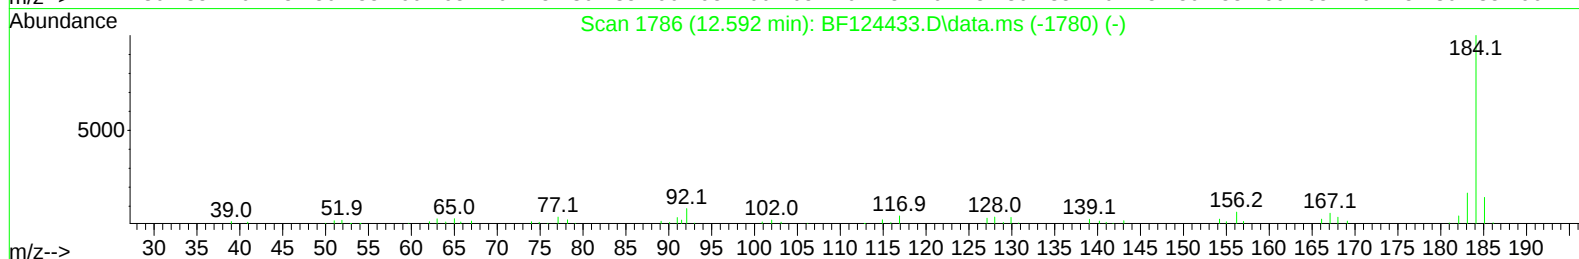
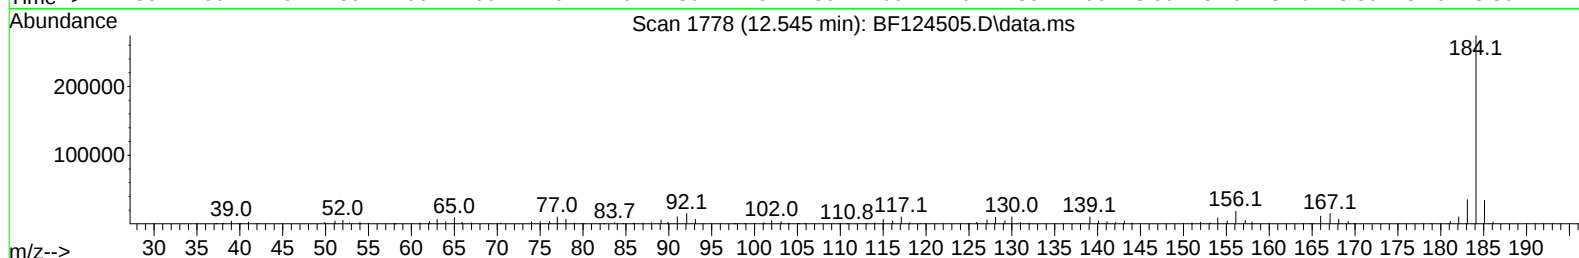


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070121\
 Data File : BF124505.D
 Acq On : 1 Jul 2021 11:28
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 14:12:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 29 12:49:33 2021
 Response via : Initial Calibration

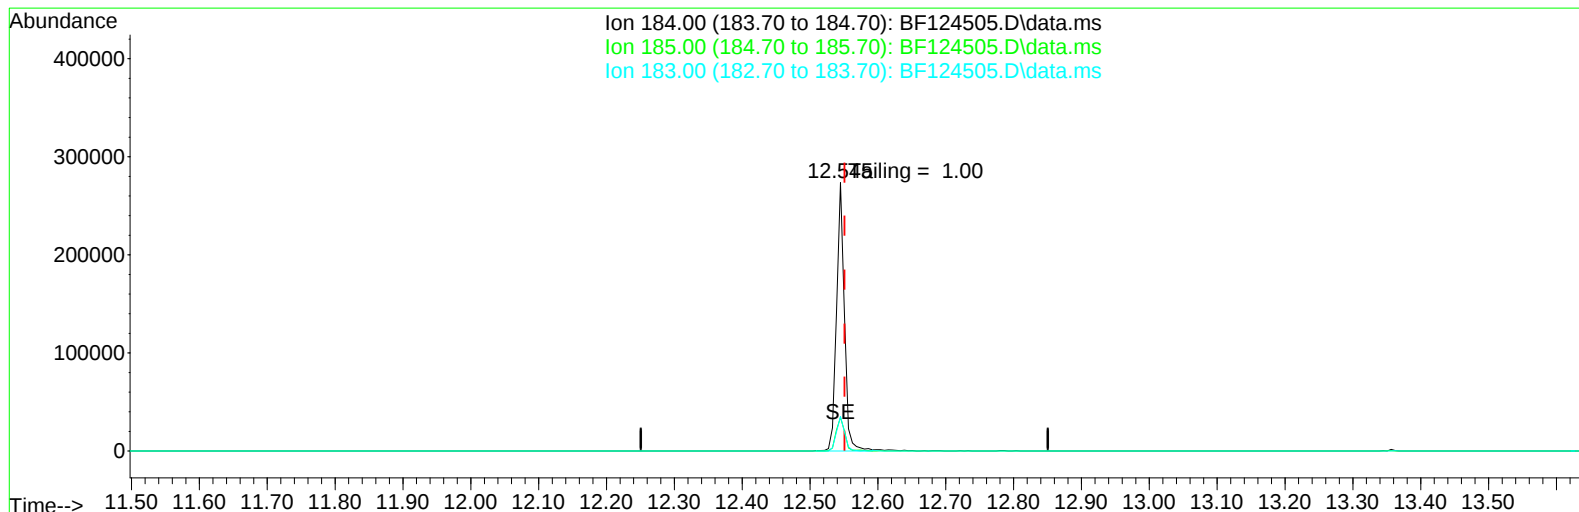

TIC: BF124505.D\data.ms

(77) Benzidine




12.545min (-0.006) 0.00 ng

response 222913

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	12.51
183.00	9.80	12.90#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070121\
Data File : BF124505.D
Acq On : 1 Jul 2021 11:28
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 14:12:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 29 12:49:33 2021
Response via : Initial Calibration

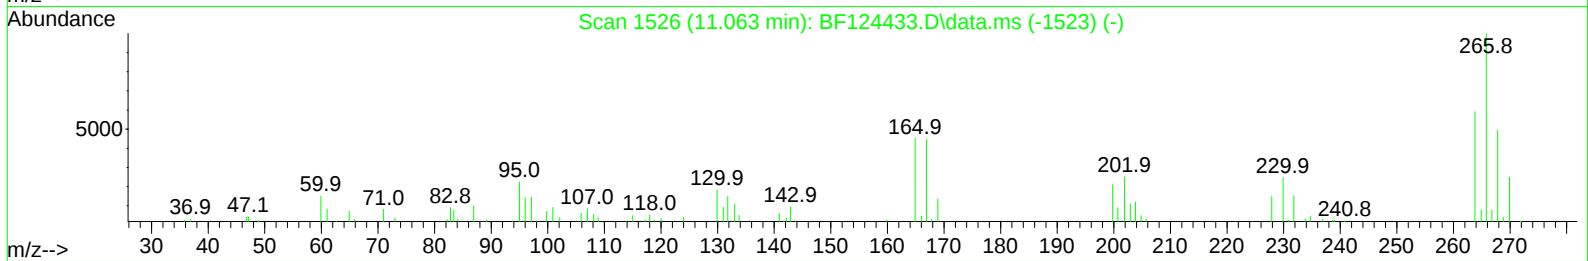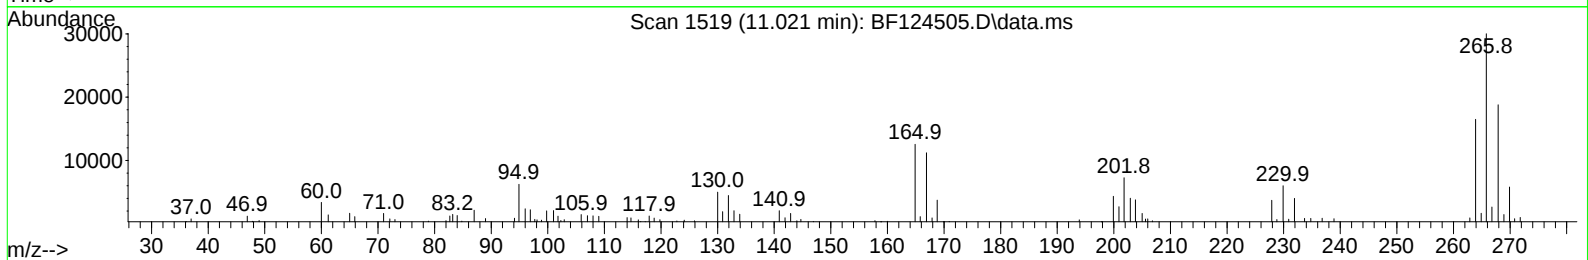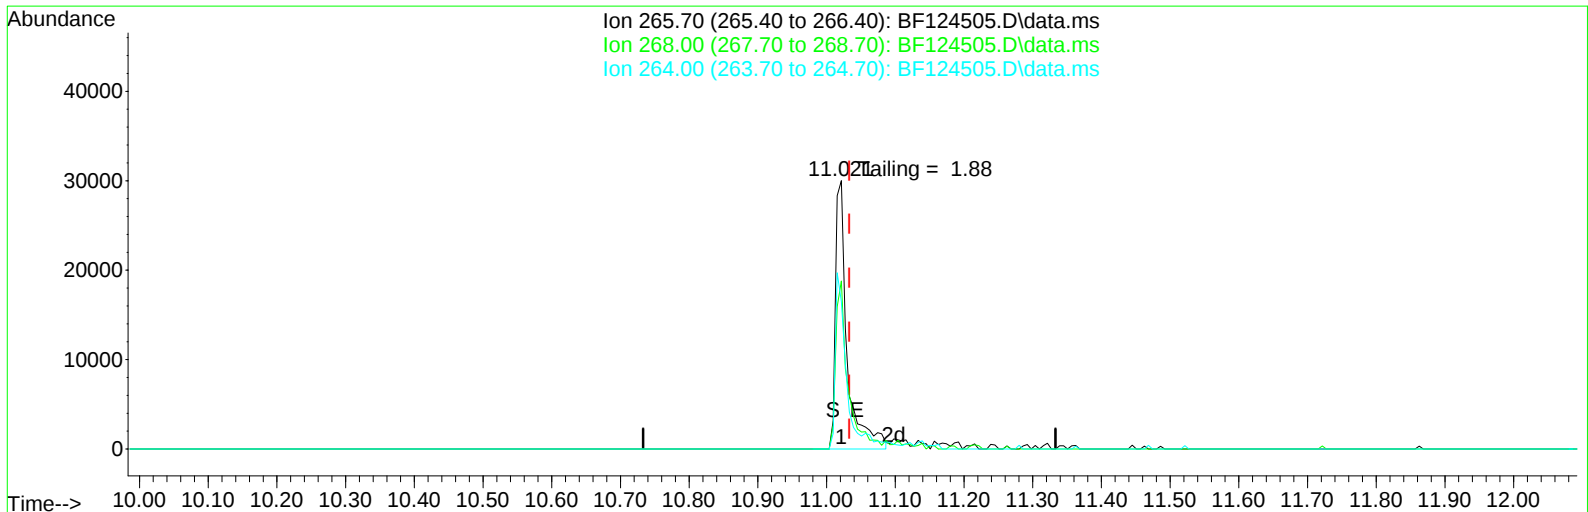

TIC: BF124505.D\data.ms

(70) Pentachlorophenol (C)

11.021min (-0.012) 21073.46 ng

response 35905

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.61
264.00	65.70	54.96
0.00	0.00	0.00