
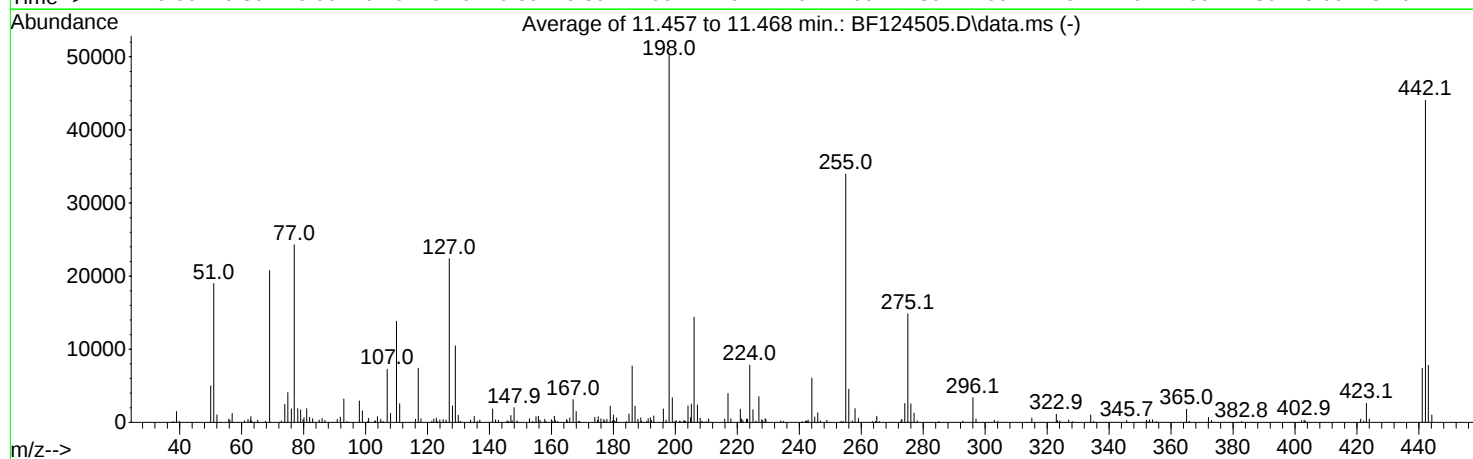


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070121\
 Data File : BF124505.D
 Acq On : 1 Jul 2021 11:28
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 02 14:41:35 2021

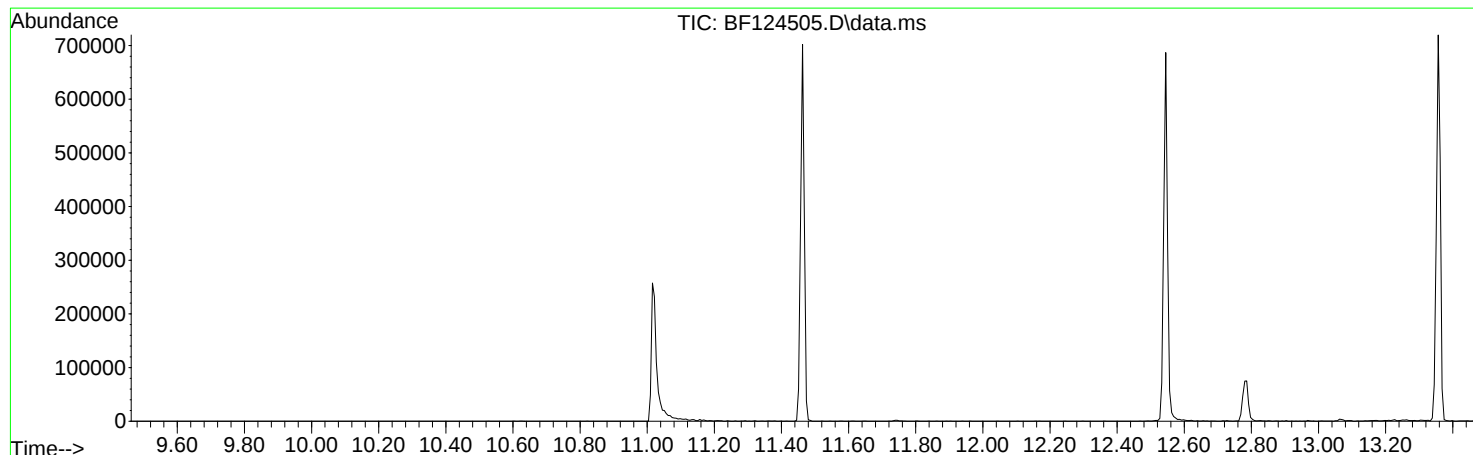

AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	19005	PASS
68	69	0.00	2	0.8	164	PASS
69	198	0.00	100	41.3	20775	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.5	22390	PASS
197	198	0.00	2	0.6	307	PASS
198	198	100	100	100.0	50317	PASS
199	198	5	9	6.7	3365	PASS
275	198	10	60	29.5	14847	PASS
365	198	1	100	3.6	1799	PASS
441	198	0.01	100	14.7	7405	PASS
442	442	50	100	100.0	44064	PASS
443	442	15	24	17.7	7783	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/1/2021	BNA_F	<u>BF124505.D</u>
Compound Name	Response	Retention Time
DDT	113869	13.35
DDD	1252	13.06
DDE	130	12.72
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1382	115251	1.20

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070121\
 Data File : BF124505.D
 Acq On : 1 Jul 2021 11:28
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 01 14:12:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 29 12:49:33 2021
 Response via : Initial Calibration

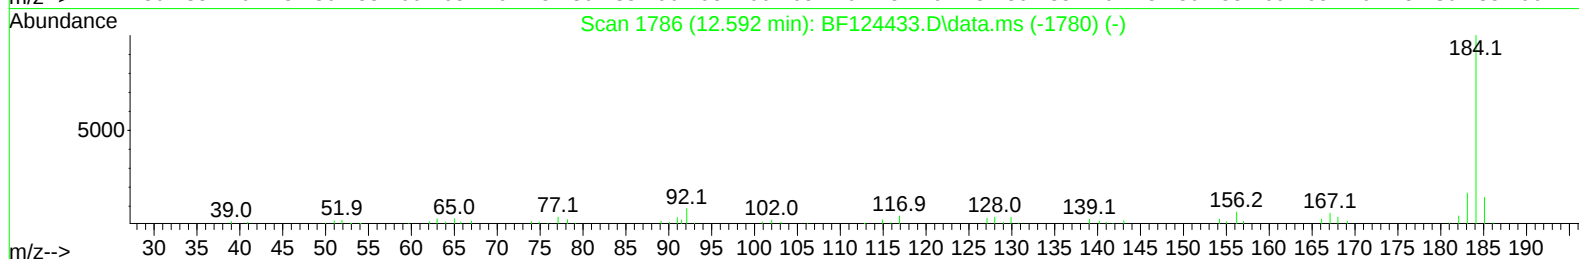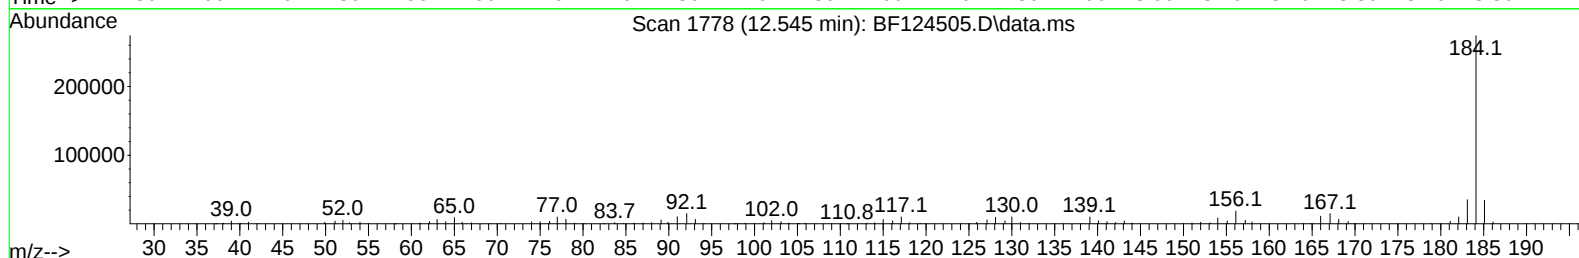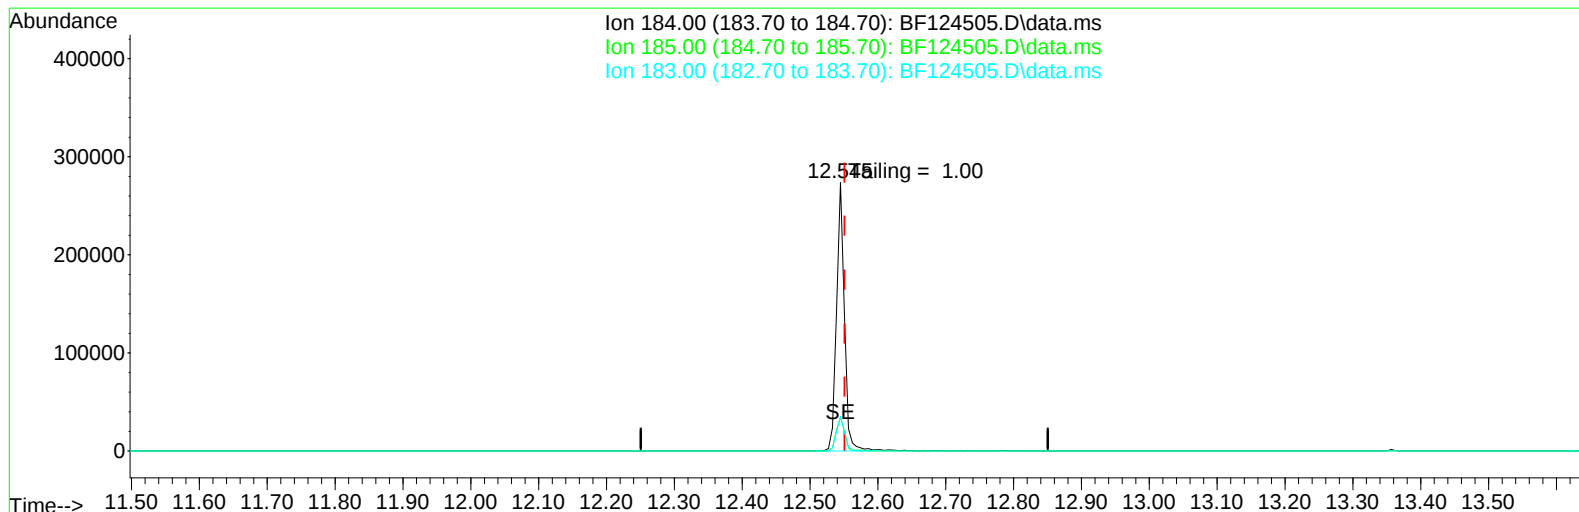

TIC: BF124505.D\data.ms

(77) Benzidine

12.545min (-0.006) 0.00 ng




response 222913

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	12.51
183.00	9.80	12.90#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070121\
Data File : BF124505.D
Acq On : 1 Jul 2021 11:28
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 01 14:12:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 29 12:49:33 2021
Response via : Initial Calibration

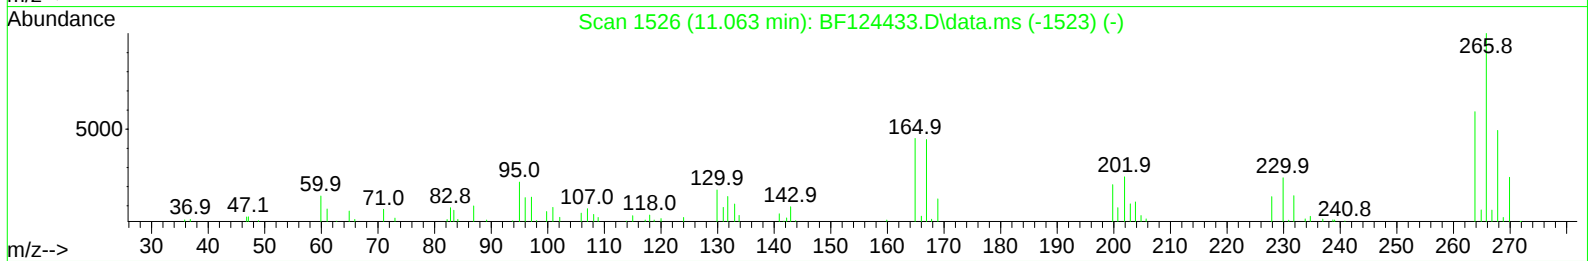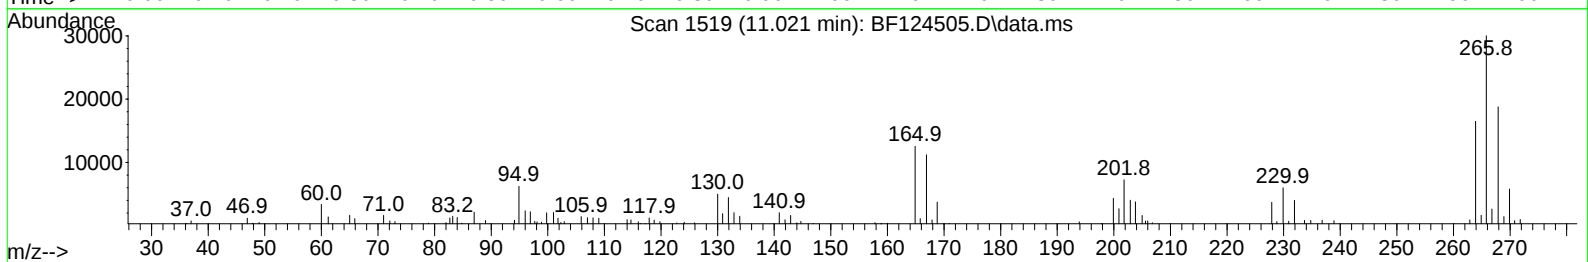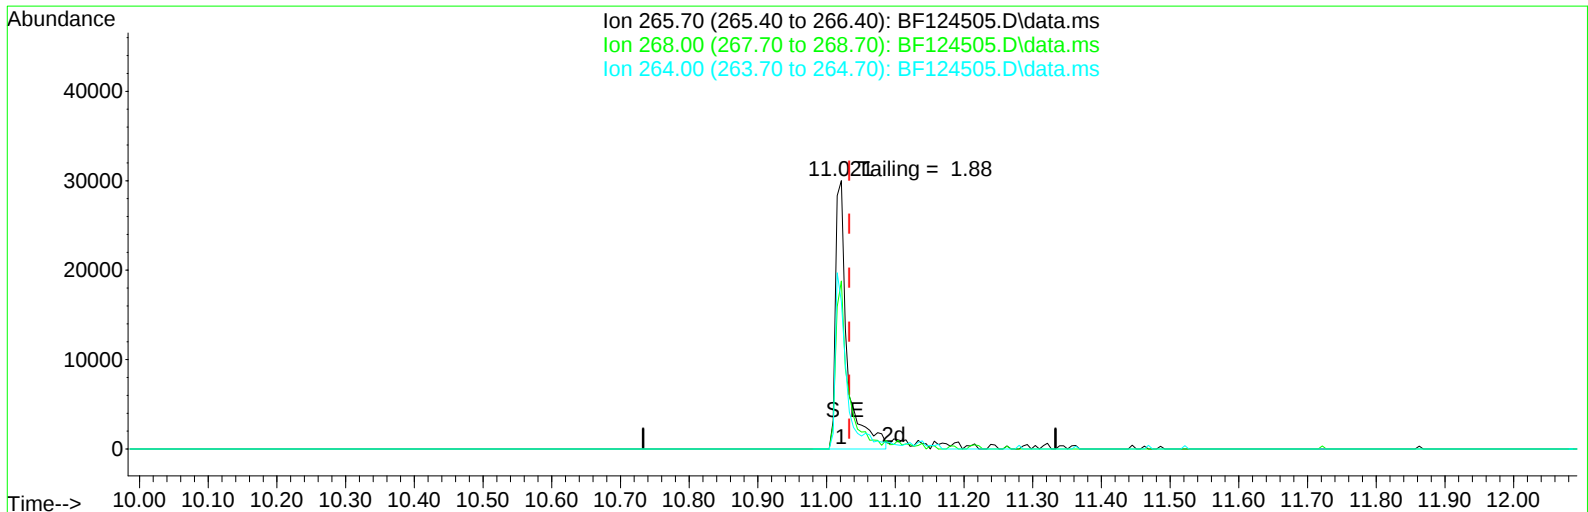

TIC: BF124505.D\data.ms

(70) Pentachlorophenol (C)

11.021min (-0.012) 21073.46 ng

response 35905

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.61
264.00	65.70	54.96
0.00	0.00	0.00