
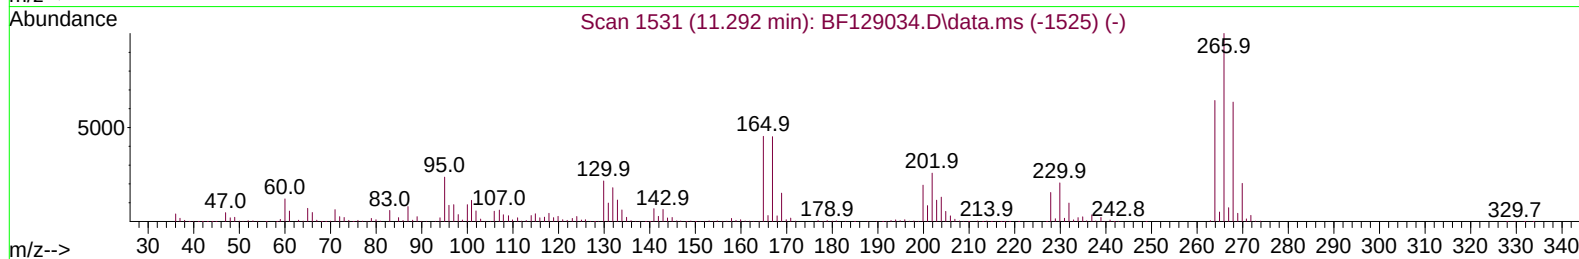
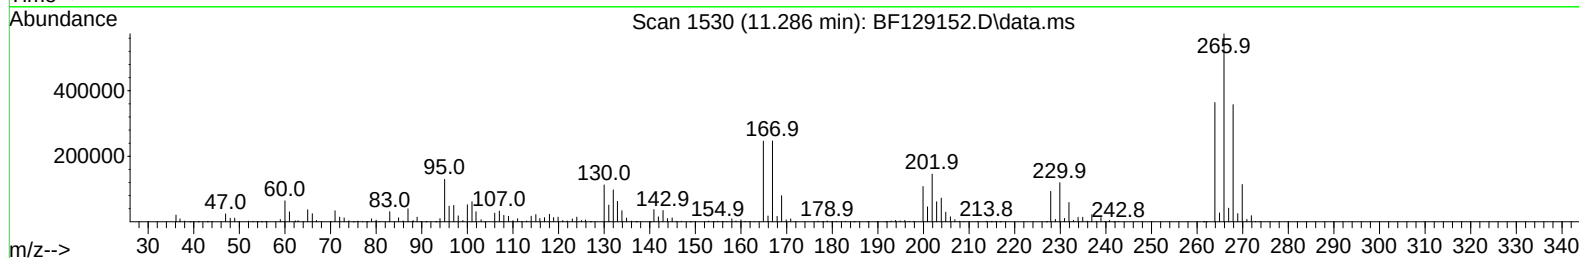


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070722\
Data File : BF129152.D
Acq On : 07 Jul 2022 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 14:35:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

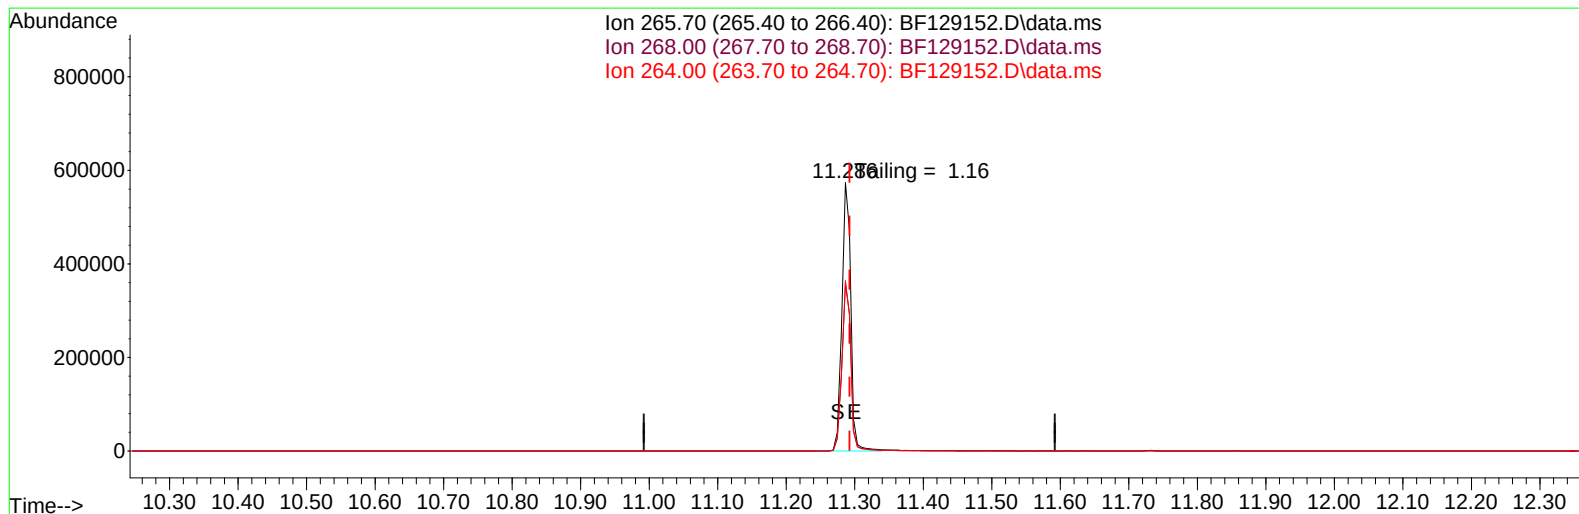

TIC: BF129152.D\data.ms

(70) Pentachlorophenol (C)




11.286min (-0.006) 347058.80 ng

response 514188

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.29
264.00	61.80	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070722\
 Data File : BF129152.D
 Acq On : 07 Jul 2022 10:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 14:35:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:05:31 2022
 Response via : Initial Calibration

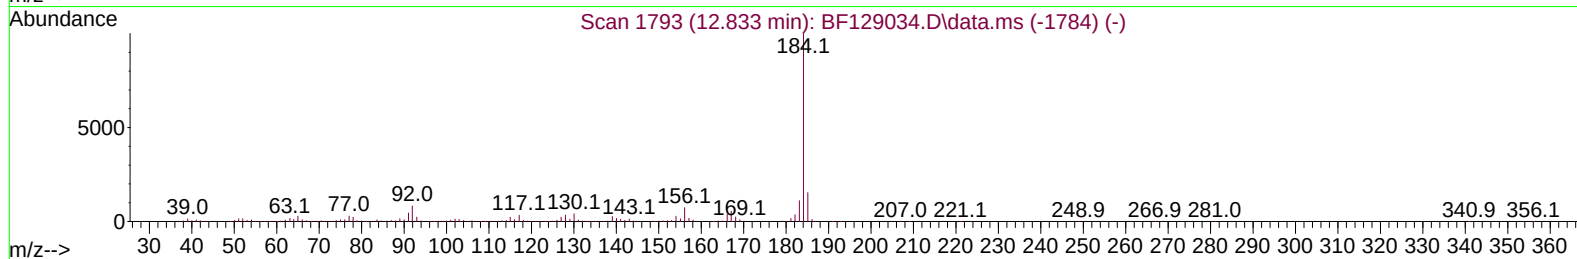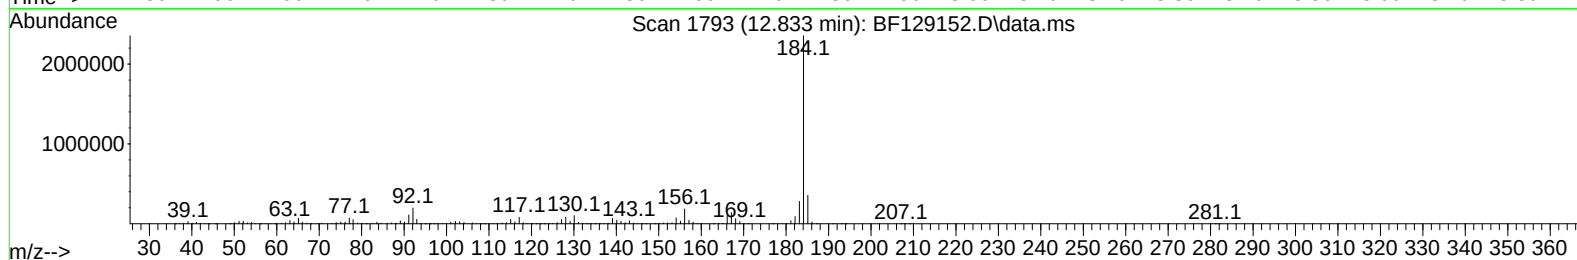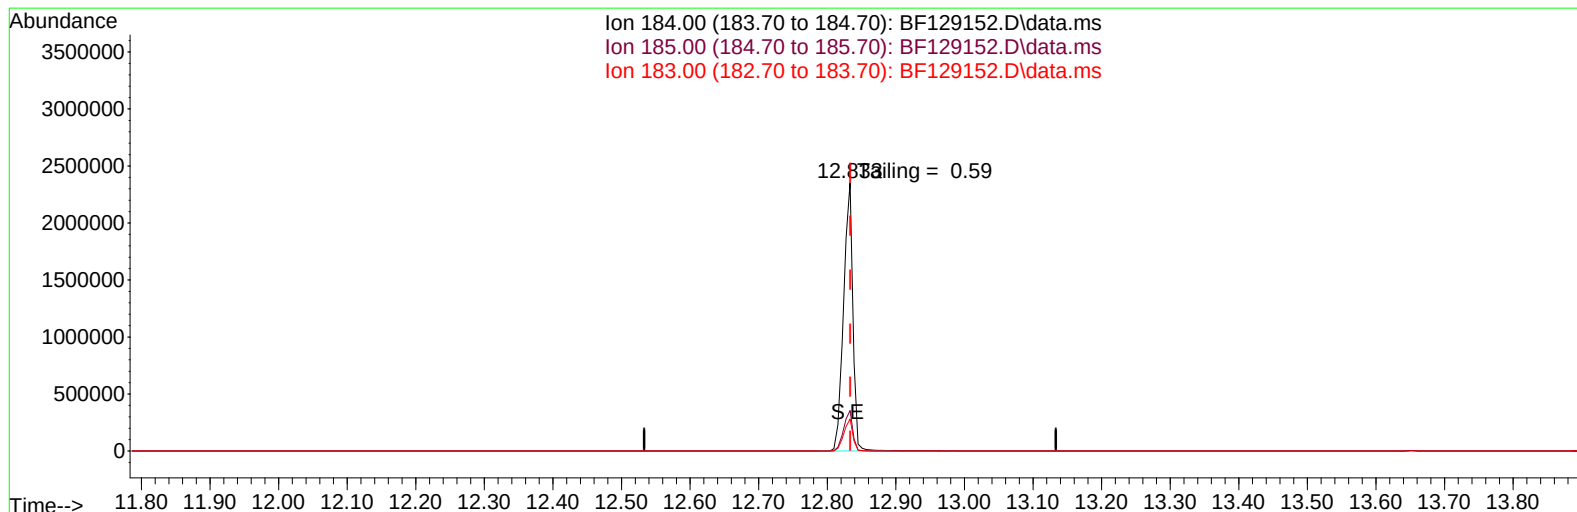

TIC: BF129152.D\data.ms

(77) Benzidine

12.833min (-0.000) 8668.39 ng m

response 2230237

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.10
183.00	11.60	11.93
0.00	0.00	0.00