


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070722\
 Data File : BF129152.D
 Acq On : 07 Jul 2022 10:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 29 17:05:31 2022

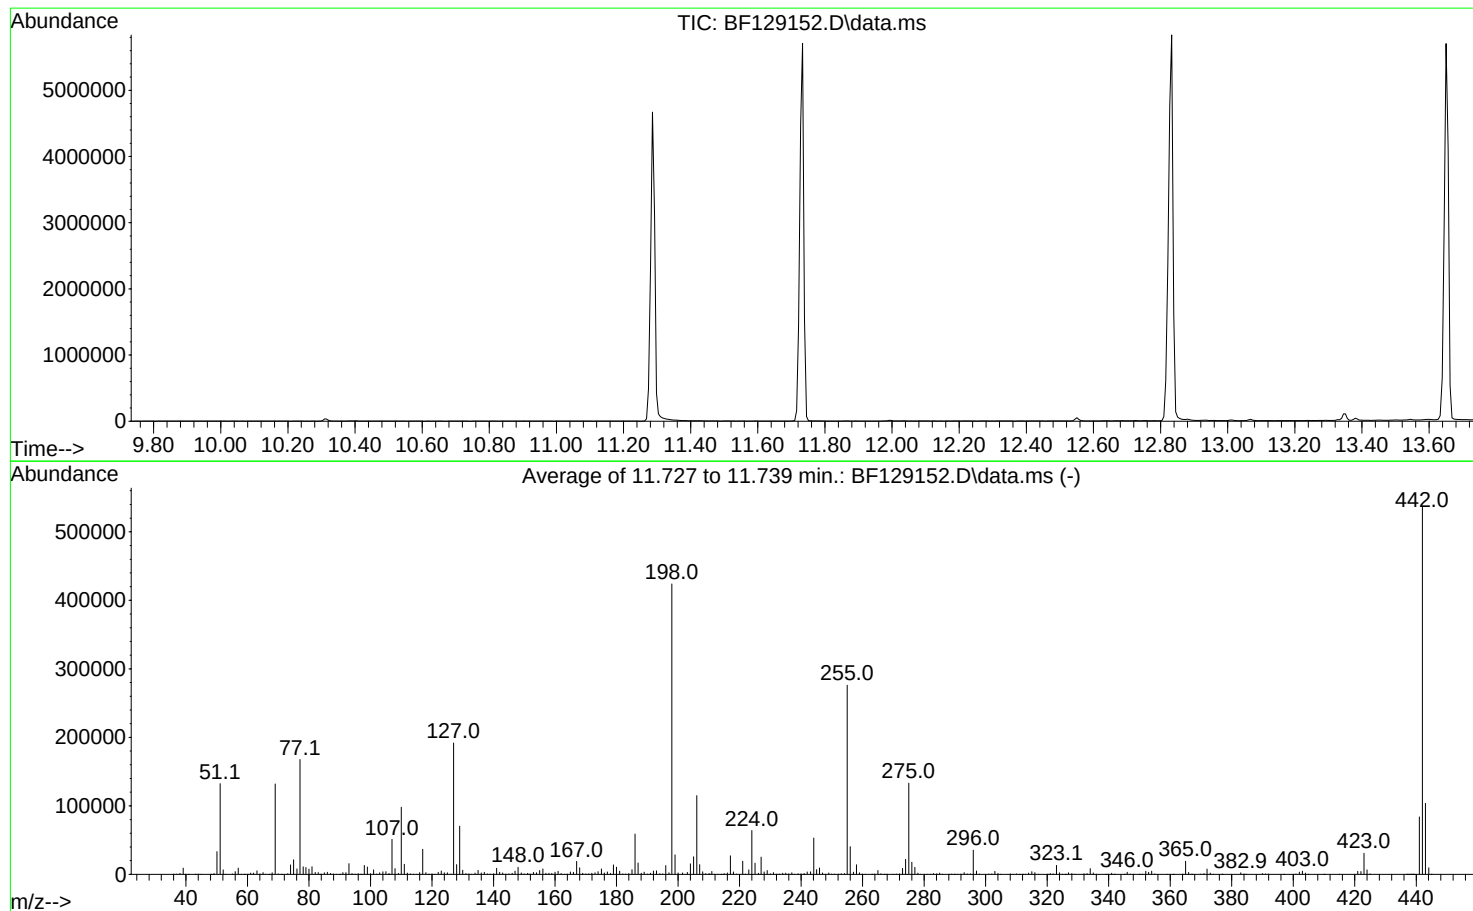




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	132539	PASS
68	69	0.00	2	1.8	2416	PASS
69	198	0.00	100	31.1	131939	PASS
70	69	0.00	2	0.6	778	PASS
127	198	10	80	45.2	191776	PASS
197	198	0.00	2	0.6	2458	PASS
198	198	100	100	100.0	423936	PASS
199	198	5	9	6.7	28466	PASS
275	198	10	60	31.4	133272	PASS
365	198	1	100	4.5	19152	PASS
441	198	0.01	100	19.8	83955	PASS
442	442	50	100	100.0	537003	PASS
443	442	15	24	19.3	103712	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070722\
 Data File : BF129152.D
 Acq On : 07 Jul 2022 10:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 07 14:35:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:05:31 2022
 Response via : Initial Calibration

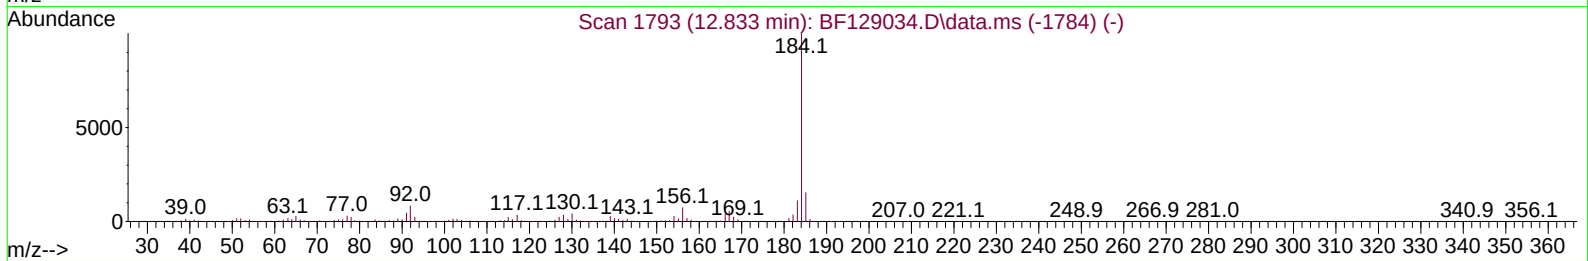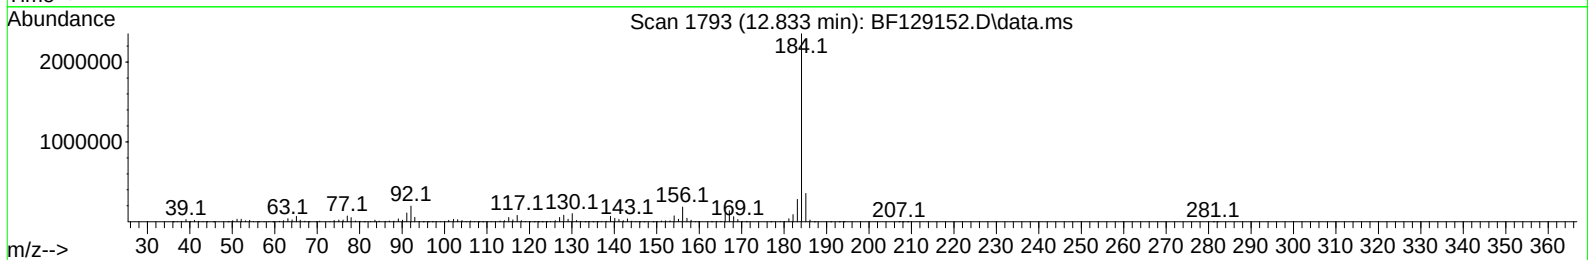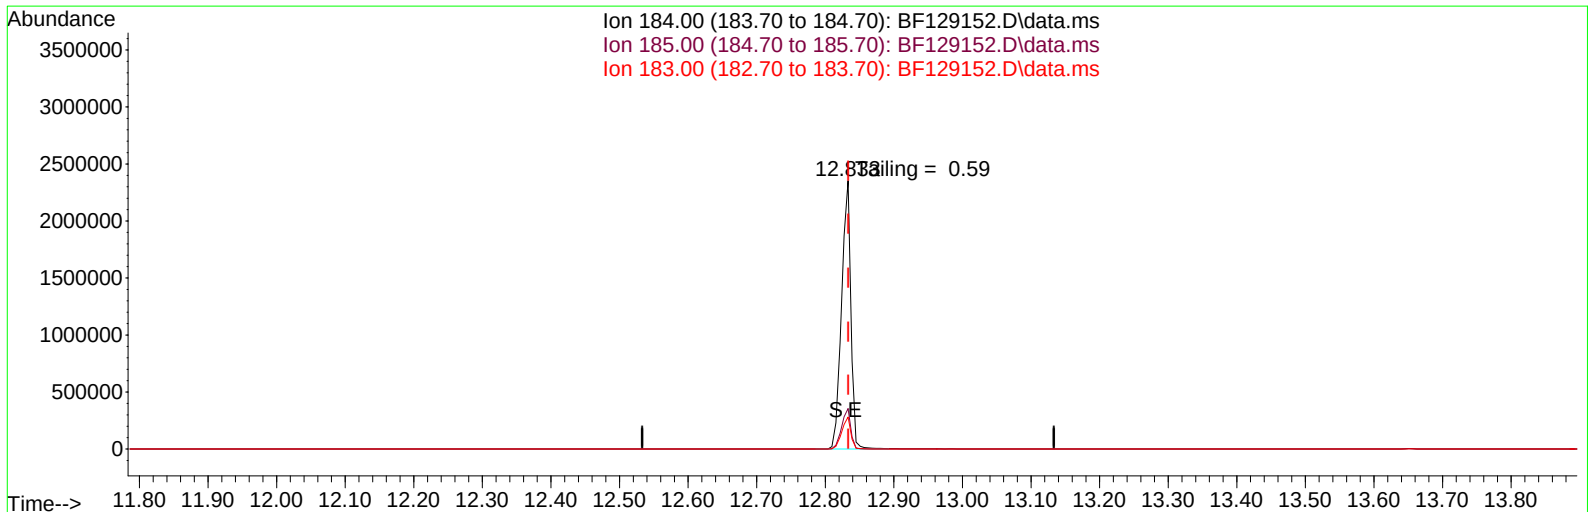

TIC: BF129152.D\data.ms

(77) Benzidine

12.833min (-0.000) 8668.39 ng m

response 2230237

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.10
183.00	11.60	11.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/7/2022	BNA_F	<u>BF129152.D</u>
Compound Name	Response	Retention Time
DDT	984321	13.65
DDD	17743	13.35
DDE	1275	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19018	1003339	1.90

Instrument :
BNA_F
ClientSampleId :
DFTPP