
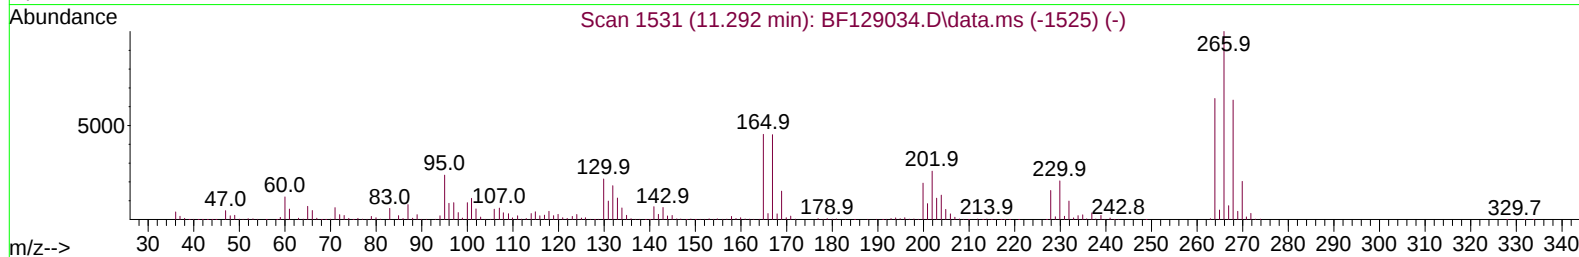
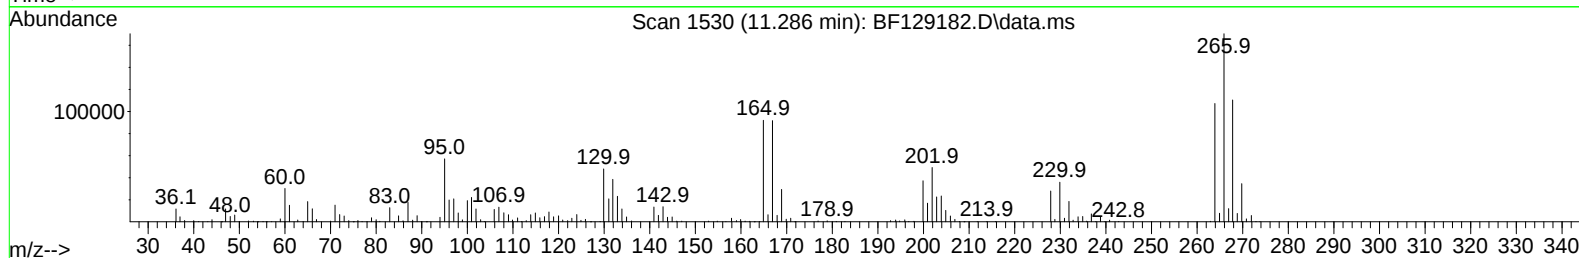


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071222\
Data File : BF129182.D
Acq On : 12 Jul 2022 09:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 14:28:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 14:13:54 2022
Response via : Initial Calibration

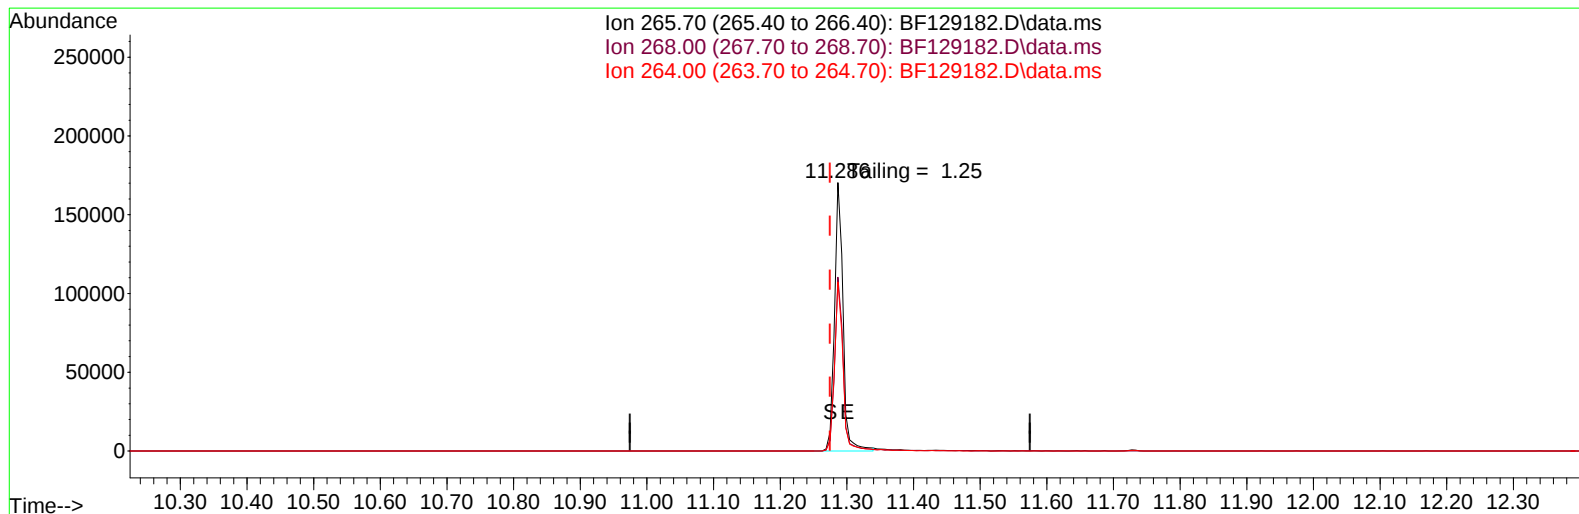

TIC: BF129182.D\data.ms

(70) Pentachlorophenol (C)




11.286min (+ 0.012) 20278.28 ng

response 153937

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.78
264.00	61.80	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071222\
Data File : BF129182.D
Acq On : 12 Jul 2022 09:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 14:28:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 12 14:13:54 2022
Response via : Initial Calibration

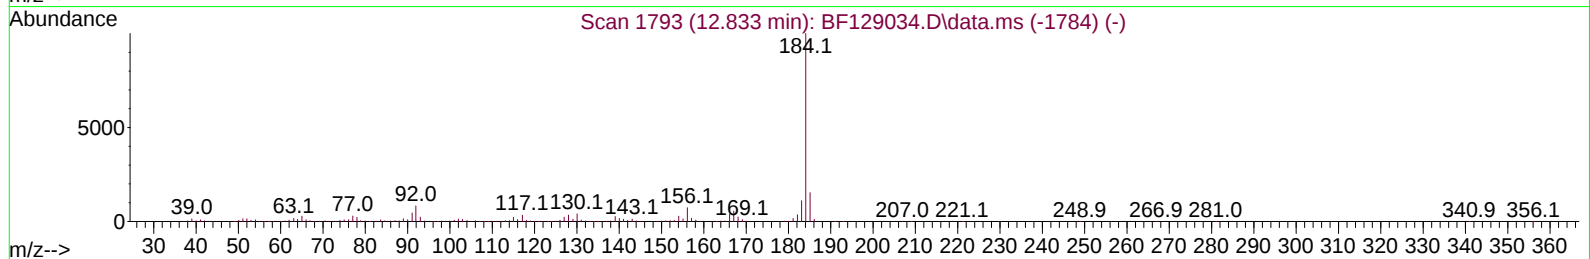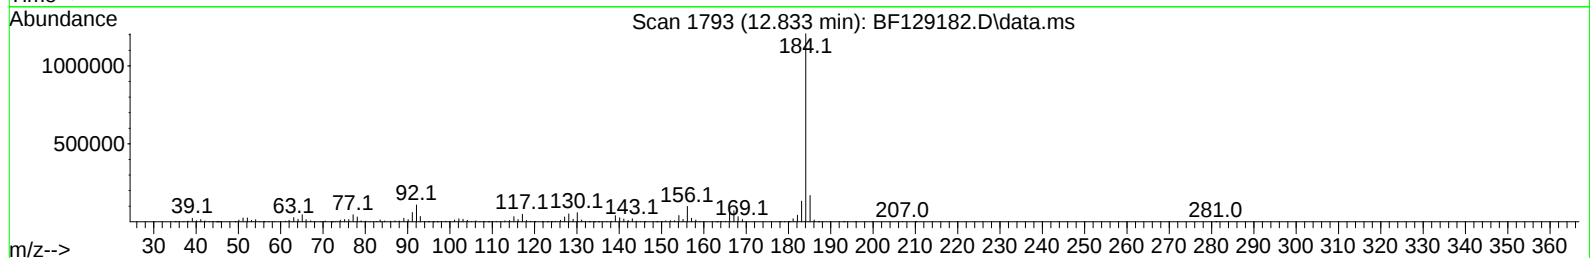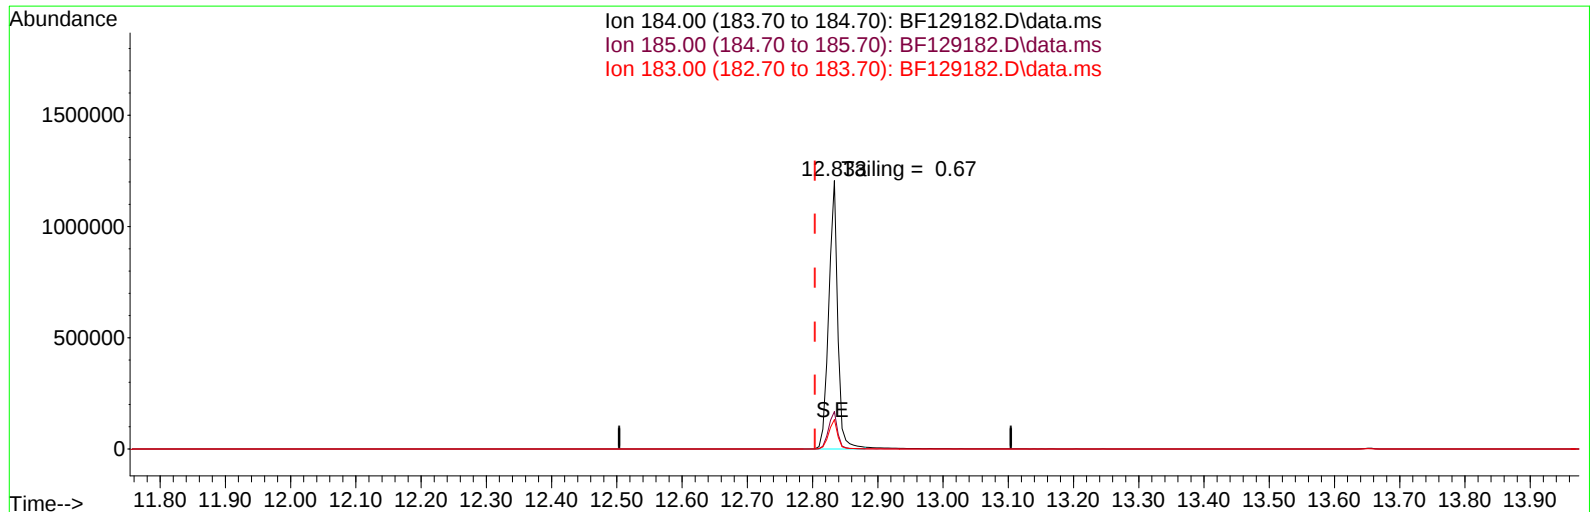

TIC: BF129182.D\data.ms

(77) Benzidine

12.833min (+ 0.030) 1095344.17 ng

response 1150740

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.95
183.00	11.60	11.01
0.00	0.00	0.00