

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071222\
 Data File : BF129199.D
 Acq On : 12 Jul 2022 20:29
 Operator : CG\JU
 Sample : N3641-01 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-01-070822

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.051	296	300	305	rVB	29136	34181	2.06%	0.260%
2	5.551	551	555	563	rBV	787058	719743	43.28%	5.466%
3	6.551	721	725	732	rBV	674520	575144	34.58%	4.368%
4	6.934	786	790	793	rBV	1754126	1368817	82.30%	10.396%
5	7.492	881	885	888	rBV	422553	351508	21.14%	2.670%
6	8.216	1001	1008	1012	rBV	2027584	1663133	100.00%	12.631%
7	9.286	1186	1190	1194	rBV	823435	661184	39.76%	5.022%
8	9.833	1280	1283	1286	rBV	24451	20439	1.23%	0.155%
9	9.974	1301	1307	1310	rBV	1898832	1490756	89.64%	11.322%
10	10.522	1397	1400	1407	rVB2	17070	24221	1.46%	0.184%
11	10.763	1437	1441	1446	rBV	338495	283687	17.06%	2.155%
12	10.880	1456	1461	1465	rVB4	24125	39497	2.37%	0.300%
13	11.063	1489	1492	1496	rBV5	12113	24854	1.49%	0.189%
14	11.316	1532	1535	1537	rBV	21739	21435	1.29%	0.163%
15	11.345	1537	1540	1547	rVB6	20867	34063	2.05%	0.259%
16	11.469	1557	1561	1563	rBV	1411479	1308826	78.70%	9.940%
17	11.486	1563	1564	1567	rVV	101572	75756	4.56%	0.575%
18	11.539	1570	1573	1575	rBV	30152	25739	1.55%	0.195%
19	11.798	1614	1617	1621	rBV2	17580	20688	1.24%	0.157%
20	11.974	1643	1647	1649	rBV3	41511	60719	3.65%	0.461%
21	12.080	1662	1665	1667	rBV2	34917	34936	2.10%	0.265%
22	12.151	1675	1677	1680	rBV	21633	20599	1.24%	0.156%
23	12.515	1737	1739	1741	rBV	39903	38724	2.33%	0.294%
24	12.680	1764	1767	1770	rBV	213334	182270	10.96%	1.384%
25	12.910	1804	1806	1809	rBV	184770	159696	9.60%	1.213%
26	13.051	1827	1830	1833	rBV	555686	491454	29.55%	3.733%
27	14.115	2007	2011	2014	rBV	1324308	1264159	76.01%	9.601%
28	14.210	2022	2027	2031	rBV	1153384	1145060	68.85%	8.697%
29	15.627	2264	2268	2277	rVB2	761373	1025366	61.65%	7.788%




Sum of corrected areas: 13166654

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071222\
Data File : BF129199.D
Acq On : 12 Jul 2022 20:29
Operator : CG\JU
Sample : N3641-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-070822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

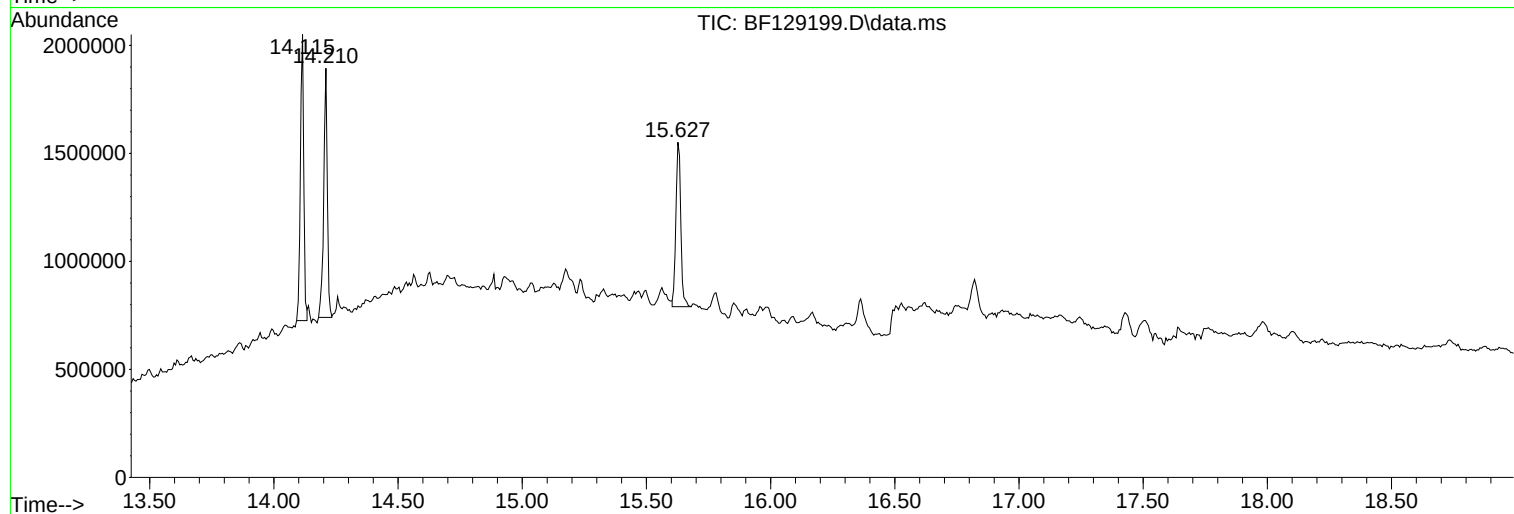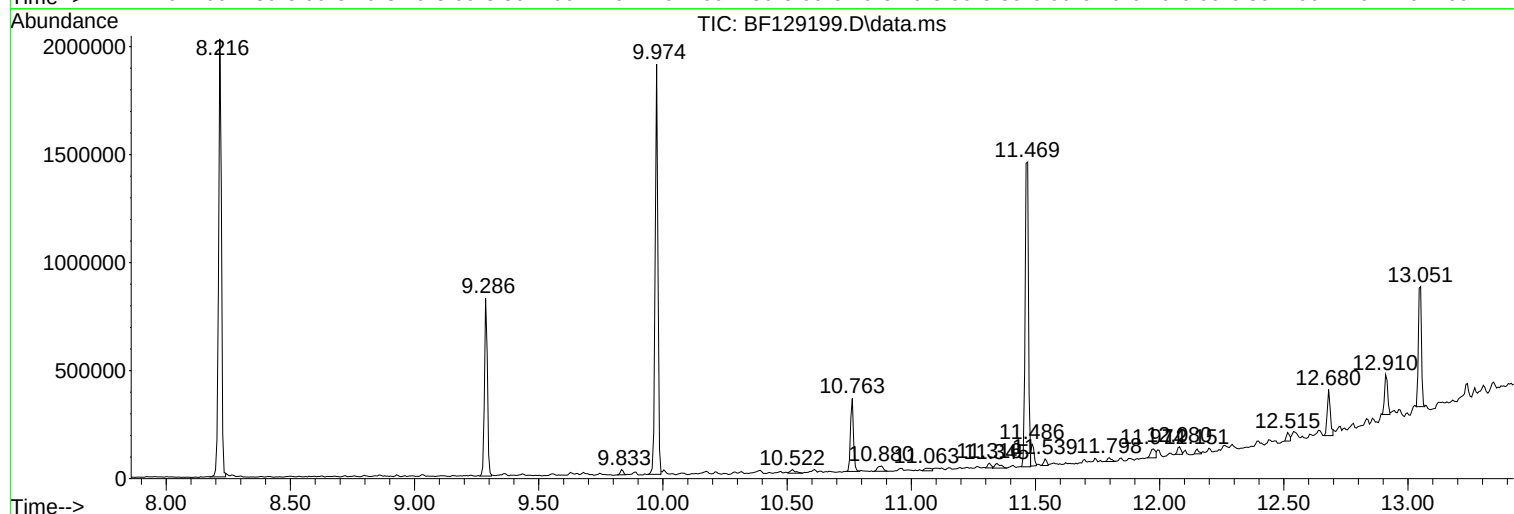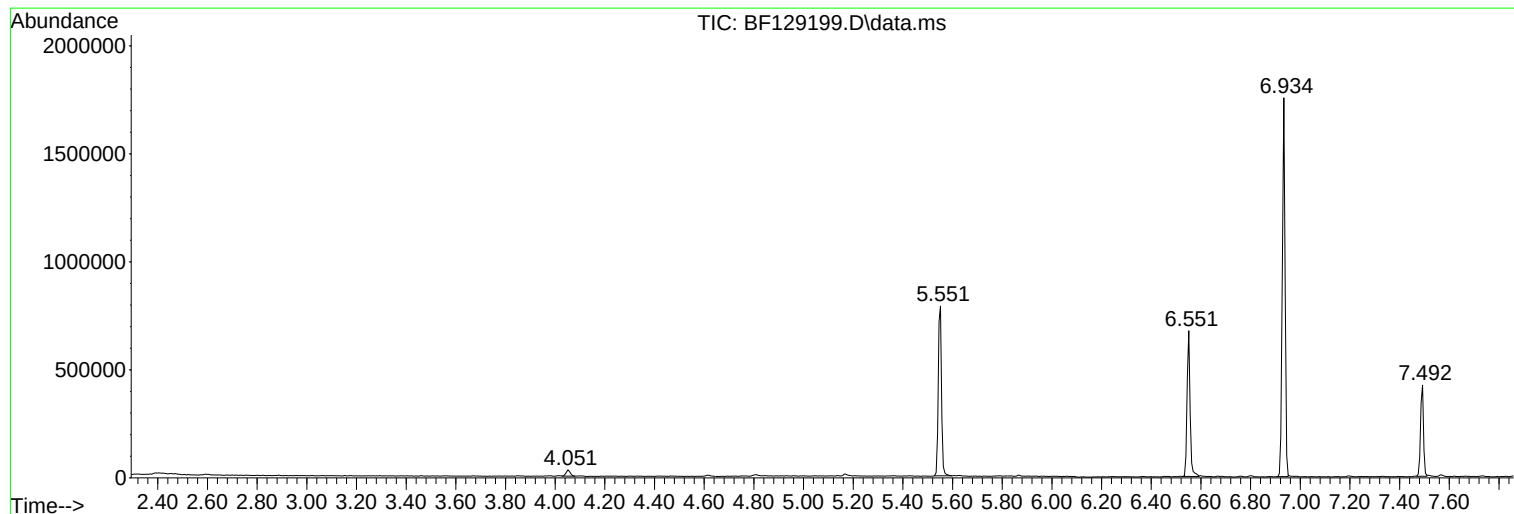

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071222\
Data File : BF129199.D
Acq On : 12 Jul 2022 20:29
Operator : CG\JU
Sample : N3641-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-070822










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.210	18.12 ng	1145060	Chrysene-d12	14.115

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Vanadium, cycloheptatrienyl-(pen...]	277	C17H22V	1000155-20-5	47
4			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	45
5			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	28

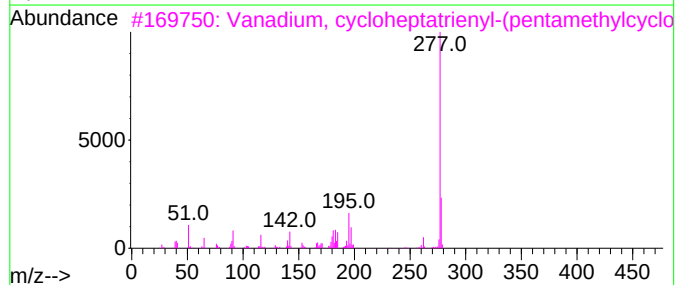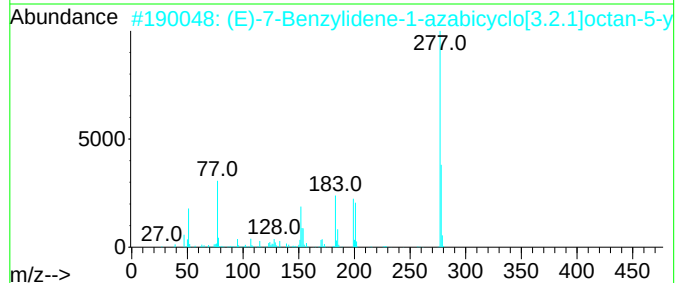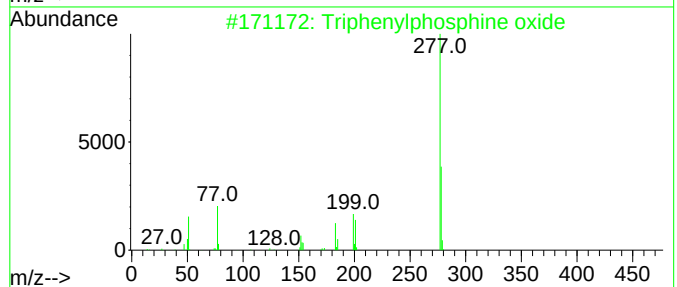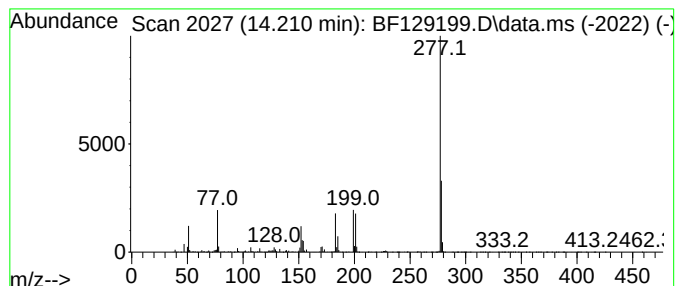

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071222\
Data File : BF129199.D
Acq On : 12 Jul 2022 20:29
Operator : CG\JU
Sample : N3641-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-01-070822

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.210	18.1	ng	1145060	5	14.115	1264160	20.0