


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071520\
 Data File : BF120868.D
 Acq On : 15 Jul 2020 11:27
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 14:16:14 2020

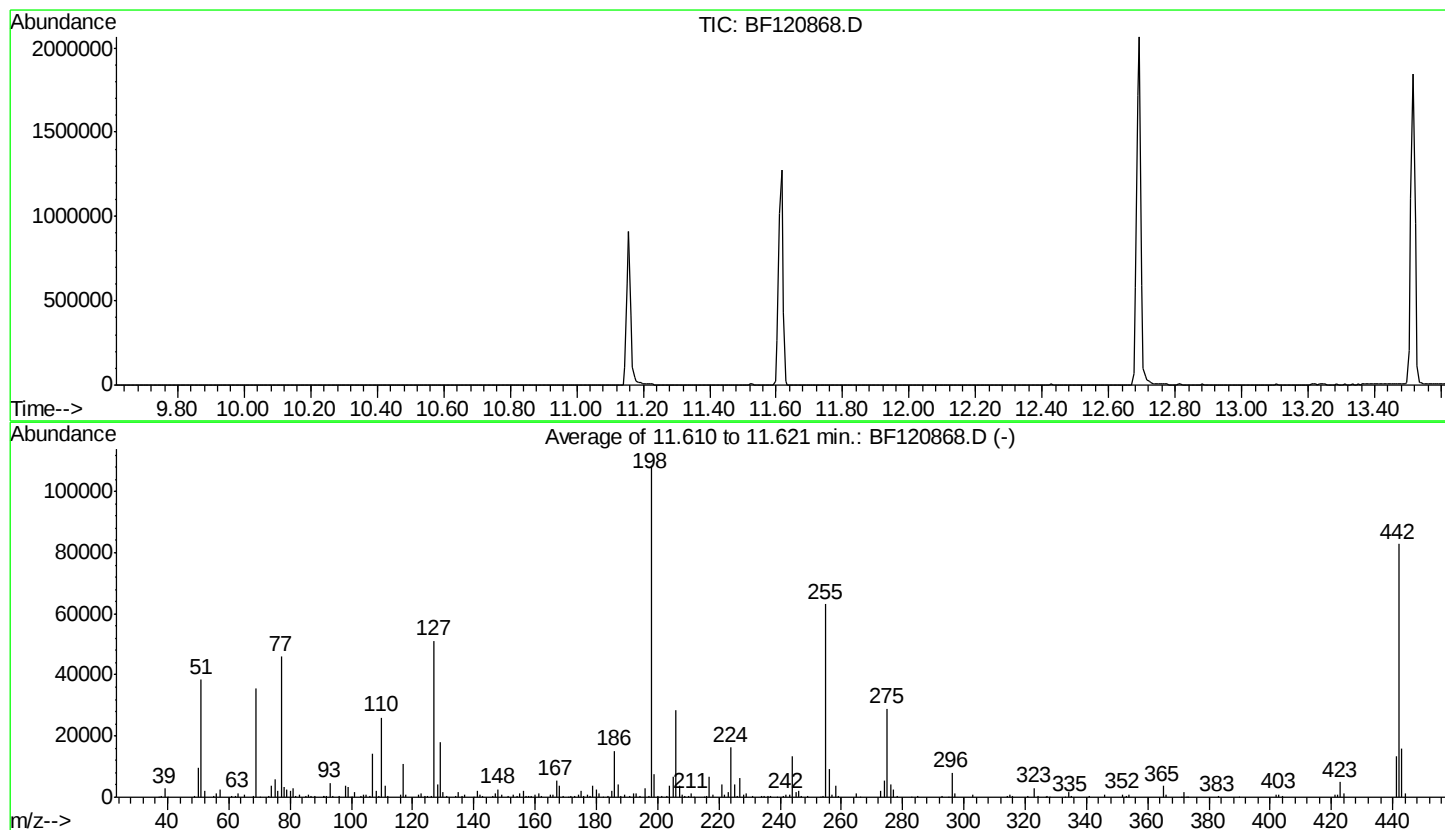

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	38471	PASS
68	69	0.00	2	1.6	583	PASS
69	198	0.00	100	32.8	35604	PASS
70	69	0.00	2	0.3	112	PASS
127	198	10	80	47.1	51128	PASS
197	198	0.00	2	0.5	499	PASS
198	198	100	100	100.0	108464	PASS
199	198	5	9	7.0	7540	PASS
275	198	10	60	26.8	29056	PASS
365	198	1	100	3.3	3627	PASS
441	198	0.01	100	12.3	13357	PASS
442	198	50	100	76.3	82768	PASS
443	442	15	24	19.3	15955	PASS