
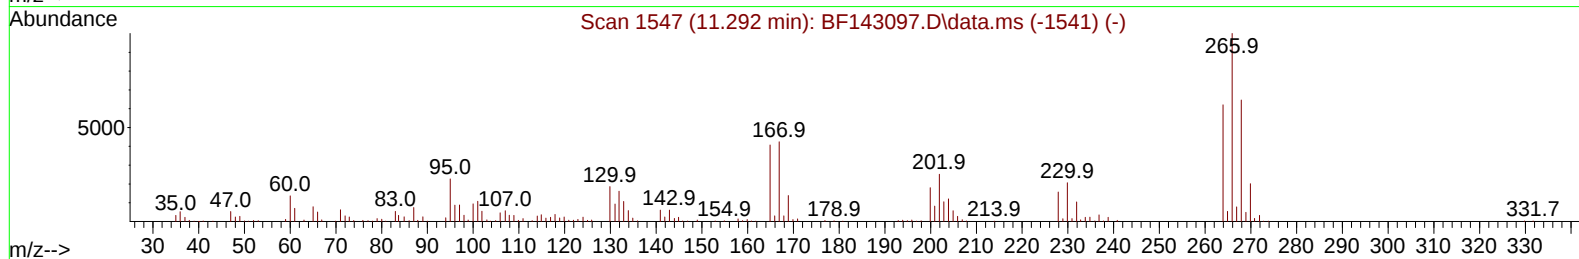
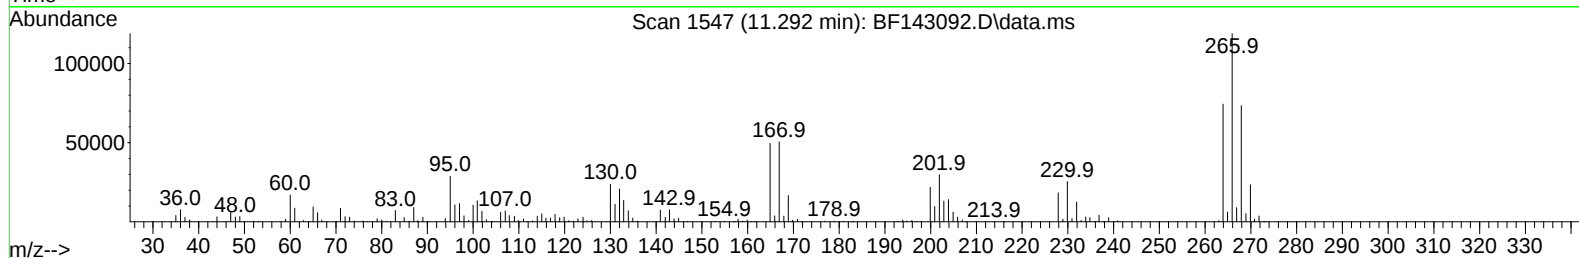


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071525\
Data File : BF143092.D
Acq On : 15 Jul 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 18:02:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 15 17:53:25 2025
Response via : Initial Calibration

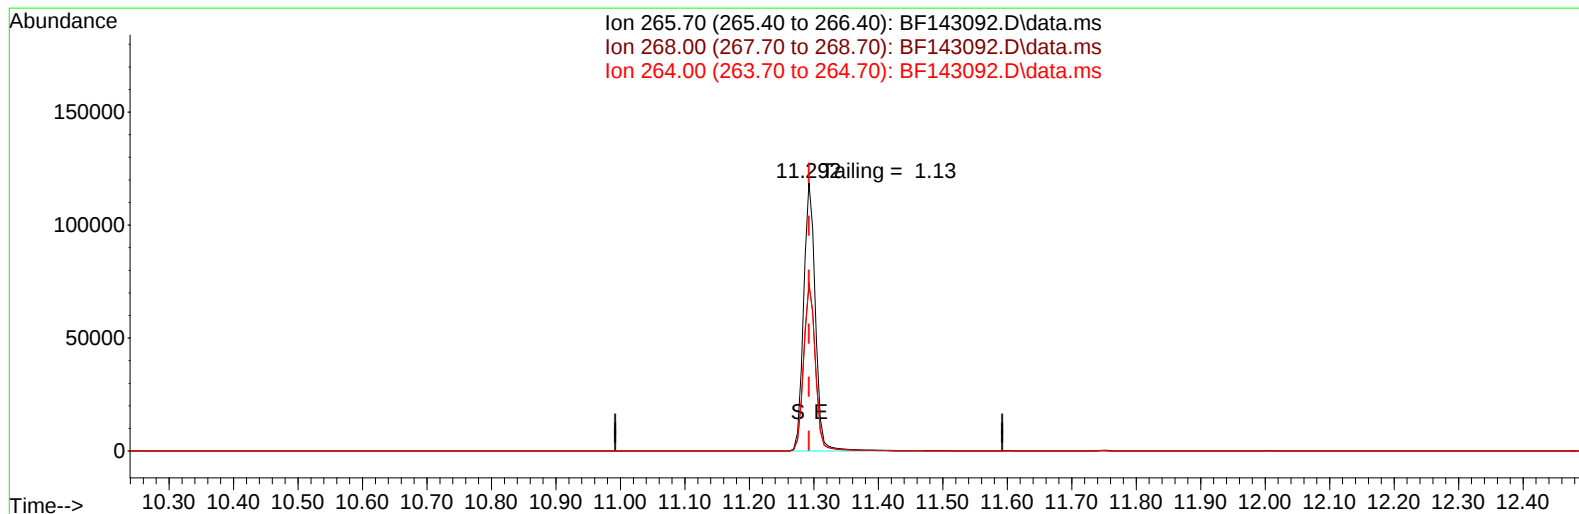

TIC: BF143092.D\data.ms

(70) Pentachlorophenol (C)




11.292min (+ 0.000) 28198.82 ng

response 151956

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	61.86
264.00	62.10	62.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071525\
Data File : BF143092.D
Acq On : 15 Jul 2025 12:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 18:02:12 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 15 17:53:25 2025
Response via : Initial Calibration

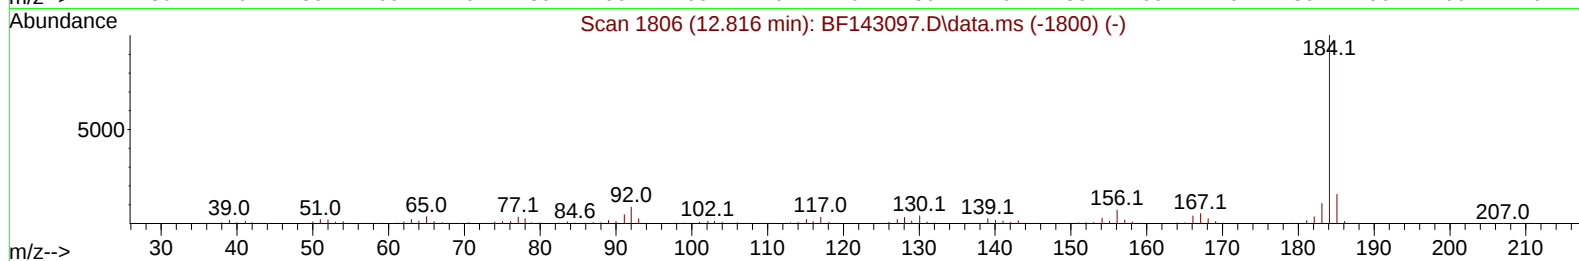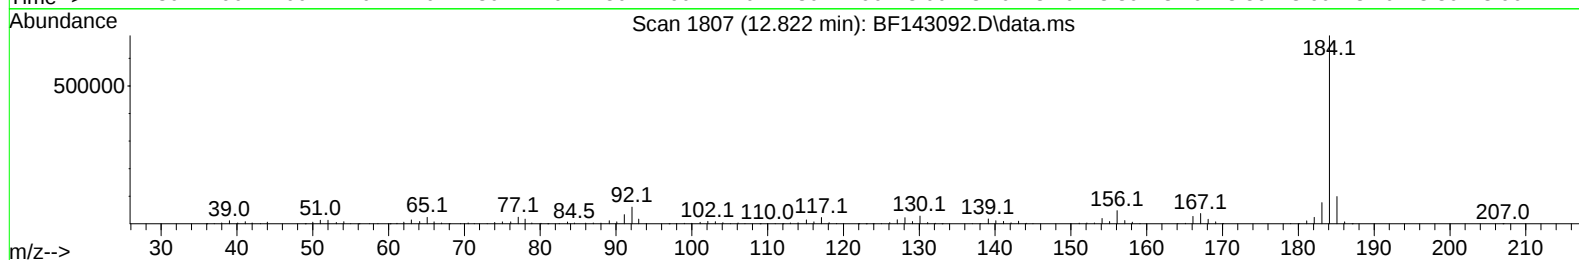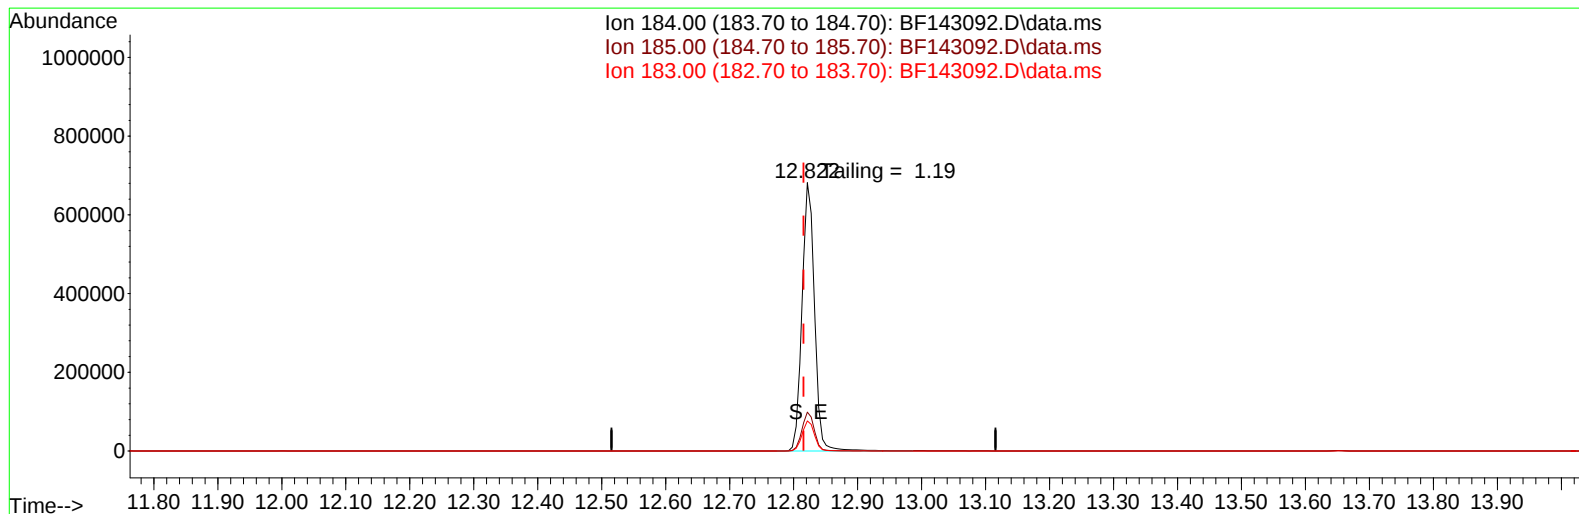

TIC: BF143092.D\data.ms

(77) Benzidine

12.822min (+ 0.006) 0.00 ng

response 925010

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.52
183.00	10.70	11.25
0.00	0.00	0.00