

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072821\
 Data File : BF124819.D
 Acq On : 28 Jul 2021 10:11
 Operator : JU/CG
 Sample : PB137987BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137987BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.146	516	520	524	rBB	2829	3975	1.11%	0.204%
2	5.504	576	581	584	rBV	218248	258040	71.93%	13.267%
3	6.504	745	751	754	rBB	221065	257467	71.77%	13.238%
4	6.869	810	813	816	rBB	60546	45989	12.82%	2.365%
5	7.440	904	910	912	rBB	144747	172950	48.21%	8.892%
6	8.151	1027	1031	1035	rBB	67295	62178	17.33%	3.197%
7	9.234	1209	1215	1218	rBV	342430	333523	92.97%	17.148%
8	9.910	1325	1330	1333	rBB	86608	72409	20.18%	3.723%
9	10.704	1459	1465	1468	rBV	226257	207258	57.77%	10.656%
10	11.398	1579	1583	1586	rBV	95540	72330	20.16%	3.719%
11	12.992	1848	1854	1856	rBV	360195	358753	100.00%	18.445%
12	14.033	2028	2031	2035	rBV	61919	57055	15.90%	2.934%
13	15.515	2278	2283	2289	rBB	34297	43014	11.99%	2.212%




Sum of corrected areas: 1944941

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072821\
Data File : BF124819.D
Acq On : 28 Jul 2021 10:11
Operator : JU/CG
Sample : PB137987BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137987BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

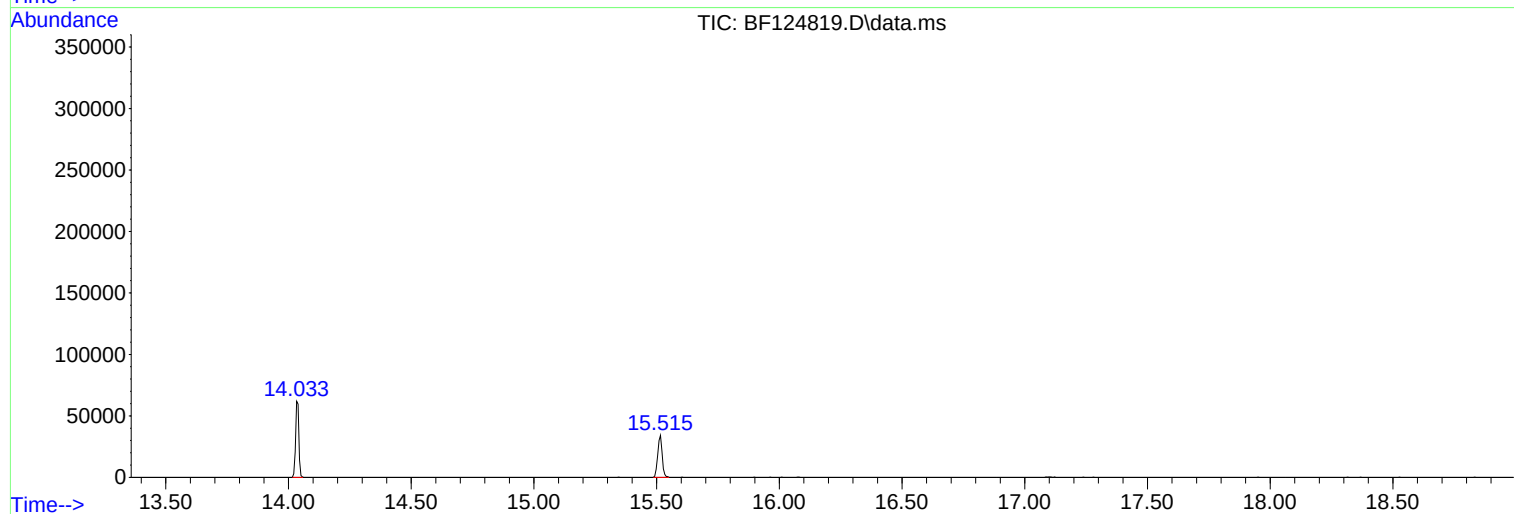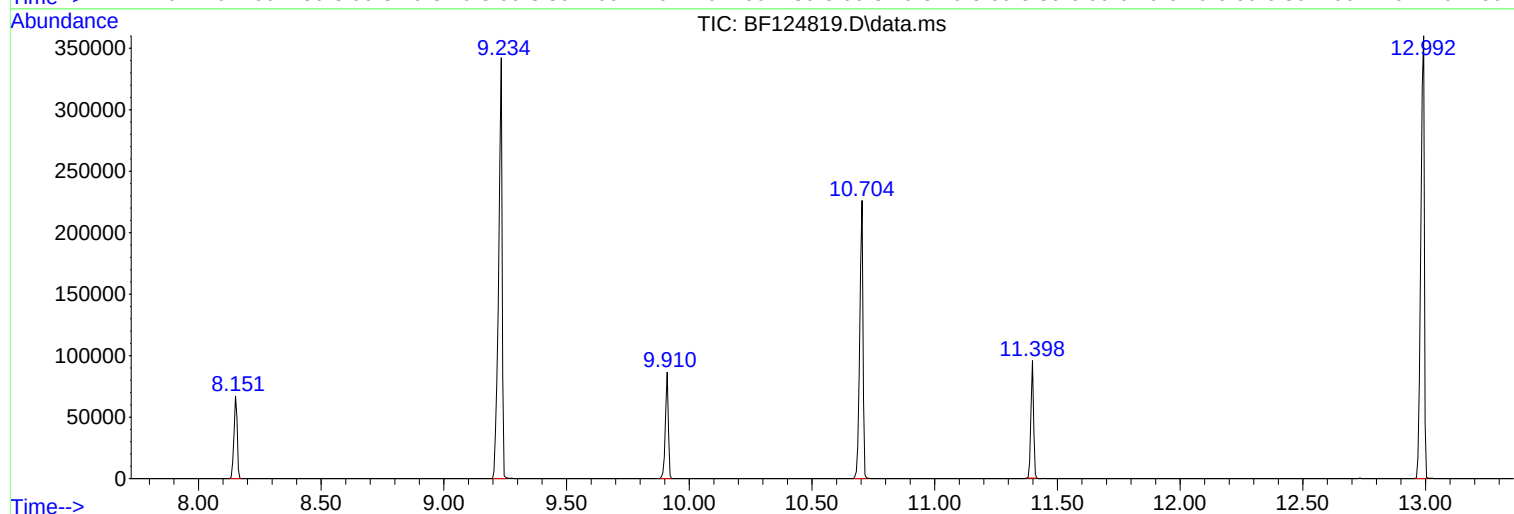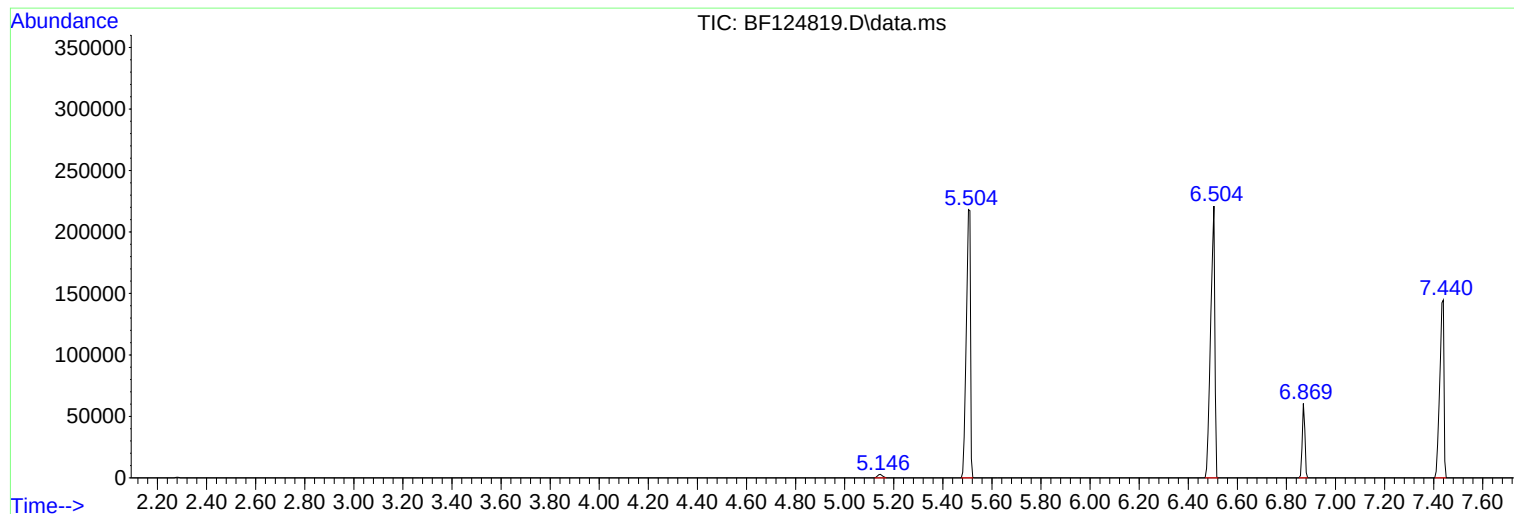

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072821\
Data File : BF124819.D
Acq On : 28 Jul 2021 10:11
Operator : JU/CG
Sample : PB137987BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137987BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072821\
Data File : BF124819.D
Acq On : 28 Jul 2021 10:11
Operator : JU/CG
Sample : PB137987BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137987BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------