

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072821\
 Data File : BF124828.D
 Acq On : 28 Jul 2021 15:21
 Operator : JU/CG
 Sample : PB138016BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138016BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124828.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.140	515	519	523	rBB	3239	4448	1.37%	0.241%
2	5.504	575	581	584	rBB	244049	249914	76.73%	13.555%
3	6.504	744	751	754	rBB	209017	254287	78.07%	13.792%
4	6.869	810	813	816	rBB	60657	45394	13.94%	2.462%
5	7.440	904	910	912	rBV	143691	169693	52.10%	9.204%
6	8.151	1027	1031	1034	rBV	68844	60086	18.45%	3.259%
7	9.234	1209	1215	1218	rBV	327388	322775	99.10%	17.507%
8	9.910	1325	1330	1333	rBB	83711	68788	21.12%	3.731%
9	10.698	1460	1464	1468	rBV	189342	190233	58.40%	10.318%
10	11.398	1579	1583	1586	rBV	77797	67656	20.77%	3.670%
11	12.986	1848	1853	1856	rBV	324800	325720	100.00%	17.667%
12	14.033	2028	2031	2035	rBV	57643	48641	14.93%	2.638%
13	15.510	2278	2282	2287	rBV	30495	36030	11.06%	1.954%




Sum of corrected areas: 1843665

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072821\
Data File : BF124828.D
Acq On : 28 Jul 2021 15:21
Operator : JU/CG
Sample : PB138016BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138016BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

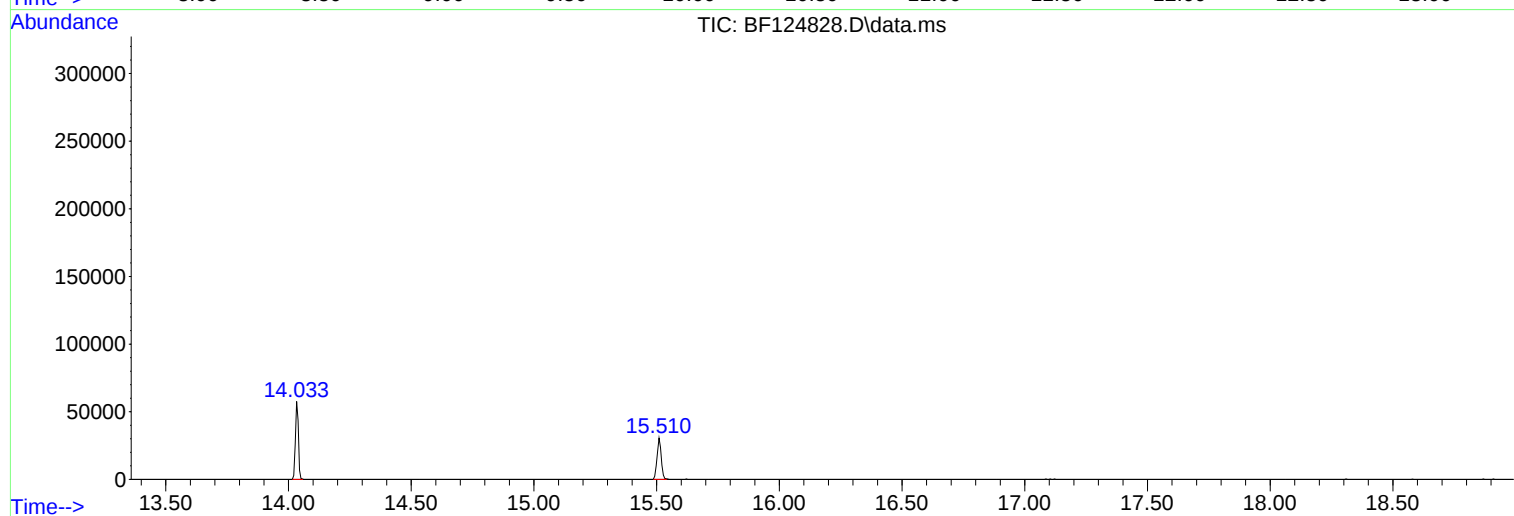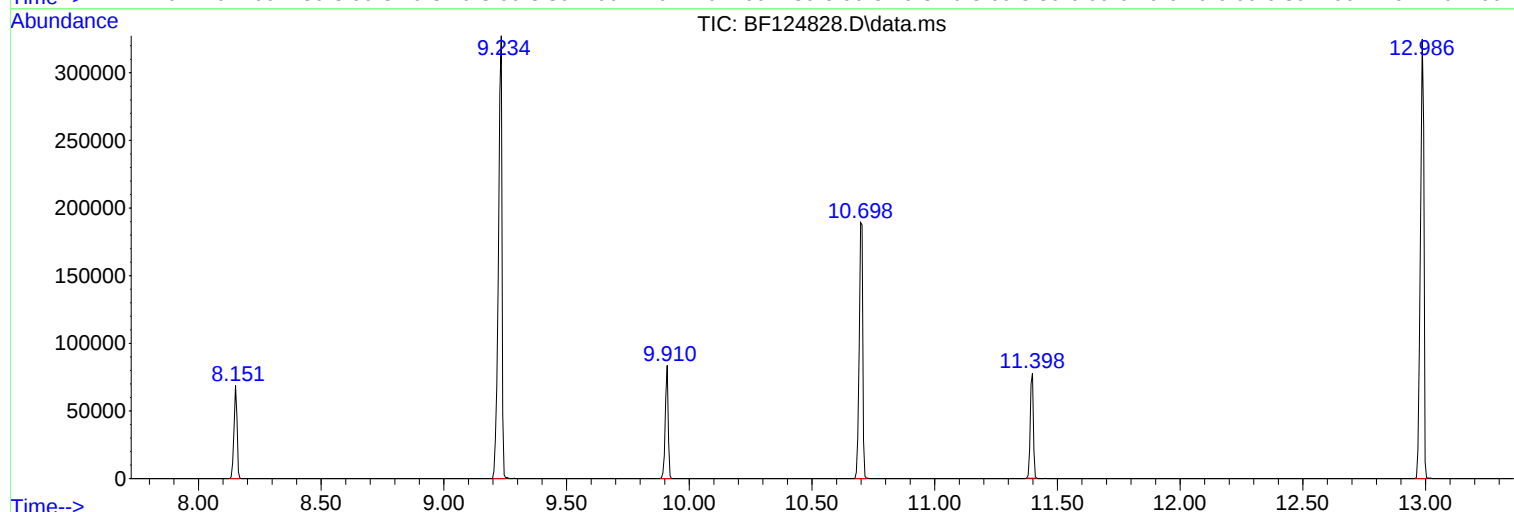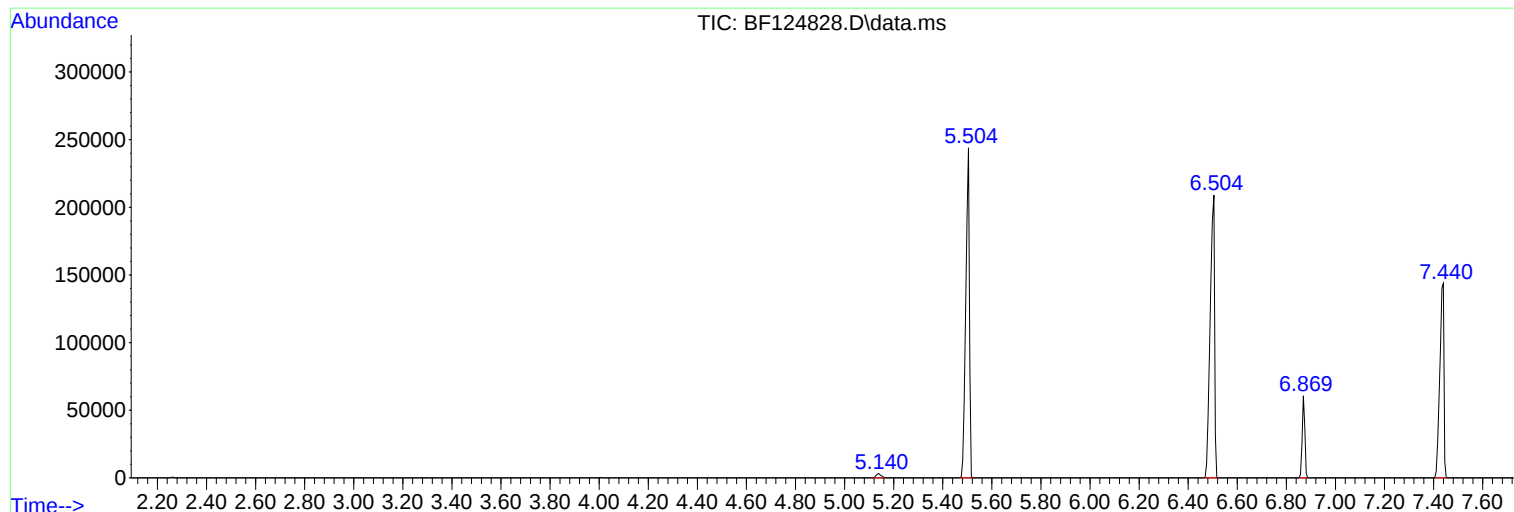

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072821\
Data File : BF124828.D
Acq On : 28 Jul 2021 15:21
Operator : JU/CG
Sample : PB138016BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138016BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072821\
Data File : BF124828.D
Acq On : 28 Jul 2021 15:21
Operator : JU/CG
Sample : PB138016BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138016BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------