
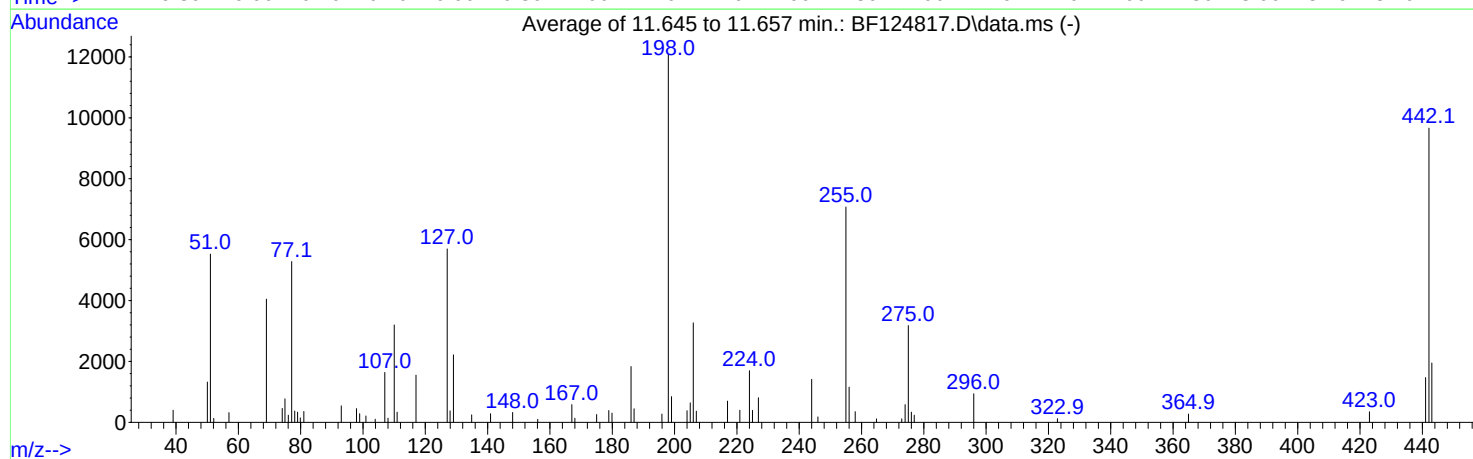


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072821\
 Data File : BF124817.D
 Acq On : 28 Jul 2021 9:07
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 22 15:28:57 2021



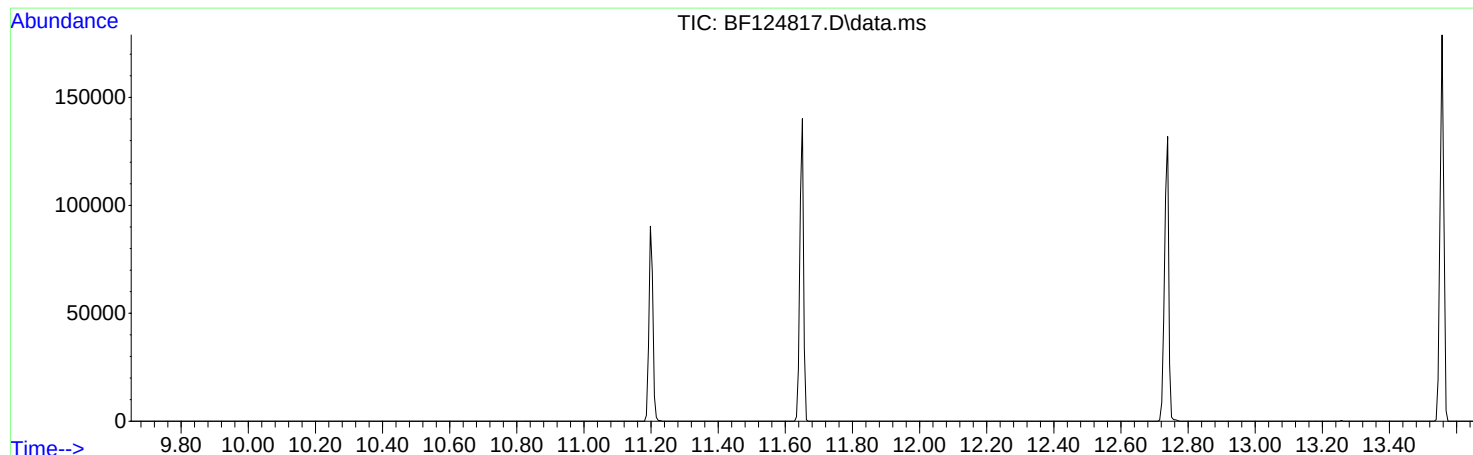


AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.8	5529	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.5	4043	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.2	5695	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12078	PASS
199	198	5	9	7.0	846	PASS
275	198	10	60	26.3	3178	PASS
365	198	1	100	2.3	273	PASS
441	198	0.01	100	12.2	1470	PASS
442	442	50	100	100.0	9662	PASS
443	442	15	24	20.2	1949	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 28 10:59:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

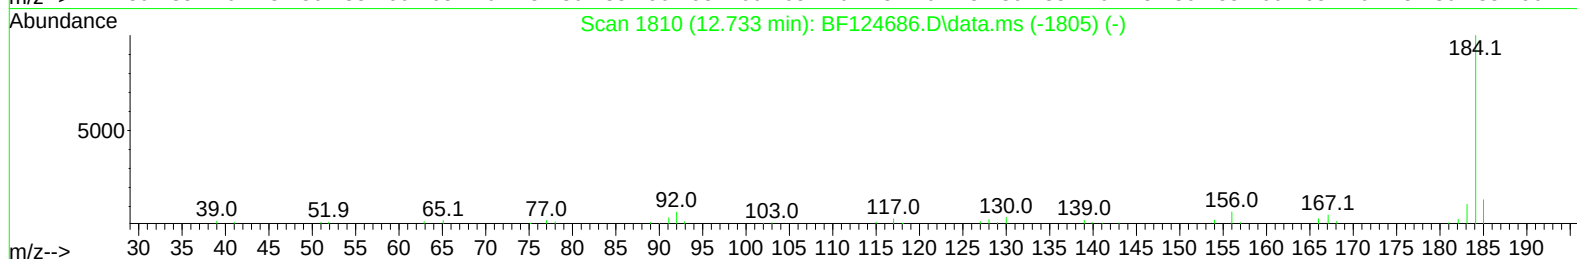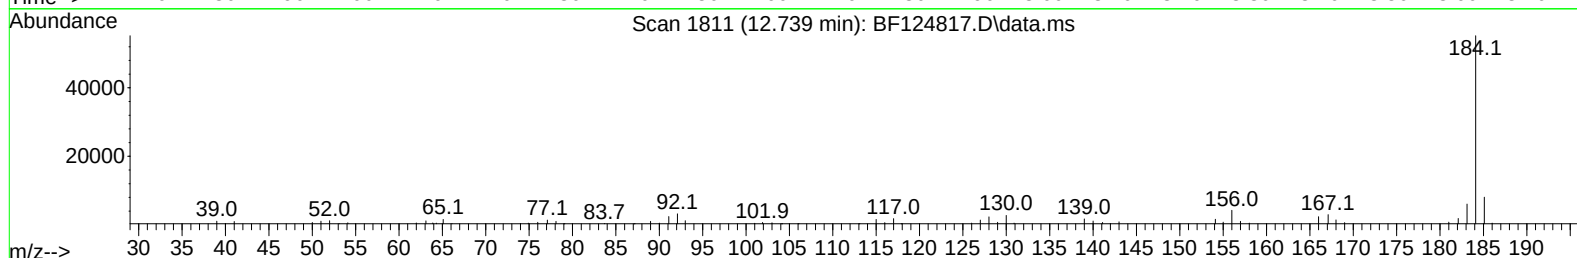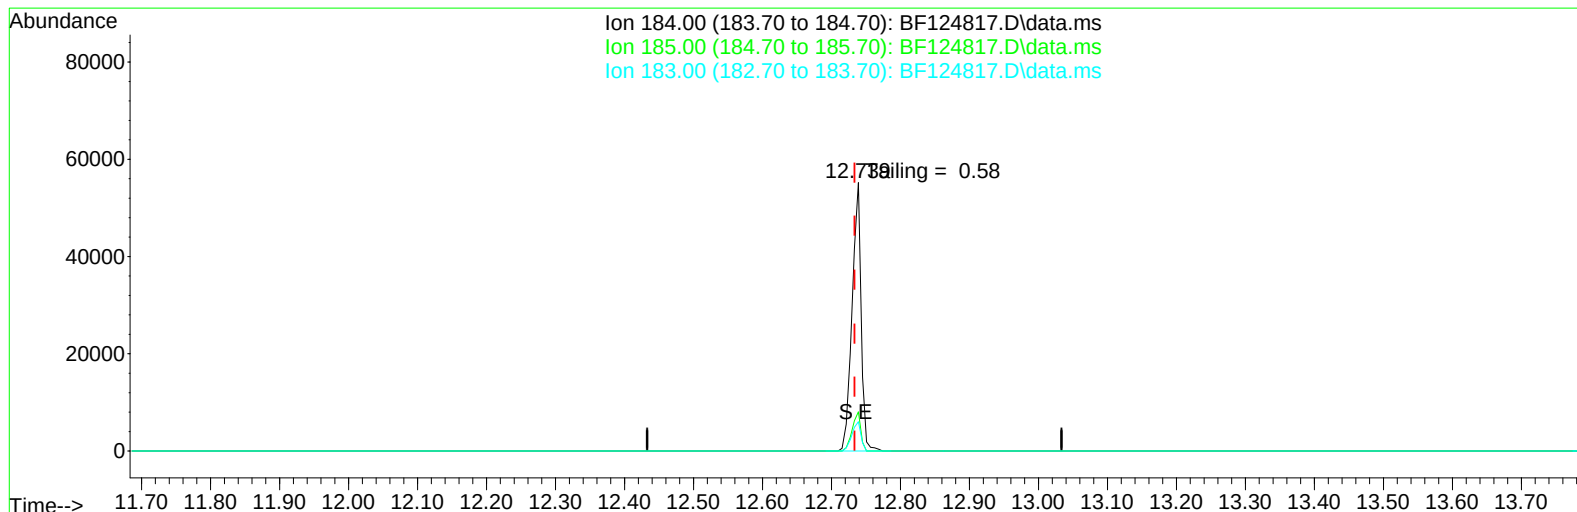

TIC: BF124817.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 0.00 ng




response **50064**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.60
183.00	10.10	10.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072821\
Data File : BF124817.D
Acq On : 28 Jul 2021 9:07
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 28 10:59:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 15:28:57 2021
Response via : Initial Calibration

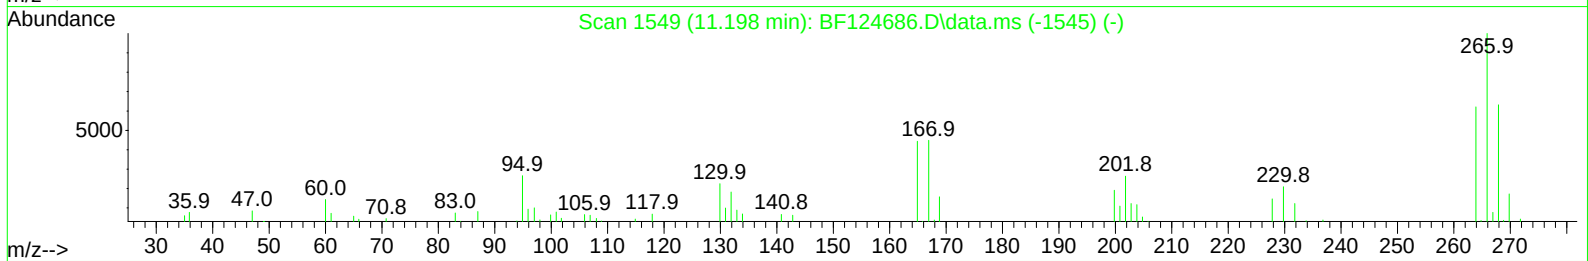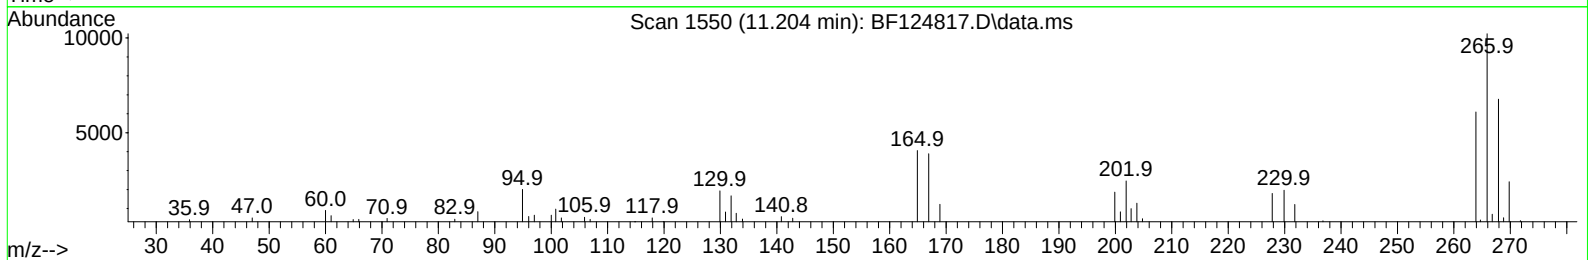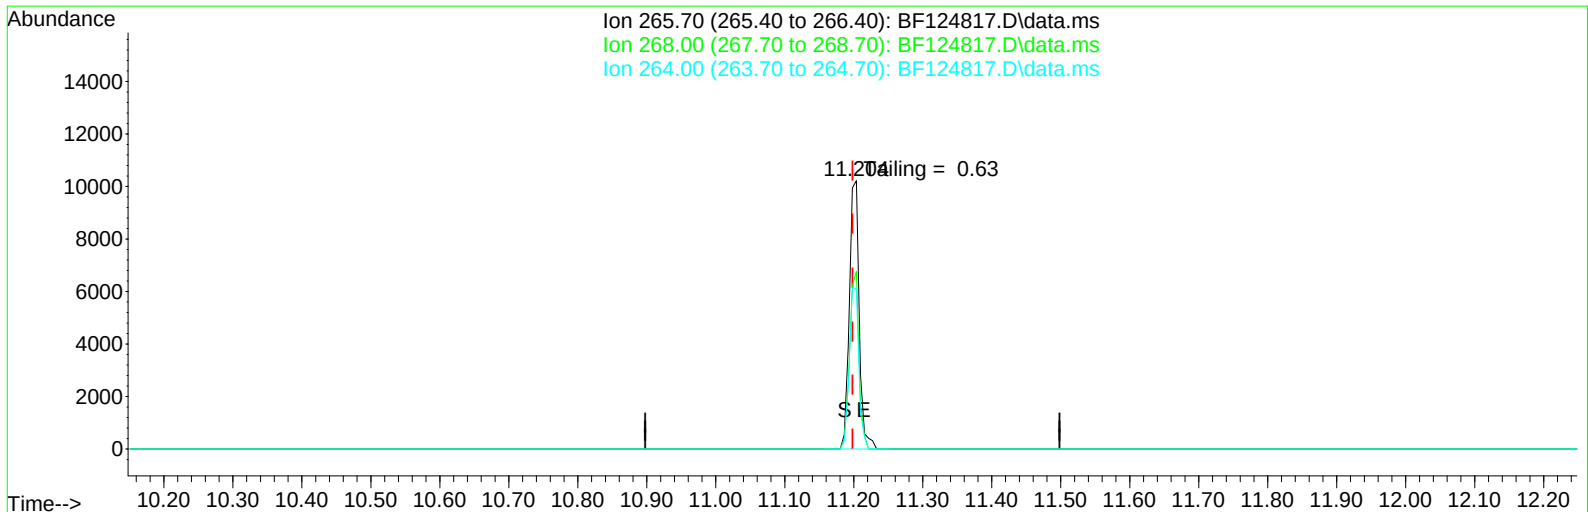

TIC: BF124817.D\data.ms

(70) Pentachlorophenol (C)

11.204min (+ 0.006) 0.00 ng

response 10127

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	66.19
264.00	69.90	63.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/28/2021	BNA_F	<u>BF124817.D</u>
Compound Name	Response	Retention Time
DDT	28490	13.55
DDD	132	13.25
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
132	28622	0.46