
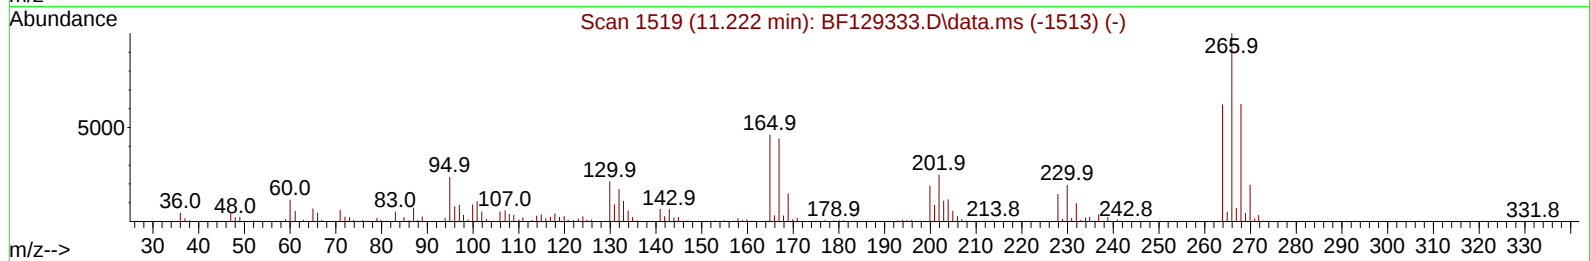
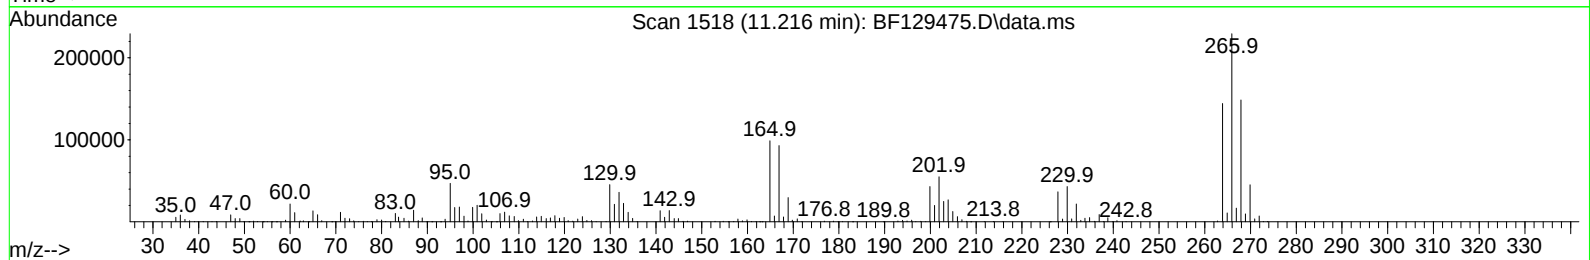


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080122\
 Data File : BF129475.D
 Acq On : 01 Aug 2022 16:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 09:09:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 01:11:25 2022
 Response via : Initial Calibration

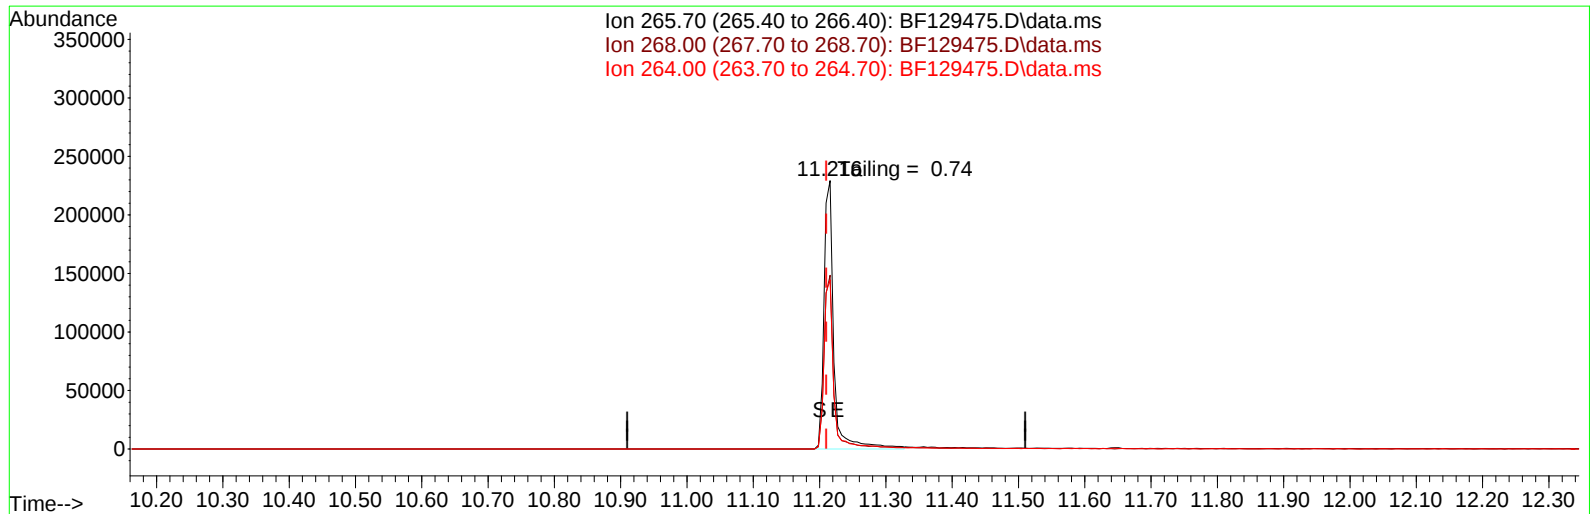

TIC: BF129475.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.006) 414639.08 ng

response 238030

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.78
264.00	61.80	62.96
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080122\  
Data File : BF129475.D  
Acq On    : 01 Aug 2022  16:05  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Aug 02 09:09:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

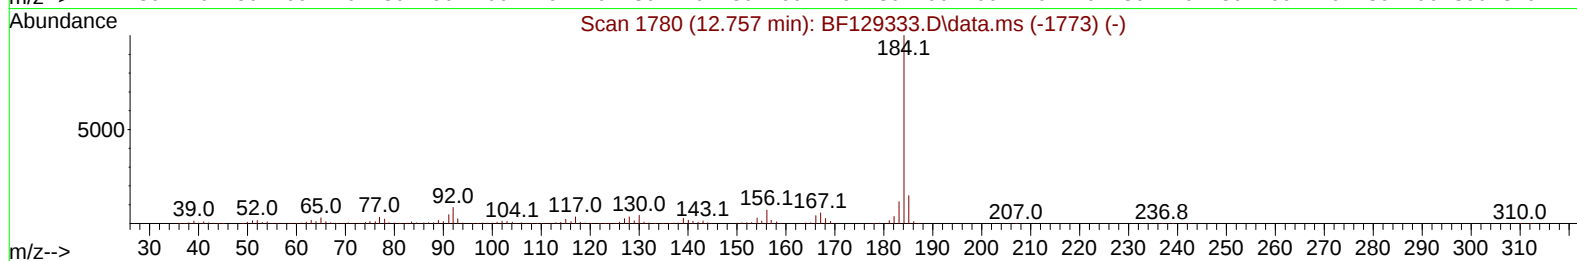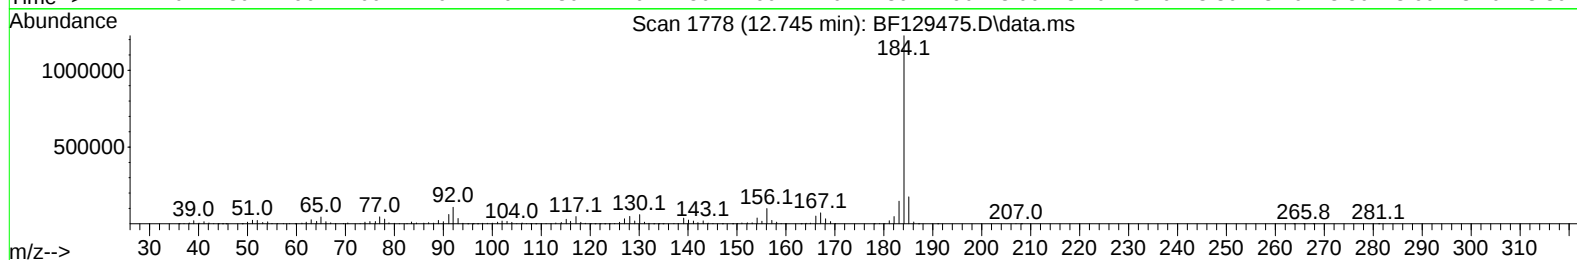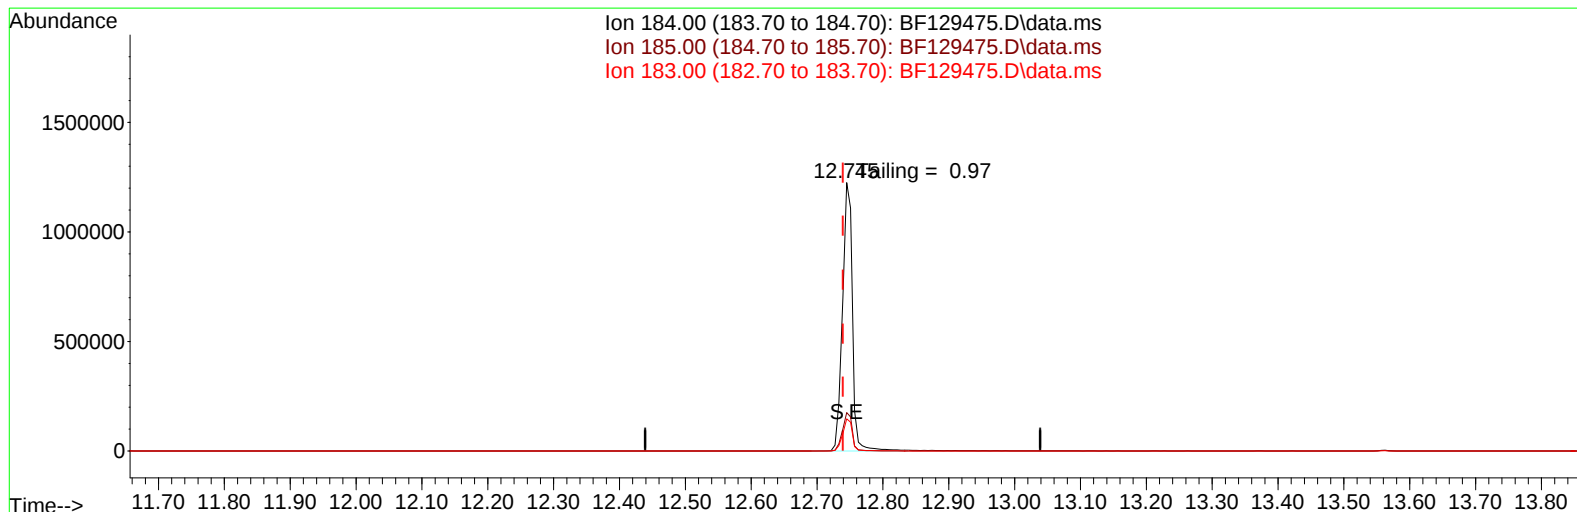

TIC: BF129475.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 53874.78 ng

```
response      1284702
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.30
183.00	11.60	11.99
0.00	0.00	0.00