

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080122\
 Data File : BF129495.D
 Acq On : 02 Aug 2022 02:46
 Operator : CG\JU
 Sample : N3976-03 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP2-0729

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 08/02/2022
 Supervised By : Jagrut Upadhyay 08/02/2022

Quant Time: Aug 02 03:57:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 01:11:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	163574	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	554857	20.000	ng	0.00
39) Acenaphthene-d10	9.916	164	250005	20.000	ng	0.00
64) Phenanthrene-d10	11.410	188	437198	20.000	ng	0.00
76) Chrysene-d12	14.051	240	323500	20.000	ng	0.00
86) Perylene-d12	15.545	264	238140	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	93668	9.328	ng	0.00
7) Phenol-d6	6.522	99	105099	8.327	ng	0.00
23) Nitrobenzene-d5	7.434	82	55911	5.501	ng	-0.01
42) 2,4,6-Tribromophenol	10.710	330	19124	7.956	ng	0.00
45) 2-Fluorobiphenyl	9.233	172	98604	6.101	ng	0.00
79) Terphenyl-d14	12.986	244	107214	6.252	ng	0.00
Target Compounds					Qvalue	
52) Acenaphthene	9.945	154	31550	2.155	ng	96
71) Phenanthrene	11.433	178	247933	10.389	ng	97
72) Anthracene	11.480	178	67896	2.895	ng	100
75) Fluoranthene	12.621	202	521621	21.571	ng	99
78) Pyrene	12.857	202	525102	19.411	ng	98
81) Benzo(a)anthracene	14.045	228	361028	16.337	ng	99
83) Chrysene	14.080	228	355866	17.087	ng	97
87) Indeno(1,2,3-cd)pyrene	17.051	276	267670	16.691	ng	95
88) Benzo(b)fluoranthene	15.104	252	519046m	32.858	ng	
89) Benzo(k)fluoranthene	15.127	252	173675m	11.219	ng	
90) Benzo(a)pyrene	15.480	252	398181	31.051	ng	97
91) Dibenzo(a,h)anthracene	17.051	278	70208	5.379	ng	# 88
92) Benzo(g,h,i)perylene	17.509	276	272770	20.452	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080122\
Data File : BF129495.D
Acq On : 02 Aug 2022 02:46
Operator : CG\JU
Sample : N3976-03 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP2-0729

Quant Time: Aug 02 03:57:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 08/02/2022
Supervised By : Jagrut Upadhyay 08/02/2022

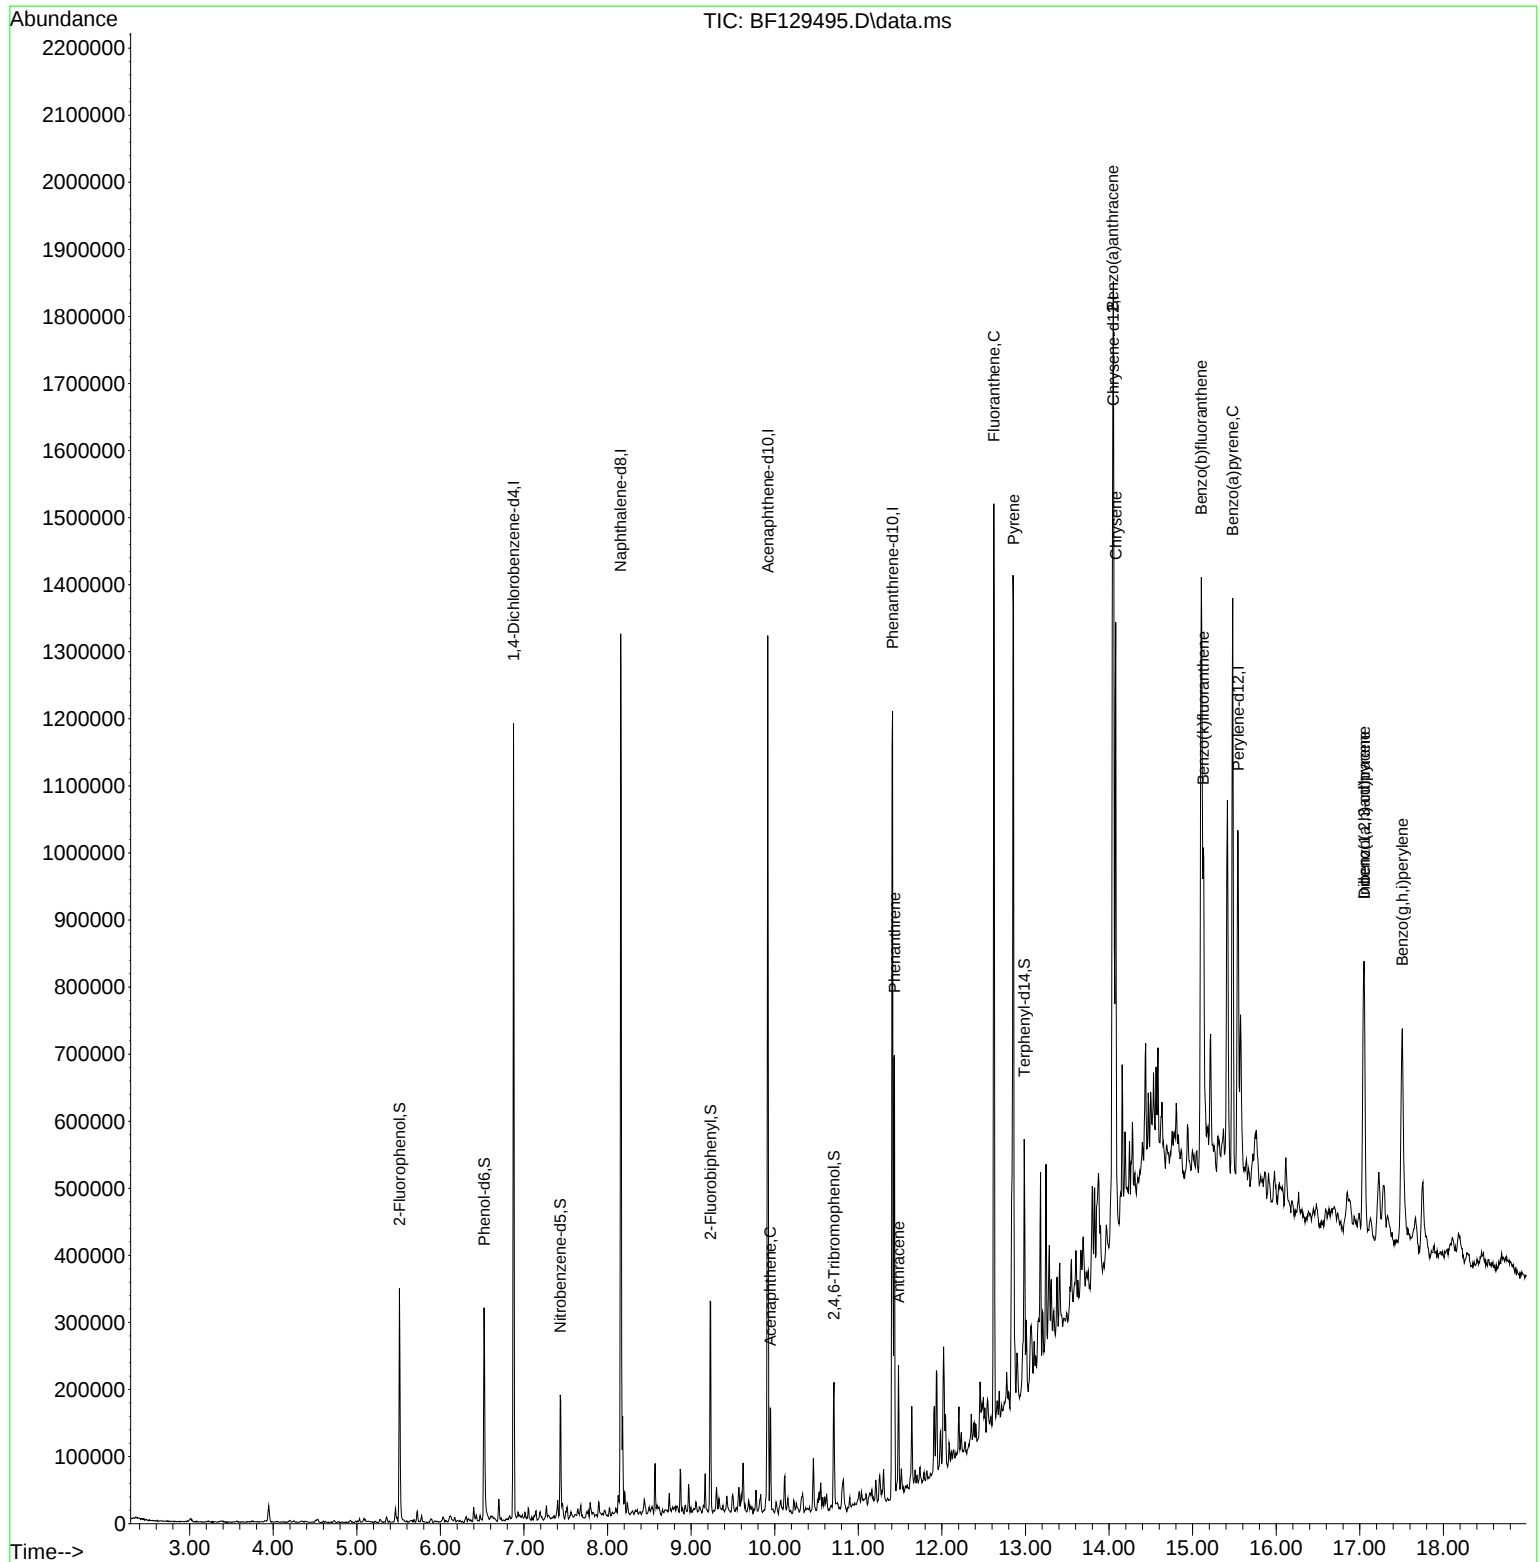



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 782
Delta R.T. -0.000 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46




Instrument :
BNA_F
ClientSampleId :
TP2-0729



Tgt Ion:152 Resp: 163574
Ion Ratio Lower Upper
152 100
150 156.8 123.7 185.5
115 65.2 49.9 74.9




Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 08/02/2022
Supervised By :Jagrut Upadhyay 08/02/2022

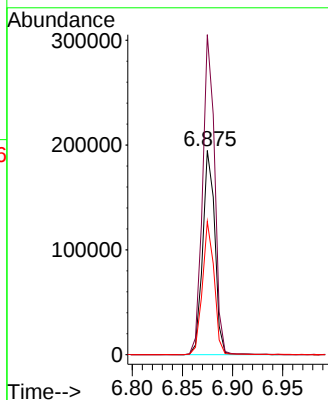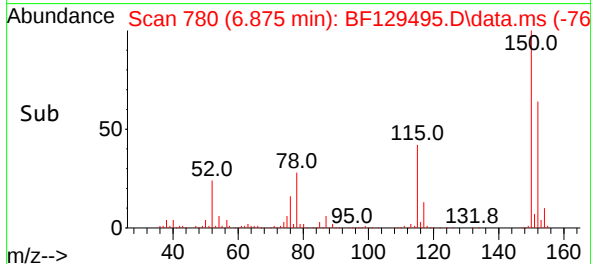

#5
2-Fluorophenol
Concen: 9.328 ng
RT: 5.510 min Scan# 548
Delta R.T. 0.006 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46


Tgt Ion:112 Resp: 93668
Ion Ratio Lower Upper
112 100
64 60.5 53.3 79.9
63 30.6 28.0 42.0

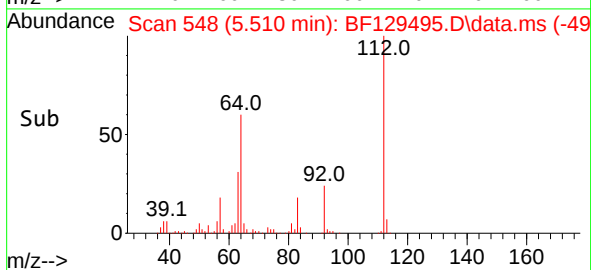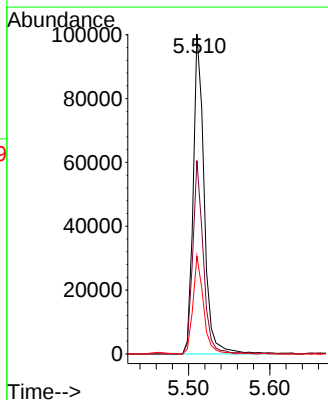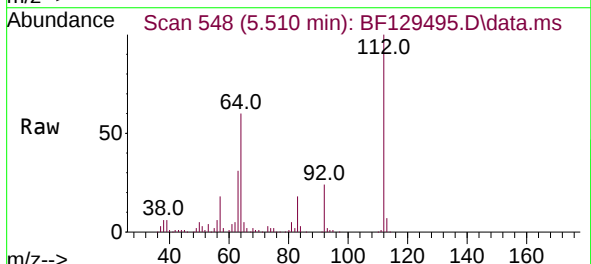



#7
Phenol-d6
Concen: 8.327 ng
RT: 6.522 min Scan# 719
Delta R.T. -0.000 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46




Instrument :
BNA_F
ClientSampleId :
TP2-0729




Tgt Ion: 99 Resp: 105099
Ion Ratio Lower Upper
99 100
42 19.1 17.3 25.9
71 33.4 28.9 43.3

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 08/02/2022
Supervised By :Jagrut Upadhyay 08/02/2022

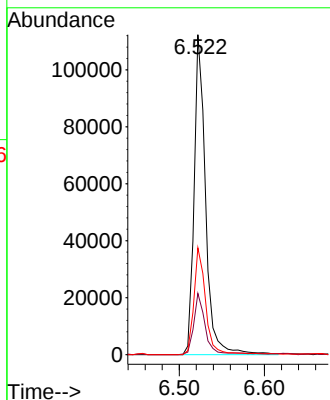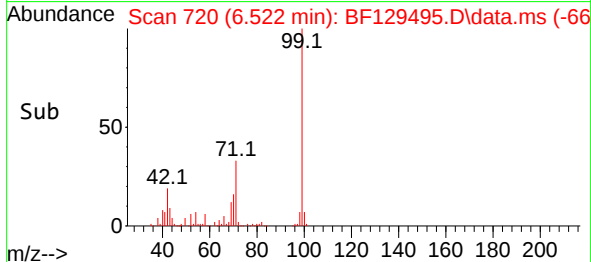


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 998
Delta R.T. -0.006 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46

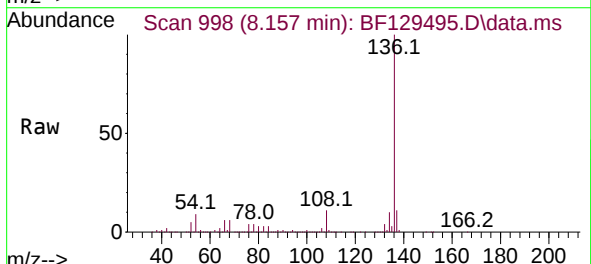

Tgt Ion:136 Resp: 554857
Ion Ratio Lower Upper
136 100
137 11.3 8.8 13.2
54 8.6 7.5 11.3
68 6.2 4.7 7.1

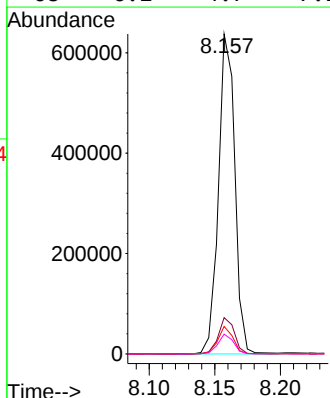







#23
Nitrobenzene-d5
Concen: 5.501 ng
RT: 7.434 min Scan# 81
Delta R.T. -0.012 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46

Instrument :
BNA_F
ClientSampleId :
TP2-0729

Tgt Ion: 82 Resp: 5591
Ion Ratio Lower Upper
82 100
128 40.1 34.0 51.0
54 54.4 46.9 70.3




Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 08/02/2022
Supervised By :Jagrut Upadhyay 08/02/2022

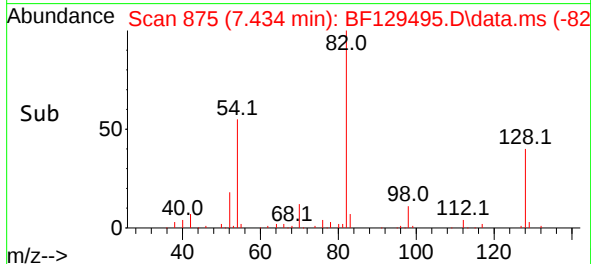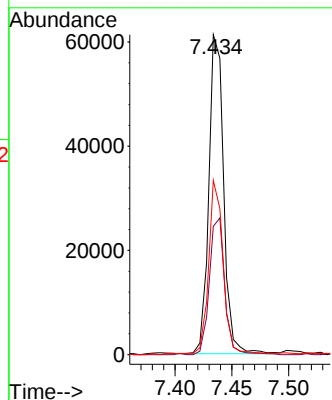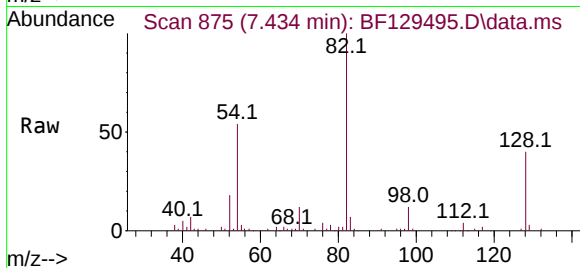

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.916 min Scan# 1297
Delta R.T. -0.000 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46

Tgt Ion:164 Resp: 250005
Ion Ratio Lower Upper
164 100
162 100.8 79.5 119.3
160 43.7 34.2 51.4

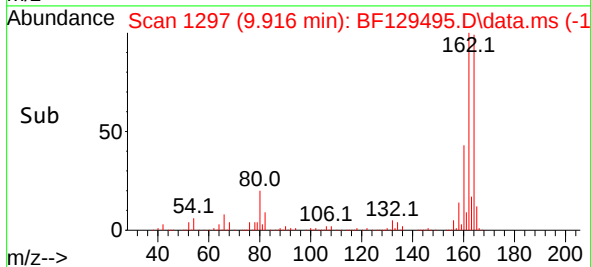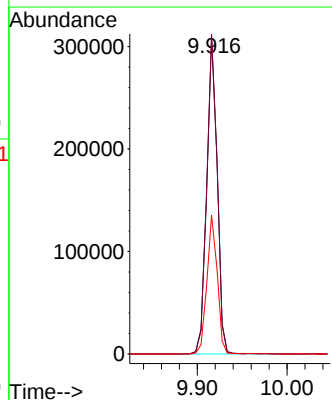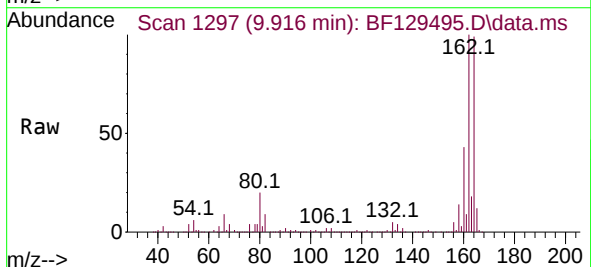



#42
2,4,6-Tribromophenol
Concen: 7.956 ng
RT: 10.710 min Scan# 1434
Delta R.T. -0.000 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46

Instrument :

BNA_F

ClientSampleId :





TP2-0729

Tgt Ion: 330 Resp: 19124
Ion Ratio Lower Upper
330 100
332 103.0 76.8 115.2
141 39.5 28.0 42.0

Manual Integrations




APPROVED


Reviewed By : Christian Giraldo 08/02/2022
Supervised By : Jagrut Upadhyay 08/02/2022

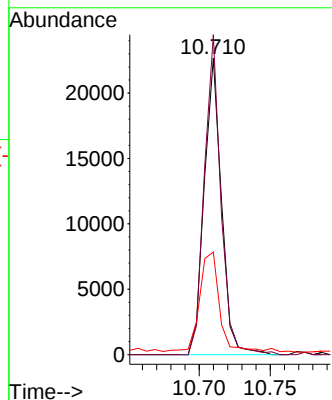

#45
2-Fluorobiphenyl
Concen: 6.101 ng
RT: 9.233 min Scan# 1181
Delta R.T. -0.000 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46


Tgt Ion: 172 Resp: 98604
Ion Ratio Lower Upper
172 100
171 34.2 28.8 43.2
170 23.1 19.8 29.8

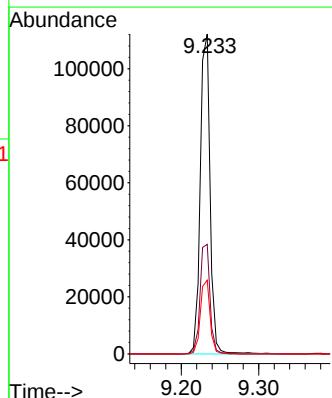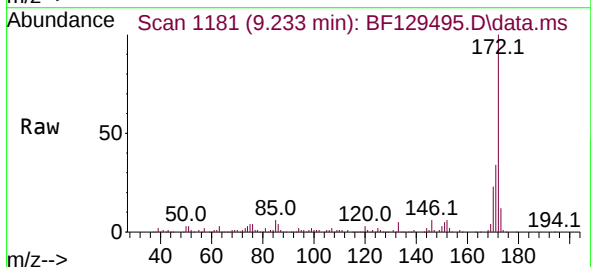



#52
Acenaphthene
Concen: 2.155 ng
RT: 9.945 min Scan# 1305
Delta R.T. -0.006 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46




Instrument :
BNA_F
ClientSampleId :
TP2-0729




Tgt Ion:154 Resp: 31550
Ion Ratio Lower Upper
154 100
153 107.5 89.6 134.4
152 50.1 42.4 63.6

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 08/02/2022
Supervised By :Jagrut Upadhyay 08/02/2022

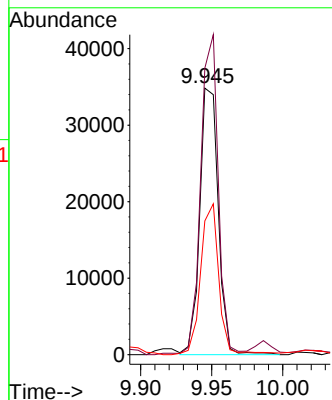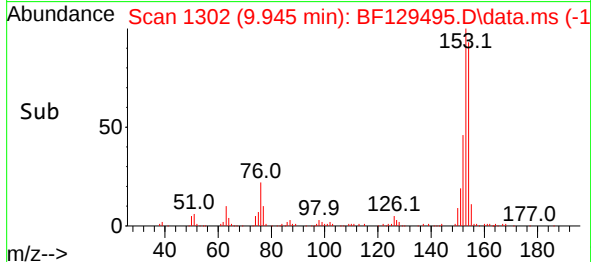


#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.410 min Scan# 1551
Delta R.T. 0.006 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46

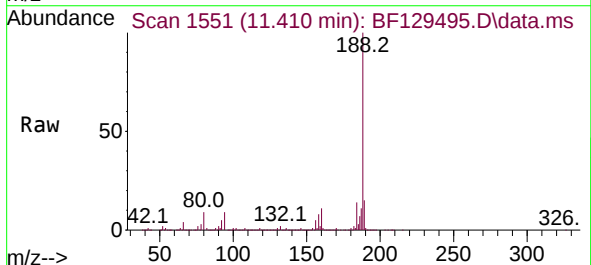

Tgt Ion:188 Resp: 437198
Ion Ratio Lower Upper
188 100
94 8.7 7.0 10.6
80 9.5 7.6 11.4

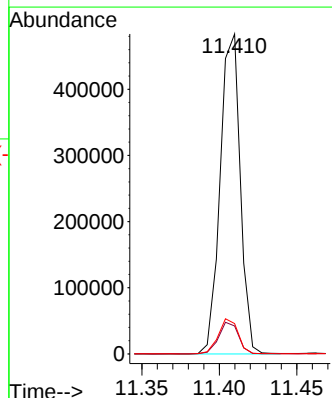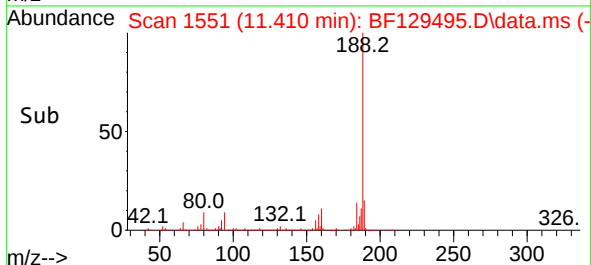

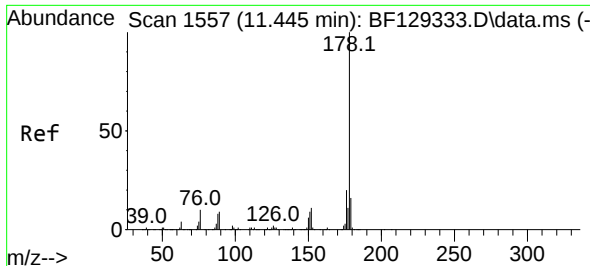





#71
Phenanthrene
Concen: 10.389 ng
RT: 11.433 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46

Instrument :
BNA_F
ClientSampleId :
TP2-0729

Tgt Ion:178 Resp: 247933
Ion Ratio Lower Upper
178 100
176 18.6 16.0 24.0
179 15.0 12.6 19.0




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 08/02/2022
Supervised By :Jagrut Upadhyay 08/02/2022

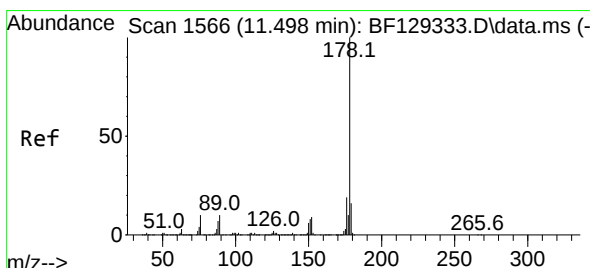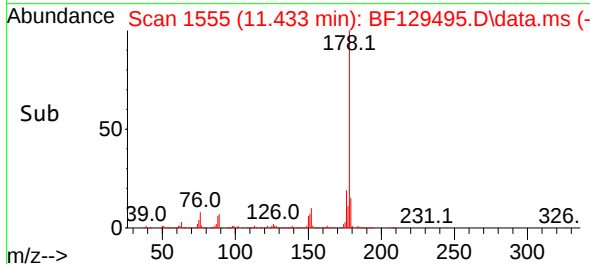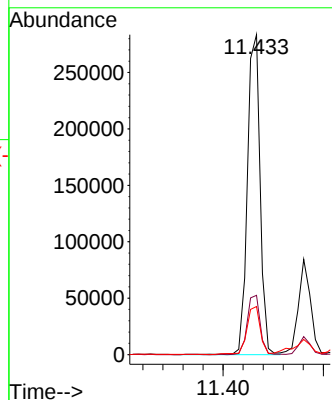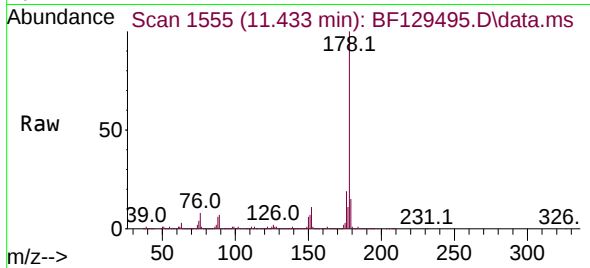

#72
Anthracene
Concen: 2.895 ng
RT: 11.480 min Scan# 1563
Delta R.T. -0.000 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46


Tgt Ion:178 Resp: 67896
Ion Ratio Lower Upper
178 100
176 19.0 15.4 23.2
179 15.9 12.6 19.0

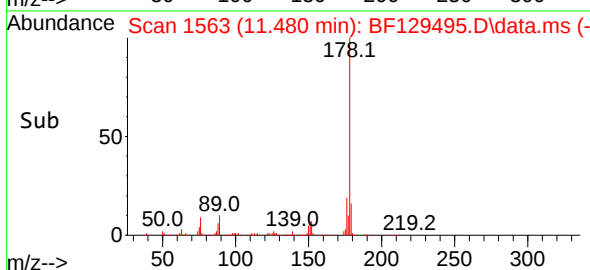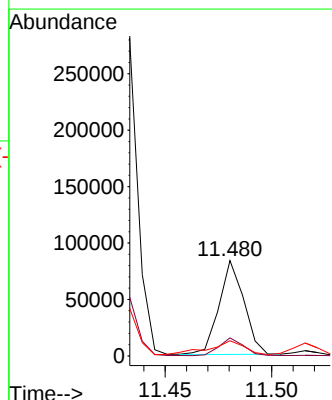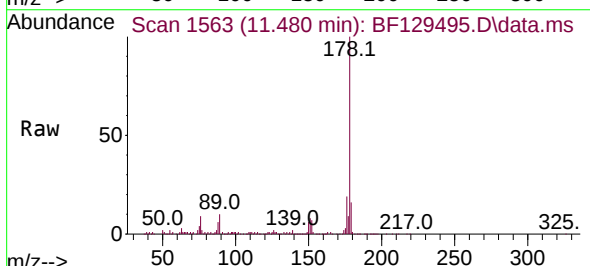



#75
Fluoranthene
Concen: 21.571 ng
RT: 12.621 min Scan# 1759
Delta R.T. -0.000 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46




Instrument :
BNA_F
ClientSampleId :
TP2-0729



Tgt Ion:202 Resp: 521621
Ion Ratio Lower Upper
202 100
101 12.0 0.0 31.4
203 17.8 0.0 38.0




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 08/02/2022
Supervised By :Jagrut Upadhyay 08/02/2022

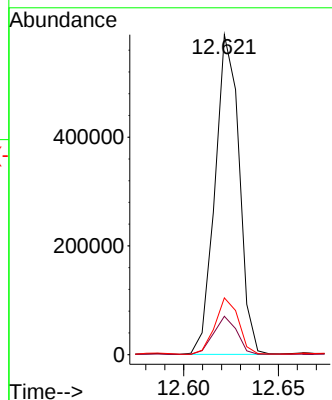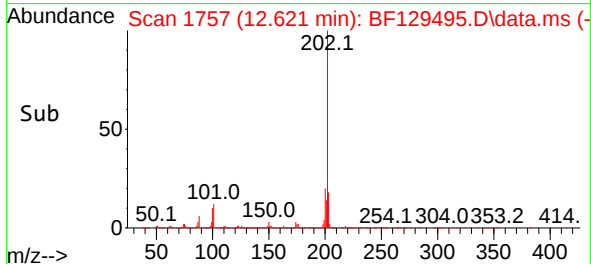

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.051 min Scan# 2000
Delta R.T. -0.000 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46

Tgt Ion:240 Resp: 323500
Ion Ratio Lower Upper
240 100
120 12.7 8.9 13.3
236 25.4 20.8 31.2

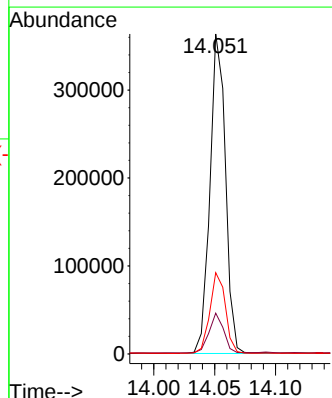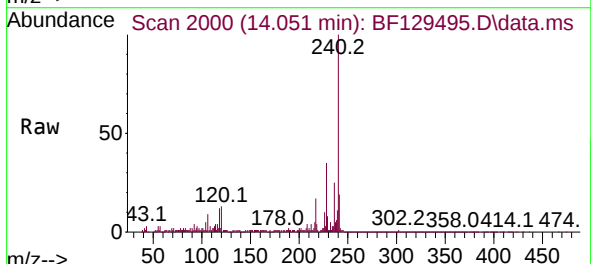



#78

Pyrene

Concen: 19.411 ng

RT: 12.857 min Scan# 11

Delta R.T. 0.006 min

Lab File: BF129495.D

Acq: 02 Aug 2022 02:46

Instrument :

BNA_F

ClientSampleId :





TP2-0729

Tgt Ion:202 Resp: 525102
 Ion Ratio Lower Upper
 202 100
 200 20.7 17.7 26.5
 203 18.0 14.6 21.8

Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 08/02/2022
 Supervised By :Jagrut Upadhyay 08/02/2022

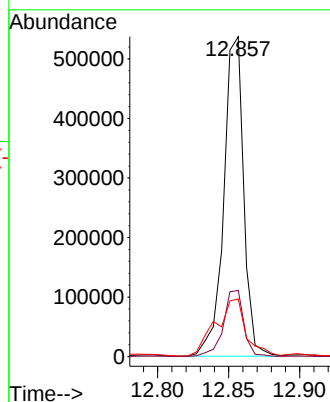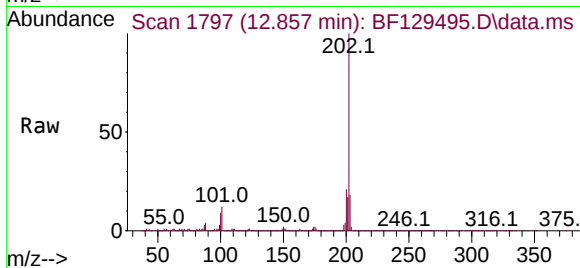

#79

Terphenyl-d14

Concen: 6.252 ng




RT: 12.986 min Scan# 1819


Delta R.T. -0.000 min

Lab File: BF129495.D

Acq: 02 Aug 2022 02:46


Tgt Ion:244 Resp: 107214
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.1 9.1
 122 12.9 8.8 13.2

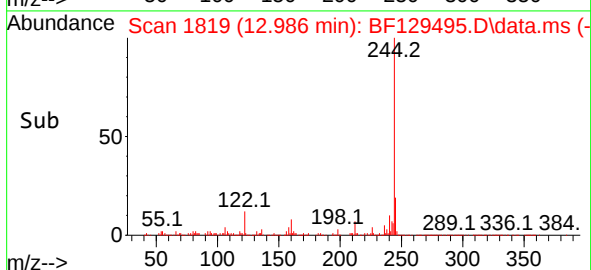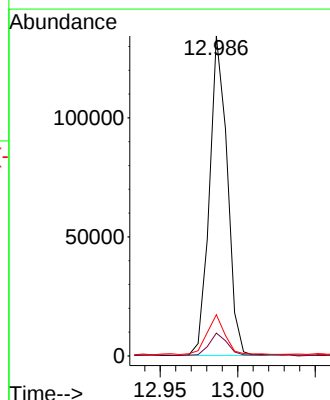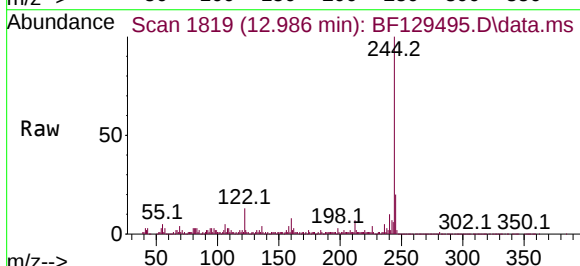



#81
Benzo(a)anthracene
Concen: 16.337 ng
RT: 14.045 min Scan# 19
Delta R.T. 0.006 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46




Instrument :
BNA_F
ClientSampleId :
TP2-0729




Tgt Ion:228 Resp: 361028
Ion Ratio Lower Upper
228 100
226 27.6 22.1 33.1
229 20.3 15.8 23.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 08/02/2022
Supervised By :Jagrut Upadhyay 08/02/2022

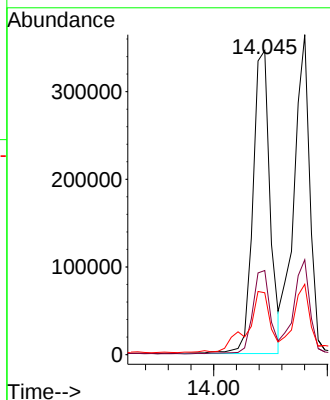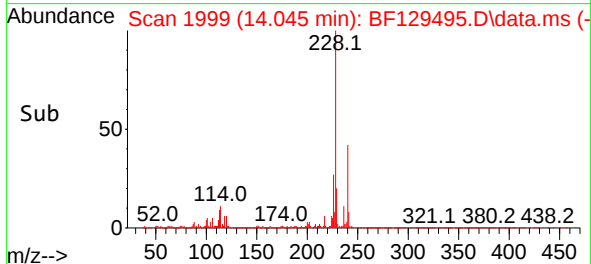


#83
Chrysene
Concen: 17.087 ng
RT: 14.080 min Scan# 2005
Delta R.T. 0.006 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46

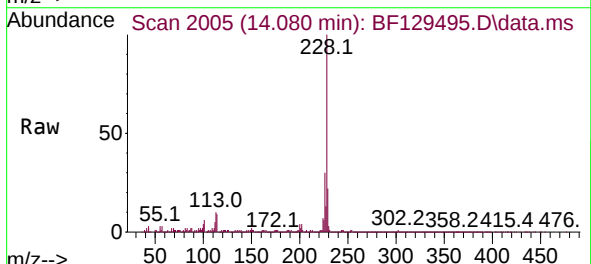


Tgt Ion:228 Resp: 355866
Ion Ratio Lower Upper
228 100
226 29.6 24.3 36.5
229 22.0 15.9 23.9

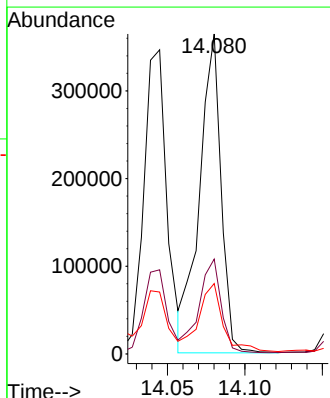



#86
Perylene-d12
Concen: 20.000 ng
RT: 15.545 min Scan# 21
Delta R.T. 0.018 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46




Instrument :
BNA_F
ClientSampleId :
TP2-0729




Tgt Ion:264 Resp: 238140
Ion Ratio Lower Upper
264 100
260 23.5 18.4 27.6
265 23.3 17.2 25.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 08/02/2022
Supervised By :Jagrut Upadhyay 08/02/2022

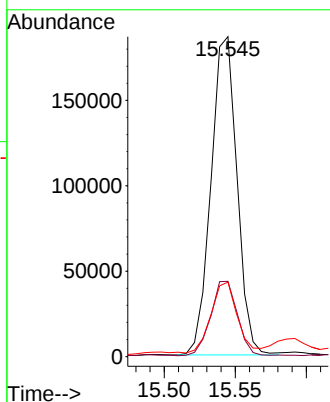


#87
Indeno(1,2,3-cd)pyrene
Concen: 16.691 ng
RT: 17.051 min Scan# 2510
Delta R.T. 0.018 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46



Tgt Ion:276 Resp: 267670
Ion Ratio Lower Upper
276 100
138 22.3 21.1 31.7
277 24.8 20.3 30.5

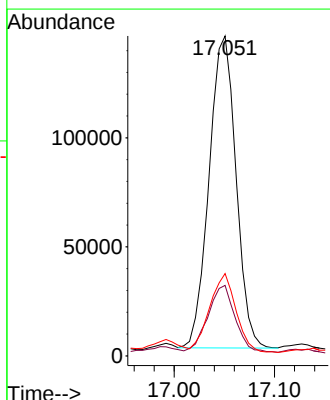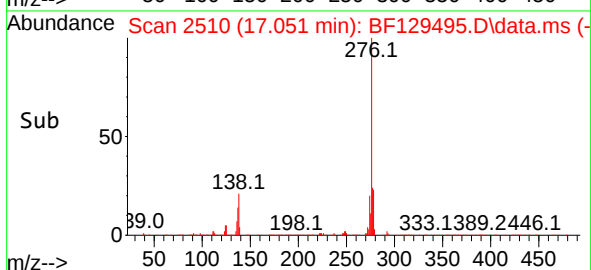

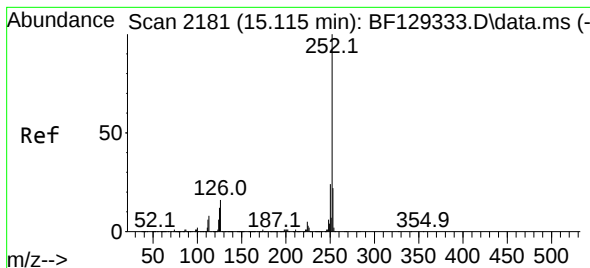

#88

Benzo(b)fluoranthene

Concen: 32.858 ng m

RT: 15.104 min Scan# 2181

Delta R.T. 0.012 min

Lab File: BF129495.D

Acq: 02 Aug 2022 02:46

Instrument :

BNA_F

ClientSampleId :

TP2-0729

Tgt Ion:252 Resp: 519046

Ion Ratio Lower Upper

252 100

253 22.7 17.7 26.5





125 11.5 8.0 12.0

Manual Integrations

APPROVED

Reviewed By :Christian Giraldo 08/02/2022

Supervised By :Jagrut Upadhyay 08/02/2022

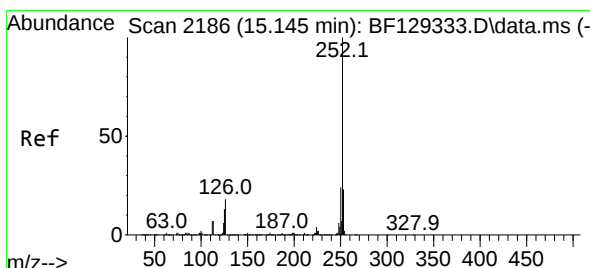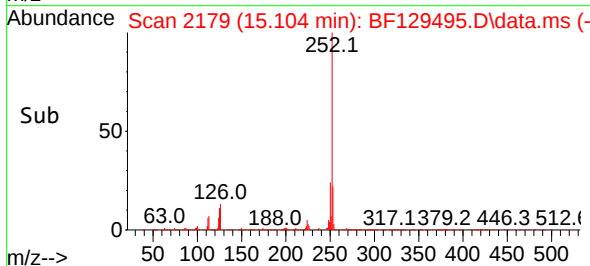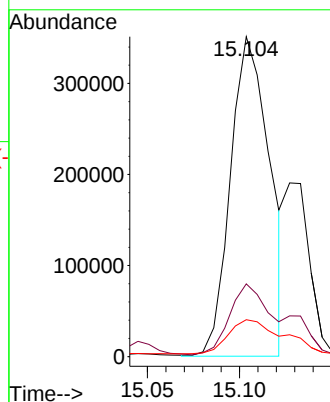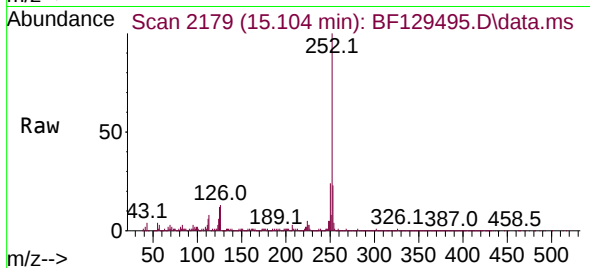

#89

Benzo(k)fluoranthene

Concen: 11.219 ng m

RT: 15.127 min Scan# 2183

Delta R.T. 0.006 min

Lab File: BF129495.D

Acq: 02 Aug 2022 02:46




Tgt Ion:252 Resp: 173675


Ion Ratio Lower Upper

252 100

253 23.5 17.8 26.6

125 12.6 8.3 12.5#

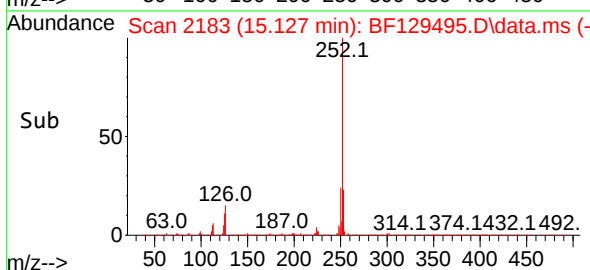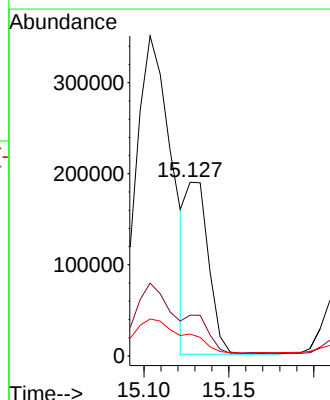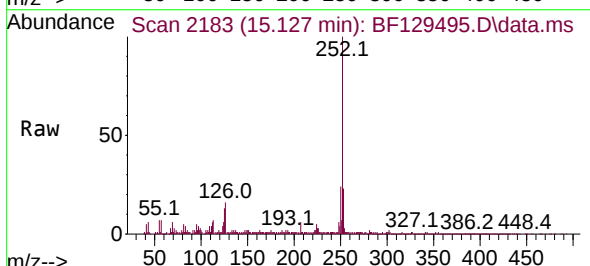



#90
Benzo(a)pyrene
Concen: 31.051 ng
RT: 15.480 min Scan# 21
Delta R.T. 0.012 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46

Instrument :

BNA_F

ClientSampleId :





TP2-0729

Tgt Ion:252 Resp: 39818
Ion Ratio Lower Upper
252 100
253 23.3 17.0 25.6
125 11.7 8.8 13.2

Manual Integrations




APPROVED


Reviewed By :Christian Giraldo 08/02/2022
Supervised By :Jagrut Upadhyay 08/02/2022

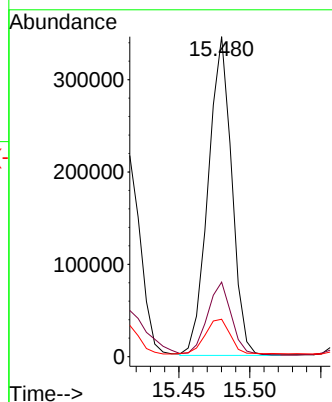

#91
Dibenzo(a,h)anthracene
Concen: 5.379 ng
RT: 17.051 min Scan# 2510
Delta R.T. 0.006 min
Lab File: BF129495.D
Acq: 02 Aug 2022 02:46


Tgt Ion:278 Resp: 70208
Ion Ratio Lower Upper
278 100
139 22.6 12.8 19.2#
279 28.4 18.6 28.0#

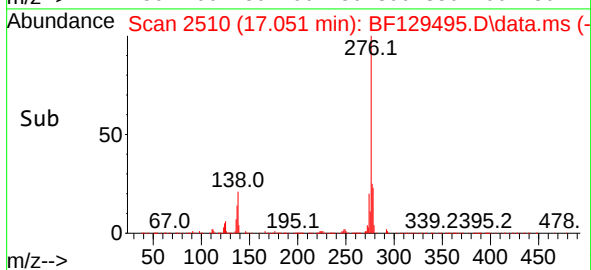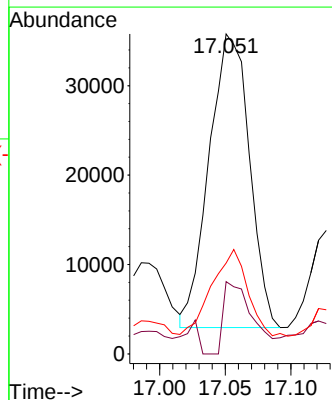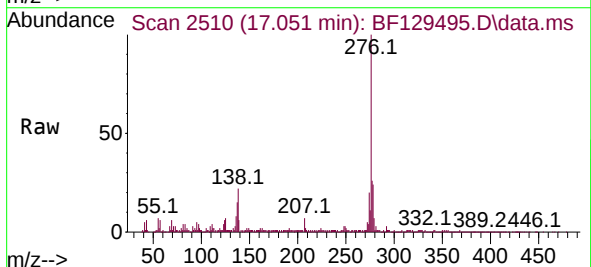



#92
 Benzo(g,h,i)perylene
 Concen: 20.452 ng
 RT: 17.509 min Scan# 2588
 Delta R.T. 0.018 min
 Lab File: BF129495.D
 Acq: 02 Aug 2022 02:46

Instrument :
 BNA_F
 ClientSampleId :
 TP2-0729



Tgt Ion: 276 Resp: 272776

Ion	Ratio	Lower	Upper
276	100		
277	24.1	19.1	28.7
138	21.0	18.0	27.0

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 08/02/2022
 Supervised By : Jagrut Upadhyay 08/02/2022

