


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080122\
 Data File : BF129464.D
 Acq On : 01 Aug 2022 10:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 02 01:11:25 2022

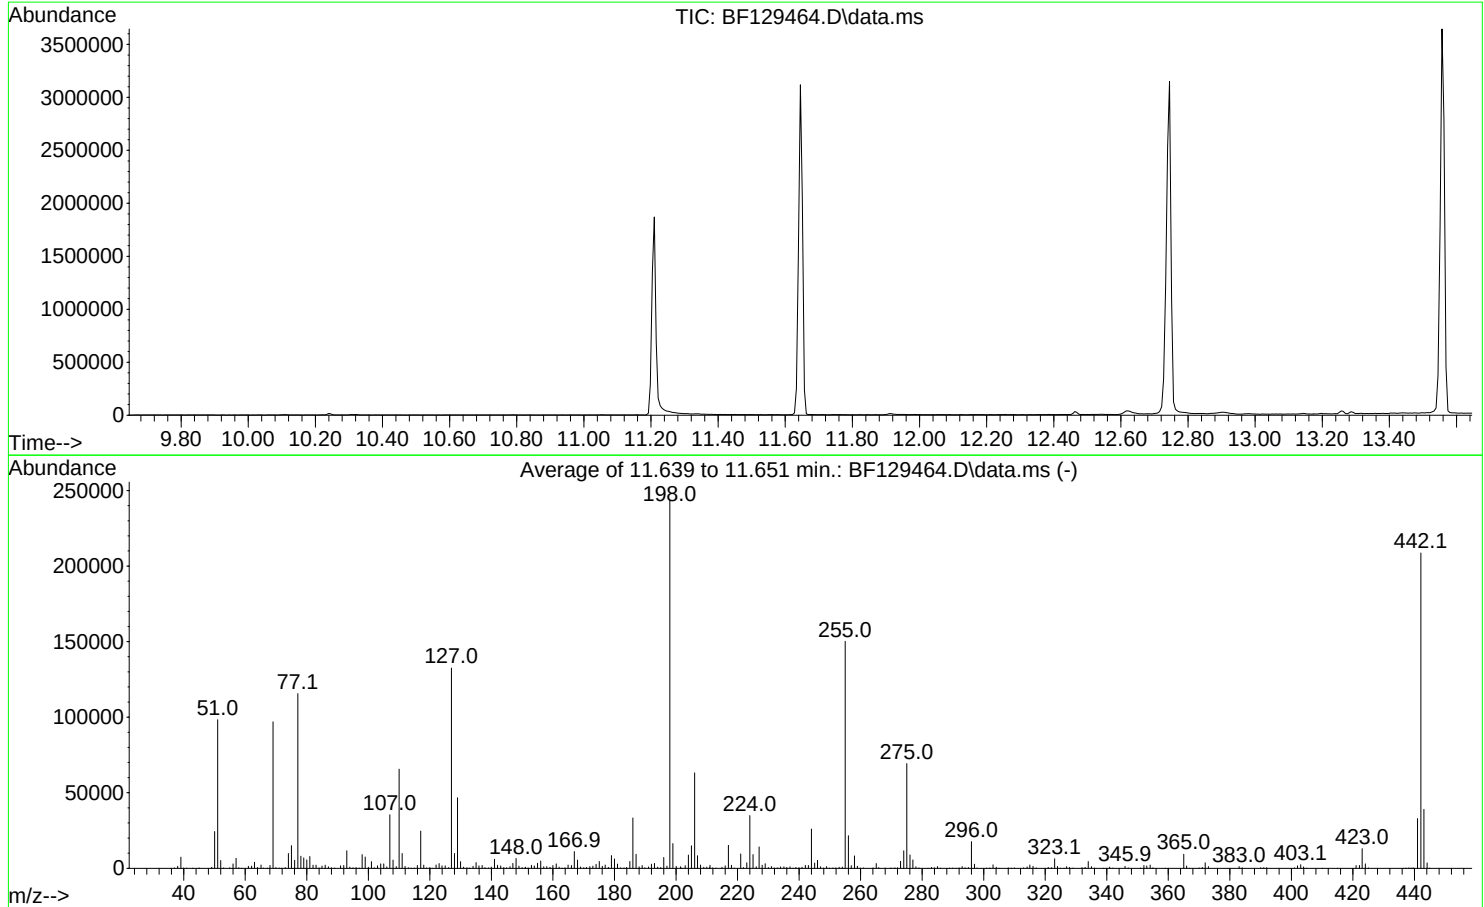




AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	98381	PASS
68	69	0.00	2	2.0	1899	PASS
69	198	0.00	100	39.8	96947	PASS
70	69	0.00	2	0.5	512	PASS
127	198	10	80	54.5	132563	PASS
197	198	0.00	2	0.6	1430	PASS
198	198	100	100	100.0	243456	PASS
199	198	5	9	6.7	16312	PASS
275	198	10	60	28.5	69349	PASS
365	198	1	100	3.8	9297	PASS
441	198	0.01	100	13.5	32897	PASS
442	442	50	100	100.0	208648	PASS
443	442	15	24	18.7	39078	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080122\
 Data File : BF129464.D
 Acq On : 01 Aug 2022 10:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 02 09:08:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 01:11:25 2022
 Response via : Initial Calibration

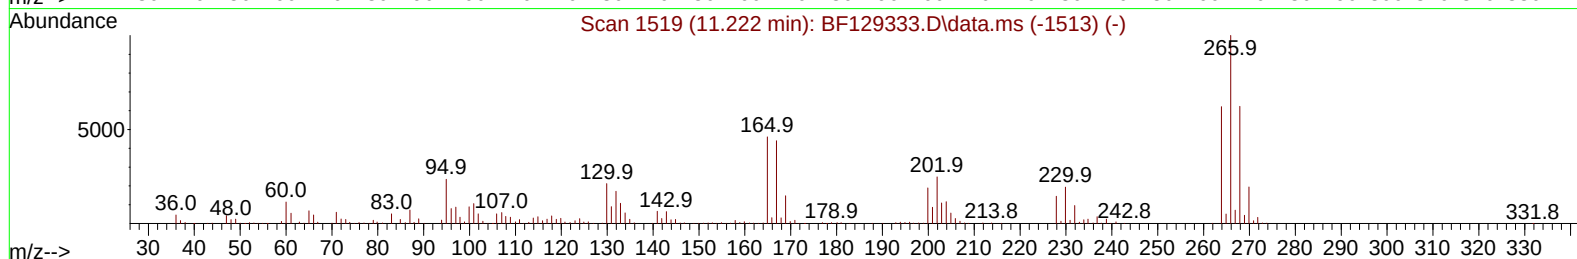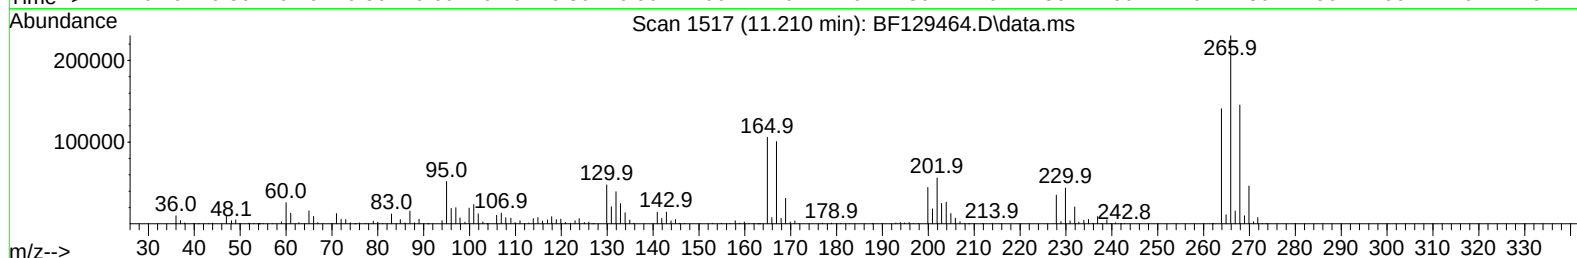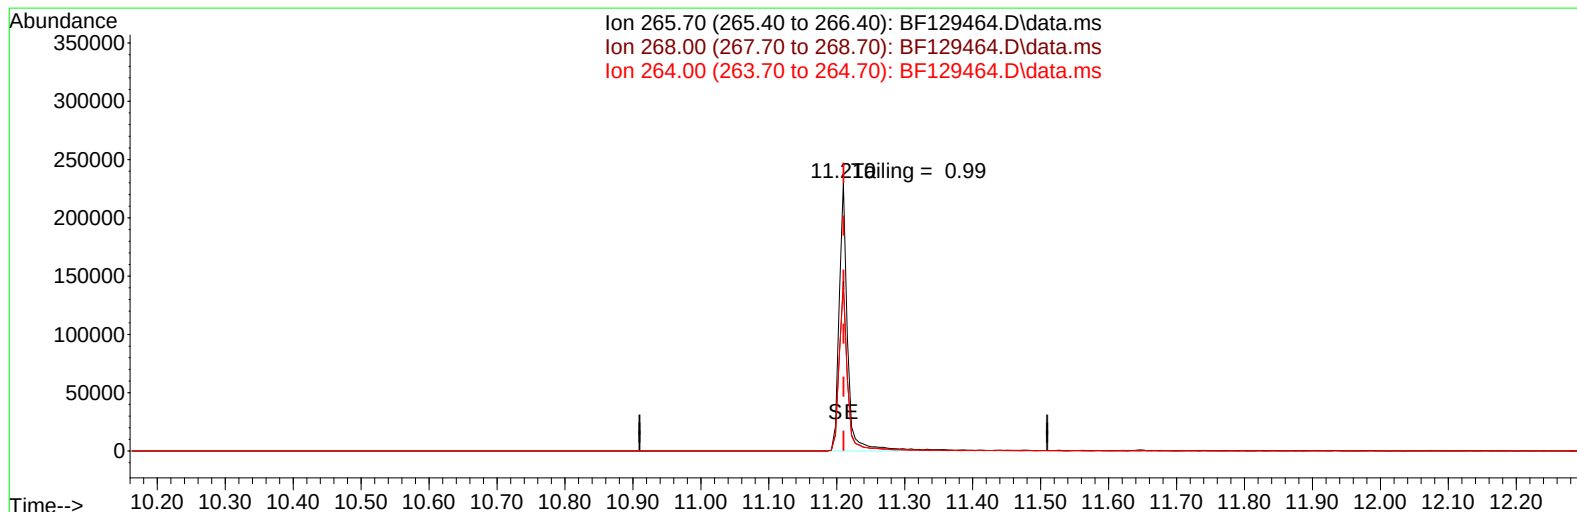

TIC: BF129464.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 554383.89 ng




response 196673

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.14
264.00	61.80	61.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080122\
Data File : BF129464.D
Acq On : 01 Aug 2022 10:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 09:08:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

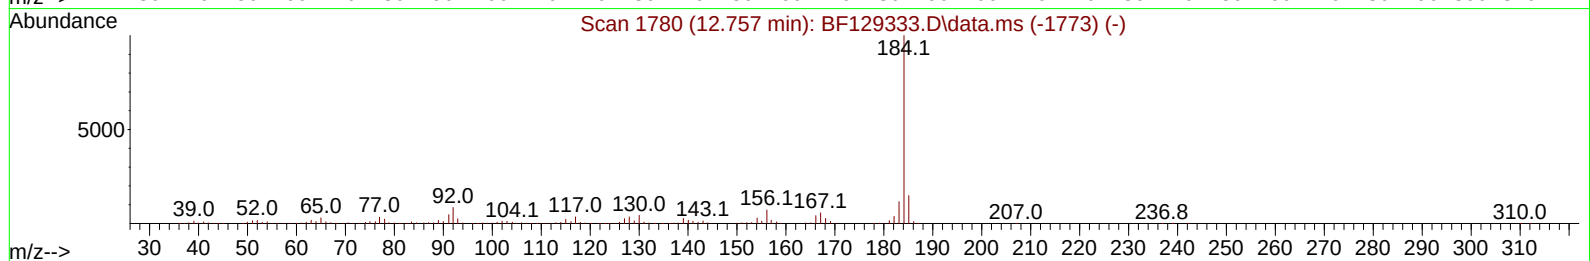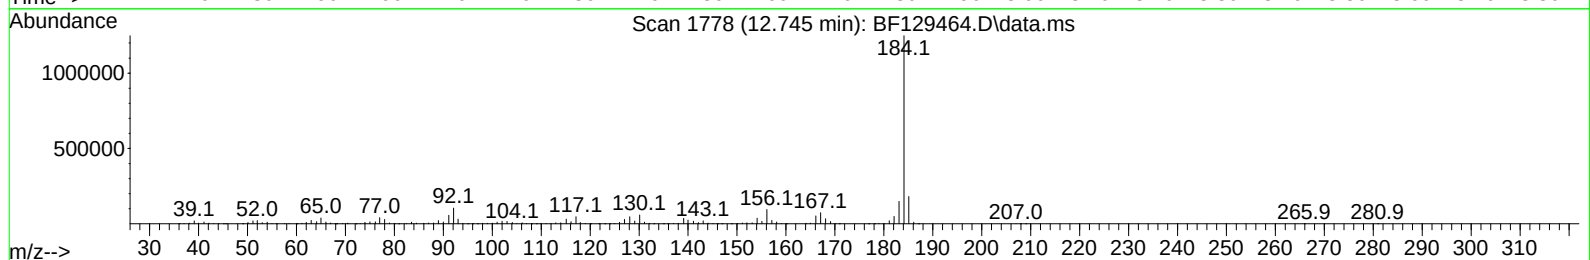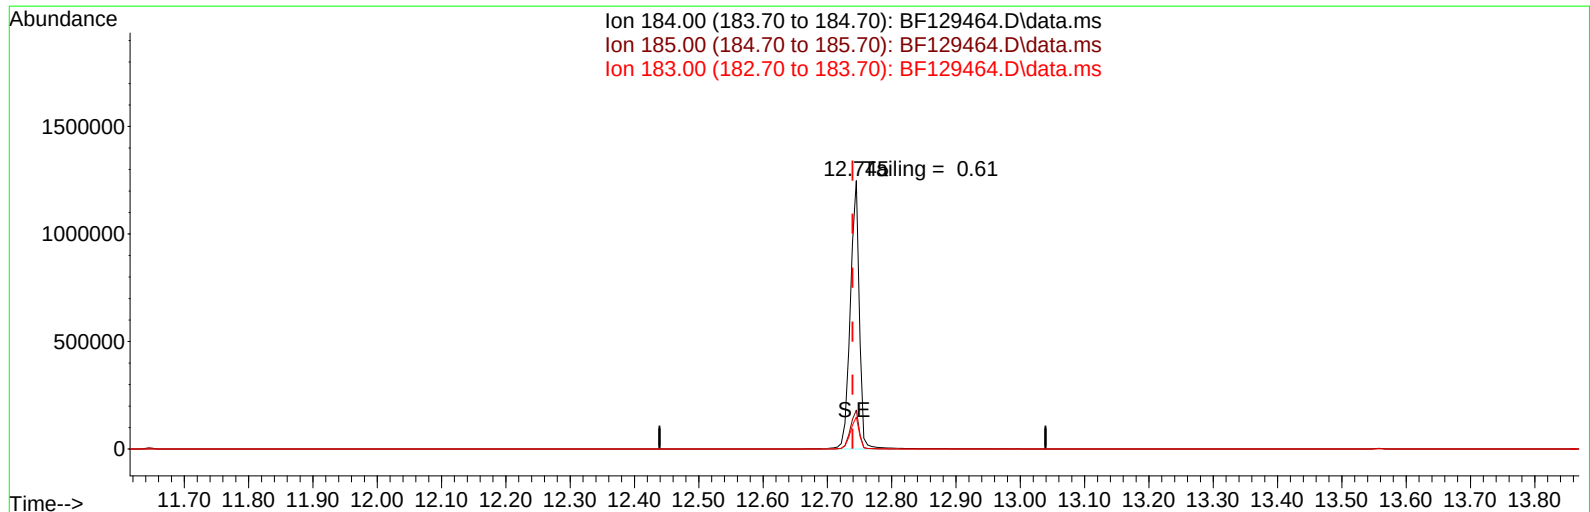

TIC: BF129464.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 41769.97 ng

response 1226248

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.48
183.00	11.60	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/1/2022	BNA_F	<u>BF129464.D</u>
Compound Name	Response	Retention Time
DDT	598843	13.557
DDD	8375	13.257
DDE	957	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9332	608175	1.53

Instrument :
BNA_F
ClientSampleId :
DFTPP