


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080122\
 Data File : BF129475.D
 Acq On : 01 Aug 2022 16:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 02 01:11:25 2022

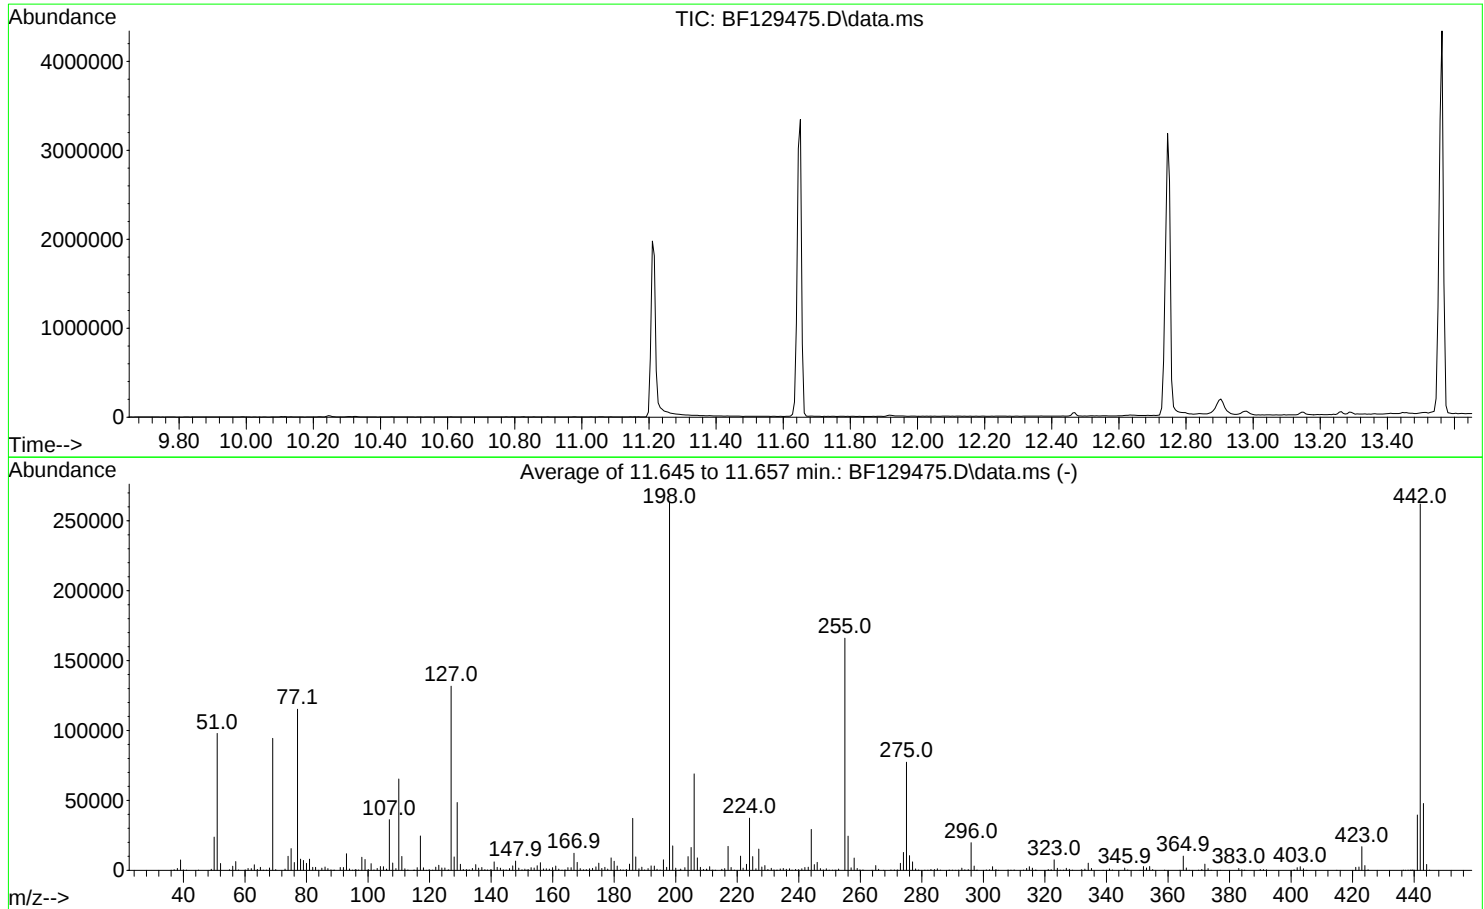




AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	97920	PASS
68	69	0.00	2	1.8	1701	PASS
69	198	0.00	100	35.9	94351	PASS
70	69	0.00	2	0.6	550	PASS
127	198	10	80	50.1	131752	PASS
197	198	0.00	2	0.8	2145	PASS
198	198	100	100	100.0	263157	PASS
199	198	5	9	6.6	17482	PASS
275	198	10	60	29.4	77336	PASS
365	198	1	100	3.8	10122	PASS
441	198	0.01	100	15.0	39509	PASS
442	442	50	100	100.0	262101	PASS
443	442	15	24	18.2	47784	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080122\
Data File : BF129475.D
Acq On : 01 Aug 2022 16:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 09:09:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

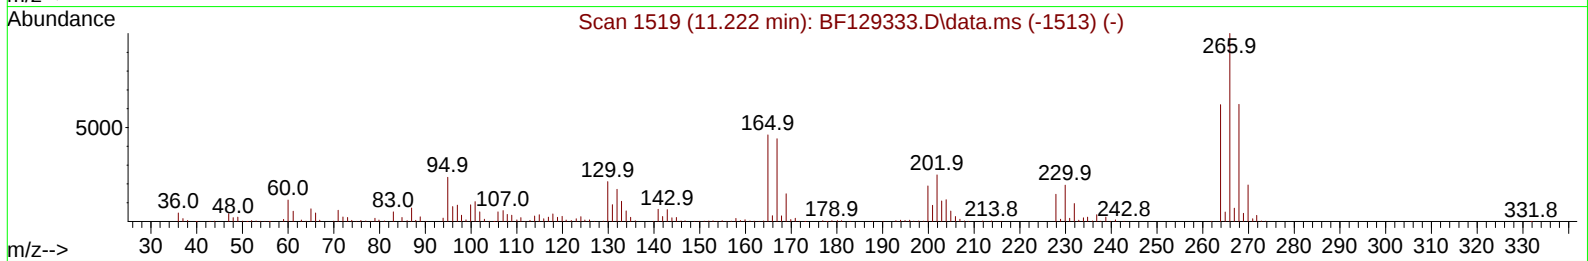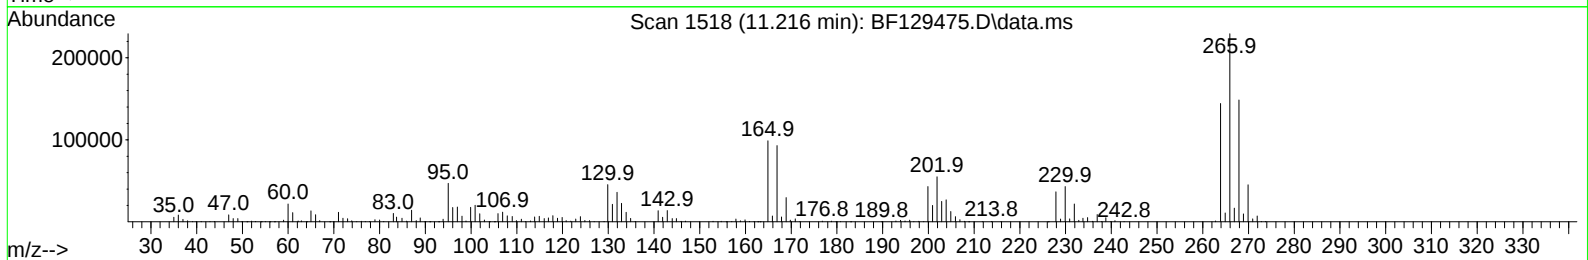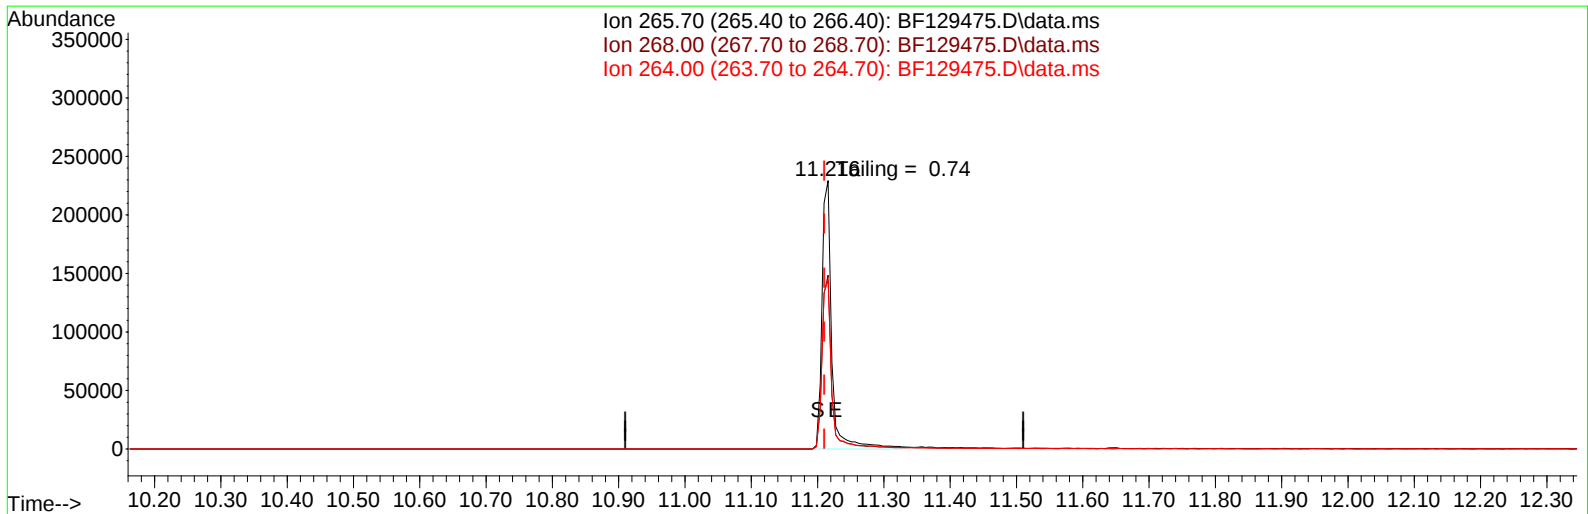

TIC: BF129475.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 414639.08 ng




response 238030

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.78
264.00	61.80	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080122\
Data File : BF129475.D
Acq On : 01 Aug 2022 16:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 09:09:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

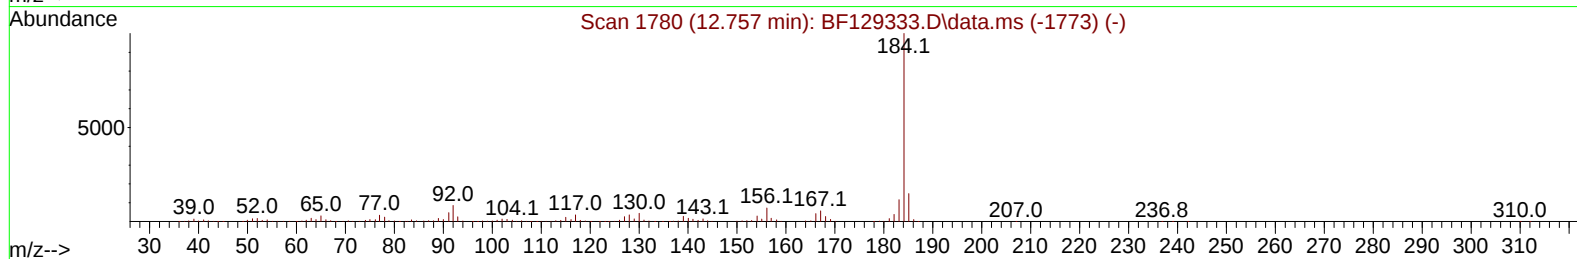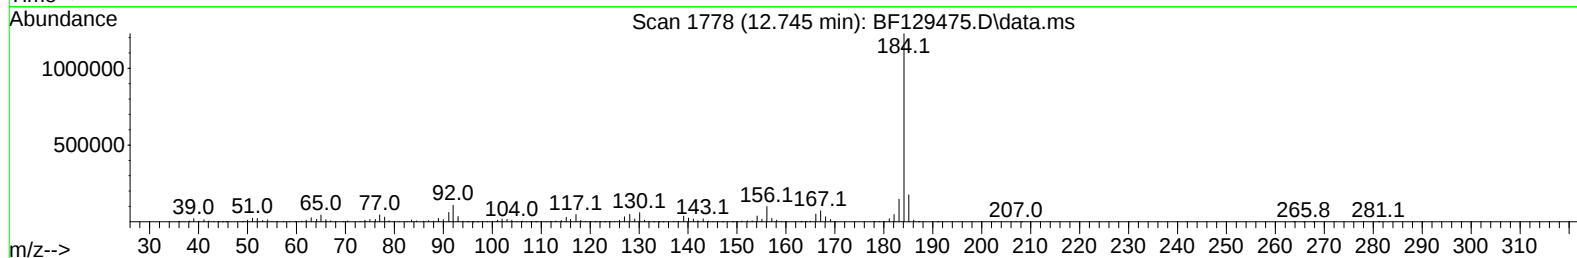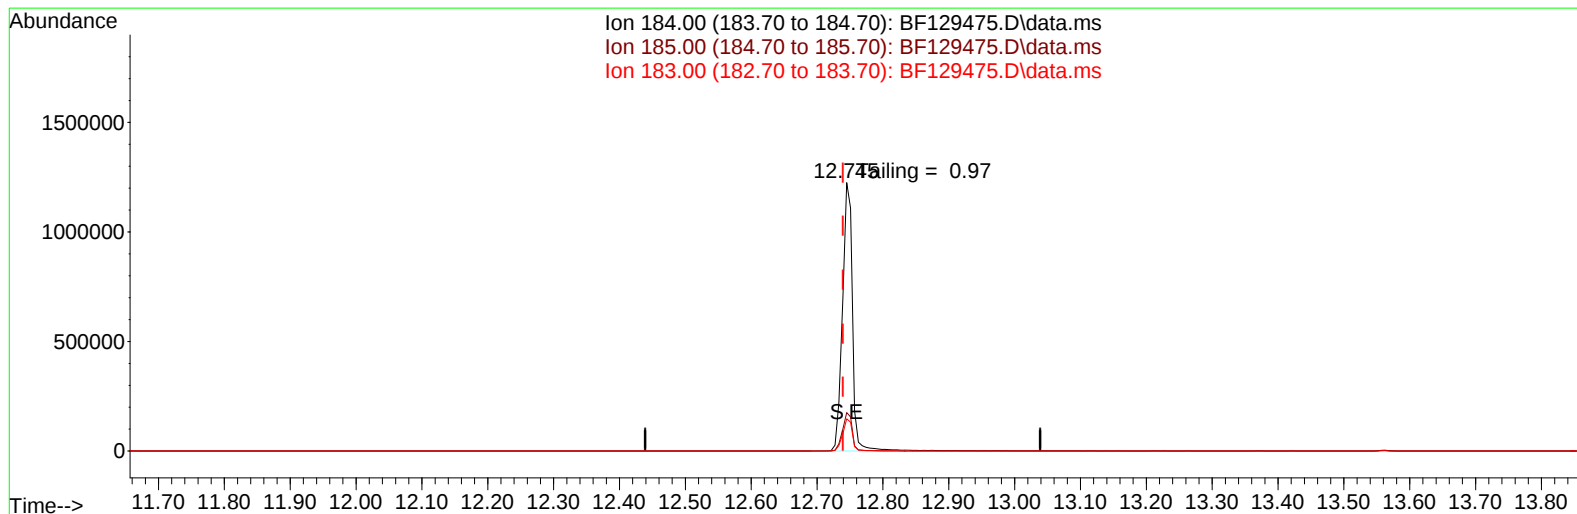

TIC: BF129475.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 53874.78 ng

response 1284702

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.30
183.00	11.60	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/1/2022	BNA_F	<u>BF129475.D</u>
Compound Name	Response	Retention Time
DDT	707861	13.563
DDD	10128	13.263
DDE	1302	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11430	719291	1.59

Instrument :
BNA_F
ClientSampleId :
DFTPP