

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080321\
 Data File : BF124916.D
 Acq On : 3 Aug 2021 15:35
 Operator : JU/CG
 Sample : PB138115BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138115BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.087	508	510	515	rBB	2710	3017	1.14%	0.195%
2	5.469	571	575	578	rBB	184118	185928	70.12%	12.028%
3	6.475	741	746	749	rBV	170856	188443	71.07%	12.190%
4	6.845	806	809	812	rBB	61529	43951	16.58%	2.843%
5	7.410	900	905	908	rBB	129599	121387	45.78%	7.853%
6	8.128	1023	1027	1030	rBB	77395	62557	23.59%	4.047%
7	9.204	1205	1210	1213	rBB	290638	240431	90.68%	15.554%
8	9.880	1321	1325	1328	rBB	96968	75591	28.51%	4.890%
9	10.674	1456	1460	1463	rBB	160737	147808	55.75%	9.562%
10	11.369	1574	1578	1581	rBV	97552	76352	28.80%	4.939%
11	12.957	1843	1848	1851	rBV	310174	265144	100.00%	17.152%
12	13.792	1987	1990	1994	rBB	3395	4141	1.56%	0.268%
13	13.839	1994	1998	2000	rBV	4544	5659	2.13%	0.366%
14	13.868	2000	2003	2007	rVB	14266	15592	5.88%	1.009%
15	14.004	2023	2026	2030	rBB	73603	60685	22.89%	3.926%
16	15.468	2271	2275	2280	rBB	40072	49142	18.53%	3.179%




Sum of corrected areas: 1545828

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080321\
Data File : BF124916.D
Acq On : 3 Aug 2021 15:35
Operator : JU/CG
Sample : PB138115BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138115BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

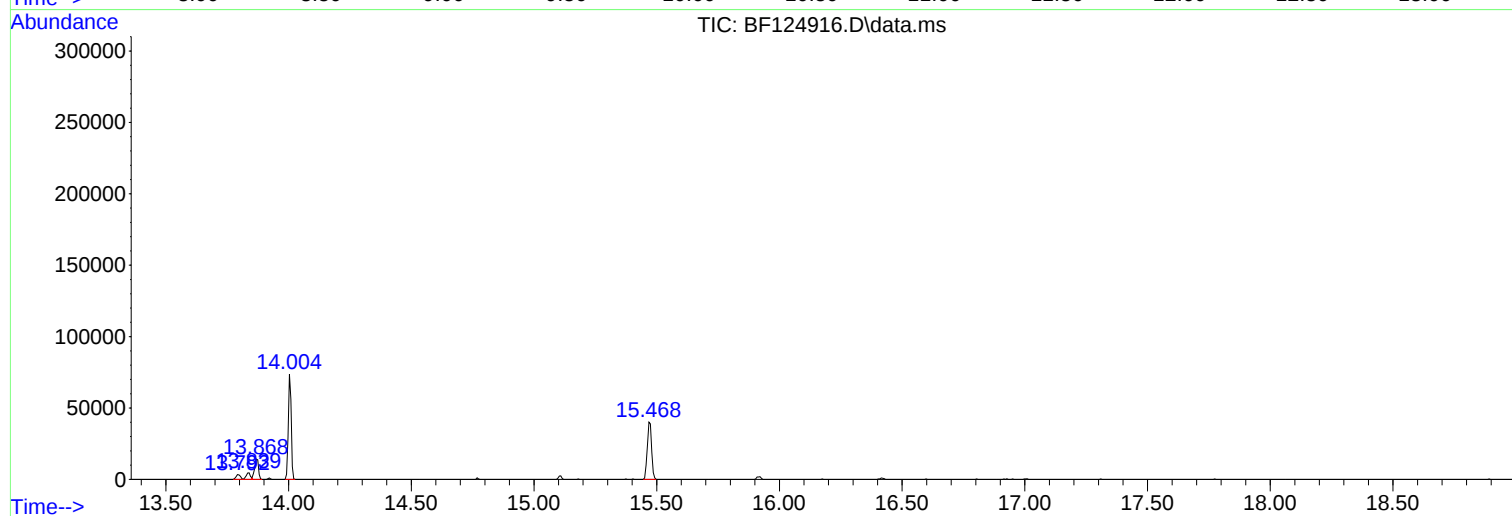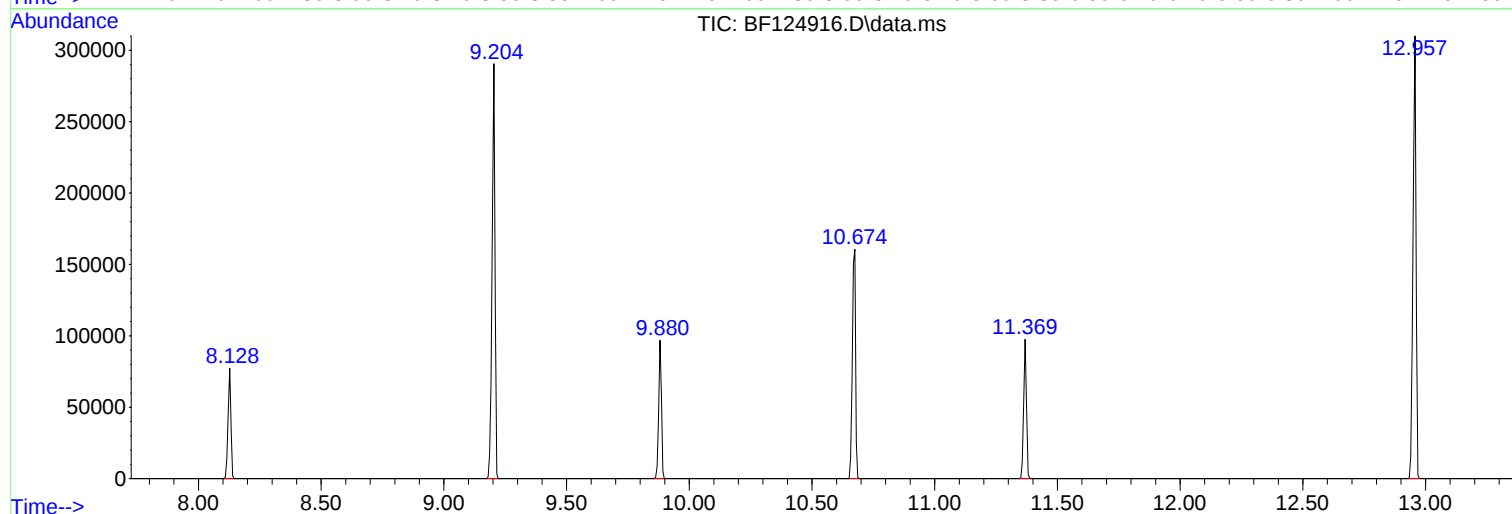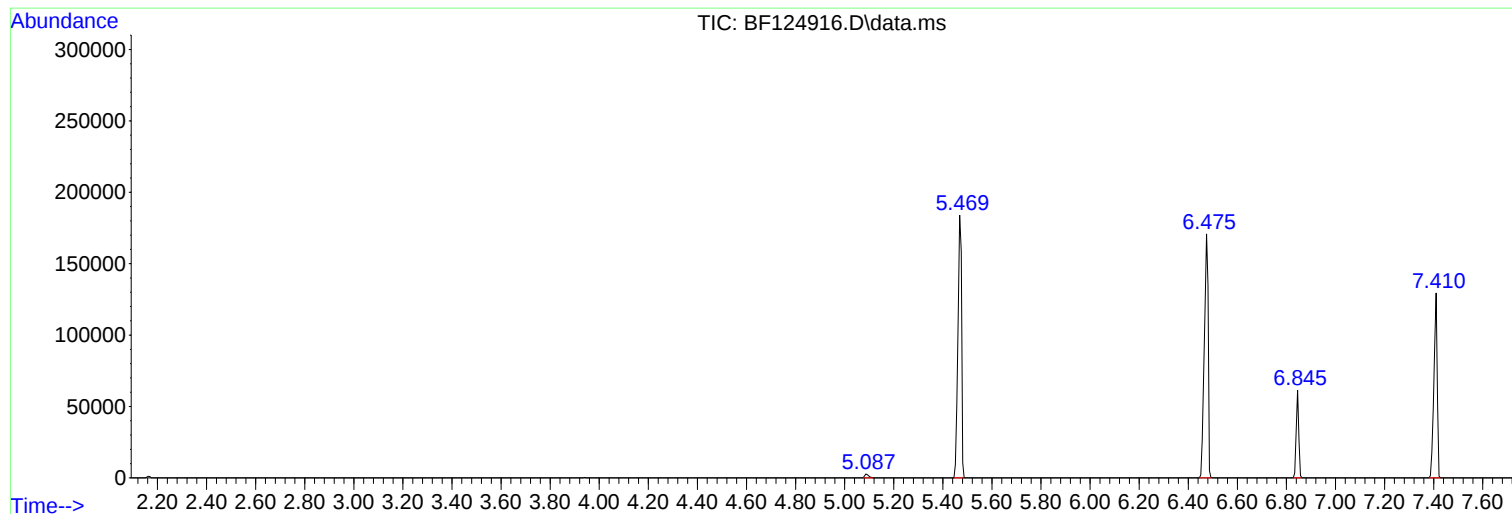

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080321\
Data File : BF124916.D
Acq On : 3 Aug 2021 15:35
Operator : JU/CG
Sample : PB138115BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138115BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethylene glycol dibenzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.868	5.14 ng	15592	Chrysene-d12	14.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	83
2			2-(2-(2-Methoxyethoxy)ethoxy)eth...	268	C14H20O5	1000366-99-1	74
3			2-(2-(2-Ethoxyethoxy)ethoxy)ethy...	282	C15H22O5	1000366-98-8	64
4			3-Benzoylamino-2-benzyl-butyric ...	311	C19H21NO3	1000193-12-7	64
5			N-(.alpha.-Methylbenzyl)-formamide	149	C9H11NO	006948-01-2	43

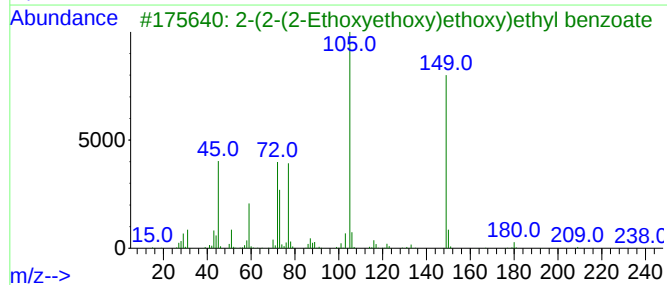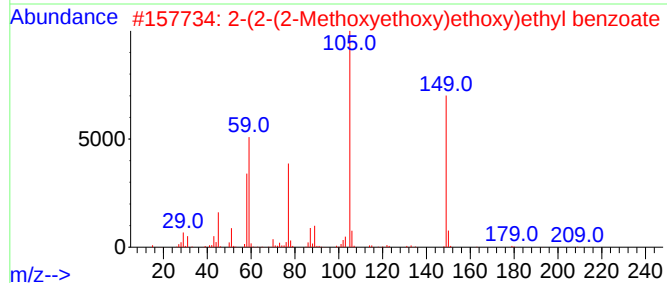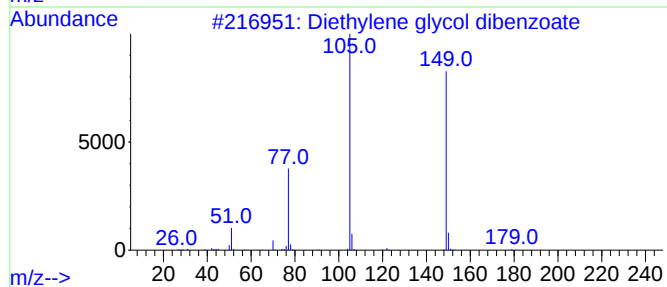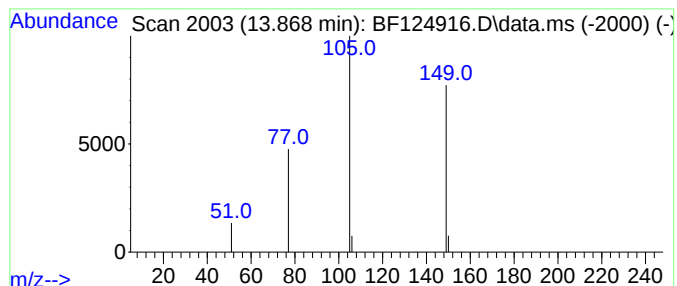

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080321\
Data File : BF124916.D
Acq On : 3 Aug 2021 15:35
Operator : JU/CG
Sample : PB138115BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138115BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethylene glyc...	13.868	5.1	ng	15592	5	14.004	60685	20.0