

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080822\
 Data File : BF129631.D
 Acq On : 08 Aug 2022 14:15
 Operator : CG\JU
 Sample : N4054-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-080422

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	538	542	555	rBV	3063152	2755058	24.24%	2.330%
2	6.492	710	715	724	rBV	2755307	2730031	24.02%	2.309%
3	6.839	770	774	777	rBV	1148061	890897	7.84%	0.754%
4	7.404	866	870	873	rBV	2036354	1706110	15.01%	1.443%
5	8.122	989	992	994	rBV	1444564	1118863	9.85%	0.946%
6	8.145	994	996	999	rVB	455925	336149	2.96%	0.284%
7	8.833	1110	1113	1117	rBV	368469	290844	2.56%	0.246%
8	8.933	1126	1130	1134	rBV	359340	297227	2.62%	0.251%
9	9.198	1171	1175	1178	rVB	3698148	2896623	25.49%	2.450%
10	9.463	1215	1220	1223	rBV2	167365	228695	2.01%	0.193%
11	9.533	1229	1232	1235	rBV	290921	290636	2.56%	0.246%
12	9.739	1264	1267	1271	rBV	755821	608028	5.35%	0.514%
13	9.880	1288	1291	1294	rVV	1279922	989389	8.71%	0.837%
14	9.910	1294	1296	1299	rVB	997763	812726	7.15%	0.687%
15	10.080	1322	1325	1329	rVV2	531716	527635	4.64%	0.446%
16	10.116	1329	1331	1335	rVB	164870	147356	1.30%	0.125%
17	10.192	1340	1344	1347	rBV2	182126	203987	1.79%	0.173%
18	10.286	1355	1360	1361	rBV2	116159	160855	1.42%	0.136%
19	10.427	1381	1384	1390	rVB	1102273	932972	8.21%	0.789%
20	10.580	1405	1410	1414	rVB2	225461	276922	2.44%	0.234%
21	10.675	1422	1426	1429	rVB	1711112	1648239	14.50%	1.394%
22	10.786	1439	1445	1452	rVB4	174005	368962	3.25%	0.312%
23	10.974	1472	1477	1480	rBV2	286832	350841	3.09%	0.297%
24	11.004	1480	1482	1485	rVV2	201183	168958	1.49%	0.143%
25	11.057	1489	1491	1494	rVB	177656	151986	1.34%	0.129%
26	11.104	1494	1499	1501	rBV3	192597	275284	2.42%	0.233%
27	11.127	1501	1503	1508	rVV2	201326	229986	2.02%	0.195%
28	11.174	1508	1511	1514	rVV2	248409	242997	2.14%	0.206%
29	11.216	1515	1518	1521	rVV	274109	304634	2.68%	0.258%
30	11.269	1521	1527	1531	rVB	442269	527627	4.64%	0.446%
31	11.374	1541	1545	1546	rBV	921383	931885	8.20%	0.788%
32	11.404	1546	1550	1552	rVV	4846544	4836979	42.56%	4.091%
33	11.451	1554	1558	1560	rVV	1886171	1652773	14.54%	1.398%
34	11.480	1560	1563	1566	rVV2	153316	184870	1.63%	0.156%
35	11.604	1579	1584	1589	rBV	479616	589362	5.19%	0.498%
36	11.663	1592	1594	1597	rVV	239746	194200	1.71%	0.164%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080822\
 Data File : BF129631.D
 Acq On : 08 Aug 2022 14:15
 Operator : CG\JU
 Sample : N4054-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-080422

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.704	1598	1601	1605	rVV2	274398	297444	2.62%	0.252%
38	11.780	1611	1614	1618	rVB	173639	191547	1.69%	0.162%
39	11.874	1626	1630	1632	rBV	1011552	917075	8.07%	0.776%
40	11.904	1632	1635	1638	rVB	1341726	1229396	10.82%	1.040%

41	11.951	1638	1643	1646	rBV	613257	615030	5.41%	0.520%
42	11.986	1646	1649	1651	rVV2	1925039	1980331	17.43%	1.675%
43	12.010	1651	1653	1658	rVB	752686	594876	5.23%	0.503%
44	12.057	1658	1661	1663	rBV	203820	197476	1.74%	0.167%
45	12.104	1667	1669	1672	rBV3	159571	147438	1.30%	0.125%

46	12.169	1676	1680	1683	rVV	818082	777947	6.85%	0.658%
47	12.198	1683	1685	1690	rVB	519231	468128	4.12%	0.396%
48	12.316	1700	1705	1708	rBV2	281047	370446	3.26%	0.313%
49	12.345	1708	1710	1713	rVV	328872	306189	2.69%	0.259%
50	12.374	1713	1715	1718	rVB	275998	217912	1.92%	0.184%

51	12.421	1719	1723	1726	rBV	828449	1032305	9.08%	0.873%
52	12.463	1726	1730	1732	rVV2	647722	857212	7.54%	0.725%
53	12.521	1736	1740	1743	rBV2	761520	879945	7.74%	0.744%
54	12.604	1748	1754	1757	rBV	7978687	10481496	92.23%	8.865%
55	12.633	1757	1759	1761	rBV	212176	173434	1.53%	0.147%

56	12.651	1761	1762	1765	rVB	266752	208524	1.83%	0.176%
57	12.686	1765	1768	1771	rBV	312455	257474	2.27%	0.218%
58	12.739	1774	1777	1781	rVV	445778	479472	4.22%	0.406%
59	12.774	1781	1783	1786	rVB2	206277	173400	1.53%	0.147%
60	12.839	1786	1794	1797	rBV2	7275708	11364490	100.00%	9.612%

61	12.868	1797	1799	1803	rVB2	623130	637317	5.61%	0.539%
62	12.957	1807	1814	1816	rBV2	2792793	3075697	27.06%	2.601%
63	12.980	1816	1818	1822	rVB2	441344	409754	3.61%	0.347%
64	13.039	1823	1828	1832	rBV3	769974	1355826	11.93%	1.147%
65	13.127	1839	1843	1844	rBV3	658051	795581	7.00%	0.673%

66	13.151	1844	1847	1849	rVB	1668756	1479264	13.02%	1.251%
67	13.216	1855	1858	1860	rBV	1324397	999353	8.79%	0.845%
68	13.257	1860	1865	1867	rBV2	1004903	1224010	10.77%	1.035%
69	13.310	1871	1874	1876	rVB	207956	185245	1.63%	0.157%
70	13.345	1877	1880	1883	rBV	595047	544725	4.79%	0.461%

71	13.374	1883	1885	1888	rBV	633295	628664	5.53%	0.532%
72	13.521	1907	1910	1912	rBV4	247667	284781	2.51%	0.241%
73	13.568	1916	1918	1921	rVB	260062	239586	2.11%	0.203%
74	13.633	1926	1929	1931	rBV	283493	298774	2.63%	0.253%
75	13.663	1931	1934	1938	rVB	829230	782627	6.89%	0.662%

76	13.768	1948	1952	1955	rBV	1013884	1200270	10.56%	1.015%
----	--------	------	------	------	-----	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080822\
 Data File : BF129631.D
 Acq On : 08 Aug 2022 14:15
 Operator : CG\JU
 Sample : N4054-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-080422

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	13.798	1955	1957	1959	rVV	1007617	814249	7.16%	0.689%
78	13.827	1959	1962	1967	rVV3	868915	1424285	12.53%	1.205%
79	13.874	1967	1970	1973	rVB	808471	855955	7.53%	0.724%
80	13.939	1979	1981	1987	rVB	277499	341678	3.01%	0.289%
81	14.021	1987	1995	1998	rBV2	4618370	6935202	61.03%	5.866%
82	14.057	1998	2001	2004	rVV	4116919	4598057	40.46%	3.889%
83	14.110	2008	2010	2012	rVV3	272132	283328	2.49%	0.240%
84	14.133	2012	2014	2016	rVV	1041094	838913	7.38%	0.710%
85	14.174	2019	2021	2026	rVV3	532301	770109	6.78%	0.651%
86	14.239	2030	2032	2033	rVV	298277	236745	2.08%	0.200%
87	14.280	2037	2039	2042	rBV2	248372	227607	2.00%	0.193%
88	14.368	2052	2054	2057	rBV2	321353	346177	3.05%	0.293%
89	14.410	2057	2061	2064	rVV	900158	945496	8.32%	0.800%
90	14.445	2064	2067	2069	rVV	405716	323474	2.85%	0.274%
91	14.539	2080	2083	2084	rBV2	393258	335173	2.95%	0.283%
92	14.557	2084	2086	2089	rVB2	529710	458838	4.04%	0.388%
93	14.910	2143	2146	2154	rVB2	359569	505587	4.45%	0.428%
94	15.086	2169	2176	2178	rBV	3038527	5373122	47.28%	4.545%
95	15.186	2189	2193	2197	rBV	847355	897843	7.90%	0.759%
96	15.386	2222	2227	2232	rVB	1770091	2536415	22.32%	2.145%
97	15.457	2233	2239	2242	rBV	2759355	3743066	32.94%	3.166%
98	15.545	2250	2254	2260	rVB2	941640	1359169	11.96%	1.150%
99	17.015	2496	2504	2510	rVB	1281969	2739457	24.11%	2.317%
100	17.468	2575	2581	2590	rVB	956447	2120454	18.66%	1.793%




Sum of corrected areas: 118231446

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080822\
Data File : BF129631.D
Acq On : 08 Aug 2022 14:15
Operator : CG\JU
Sample : N4054-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-080422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

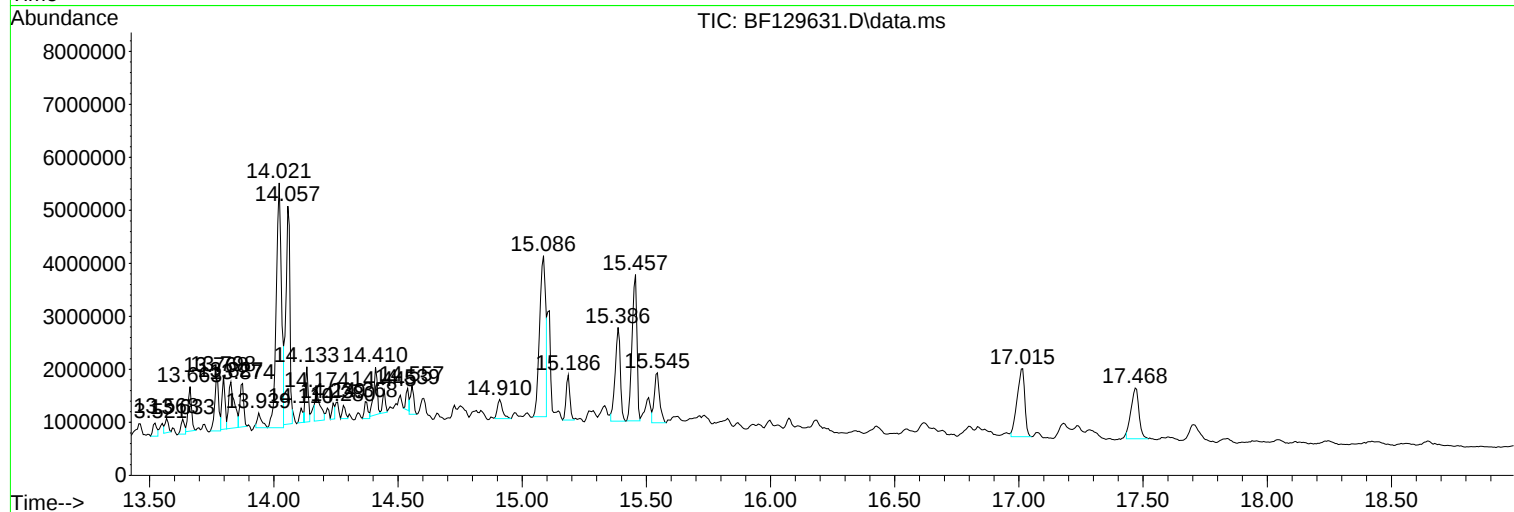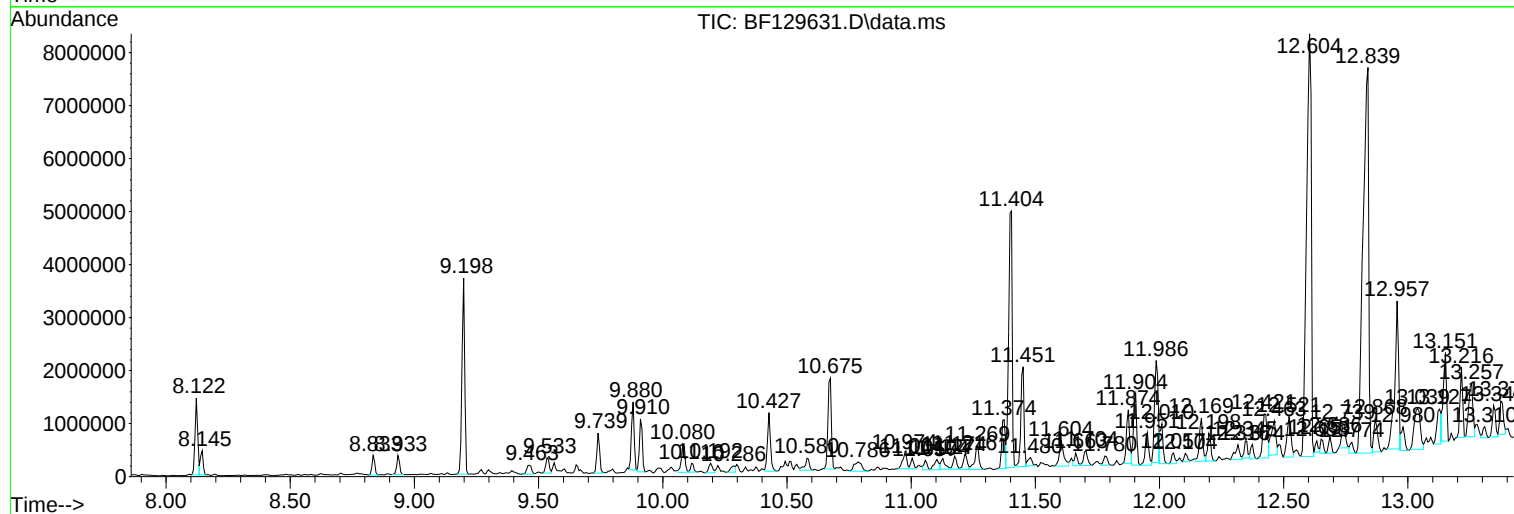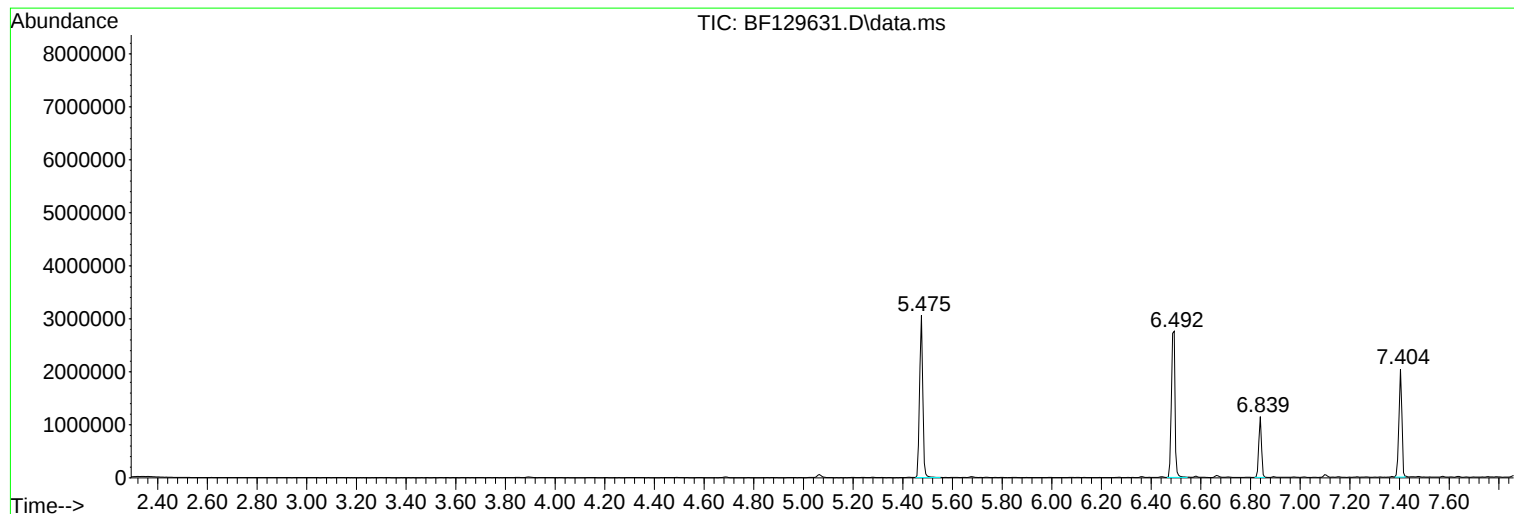

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080822\
Data File : BF129631.D
Acq On : 08 Aug 2022 14:15
Operator : CG\JU
Sample : N4054-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-080422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080822\
Data File : BF129631.D
Acq On : 08 Aug 2022 14:15
Operator : CG\JU
Sample : N4054-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-080422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------