
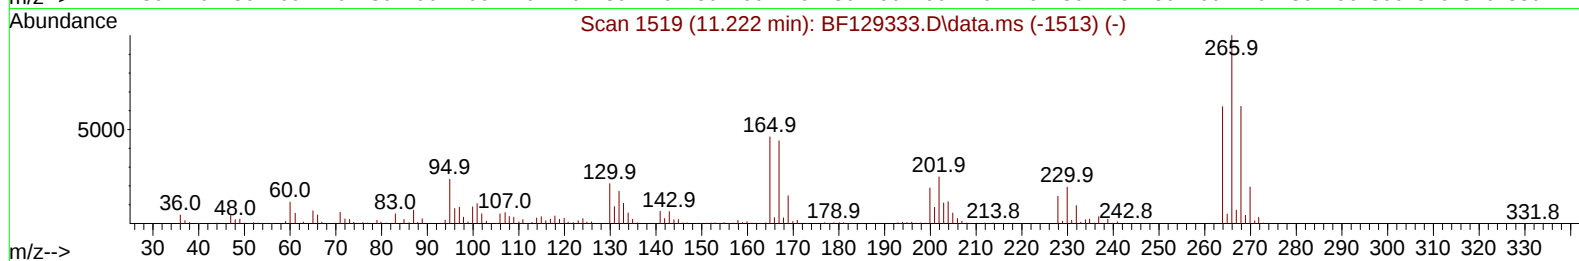
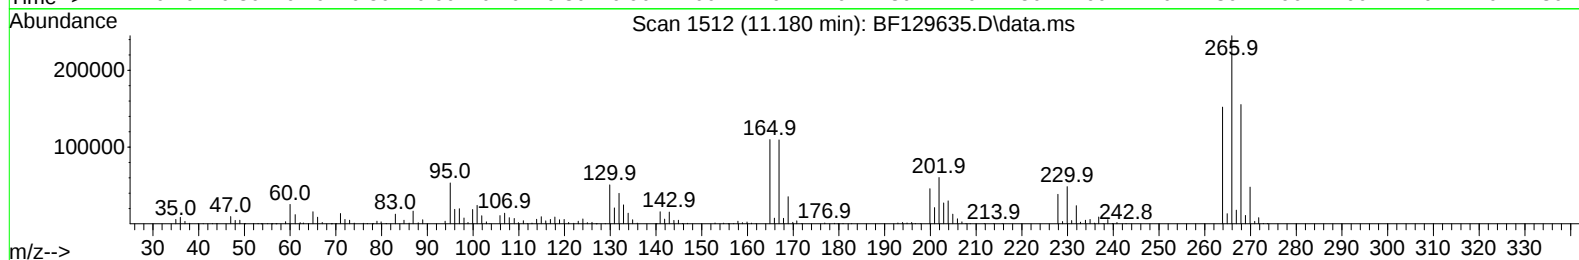


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080822\
Data File : BF129635.D
Acq On : 08 Aug 2022 17:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 09 06:47:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 16:27:34 2022
Response via : Initial Calibration

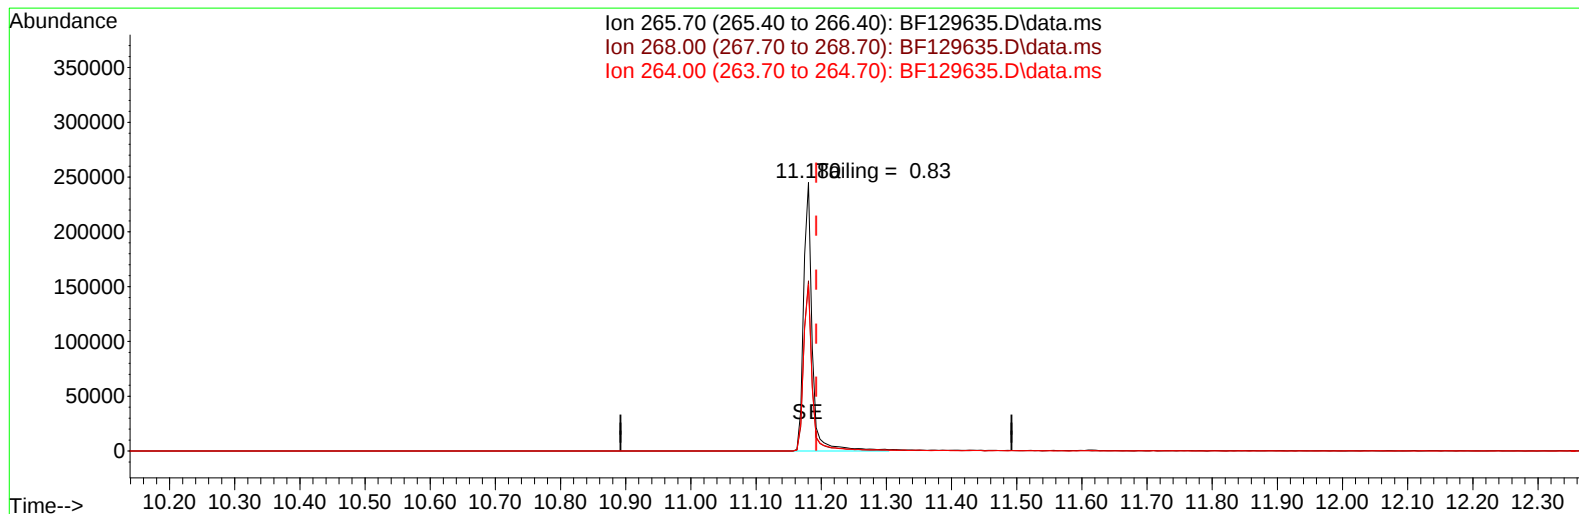

TIC: BF129635.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.012) 27886.25 ng




response 228976

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.39
264.00	61.80	62.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080822\
 Data File : BF129635.D
 Acq On : 08 Aug 2022 17:02
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 09 06:47:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 05 16:27:34 2022
 Response via : Initial Calibration

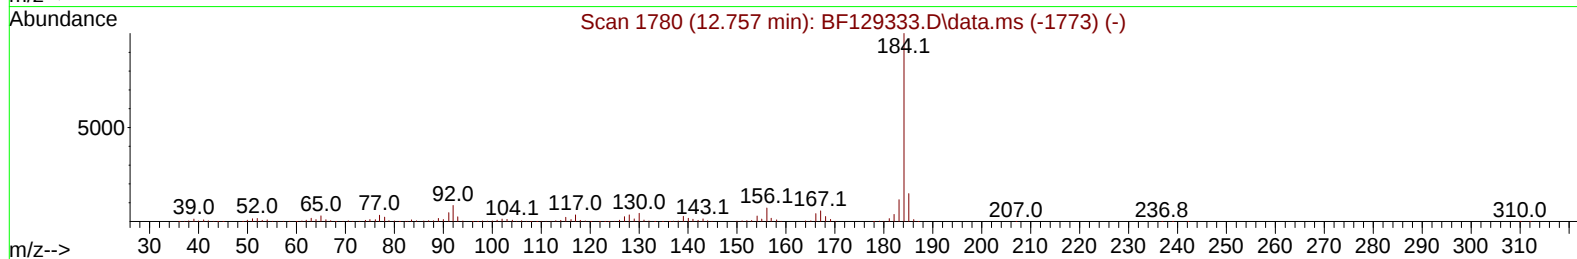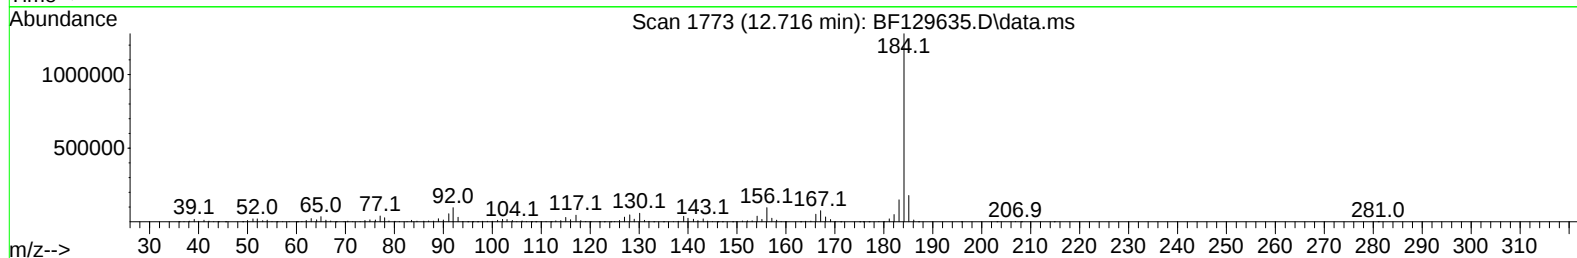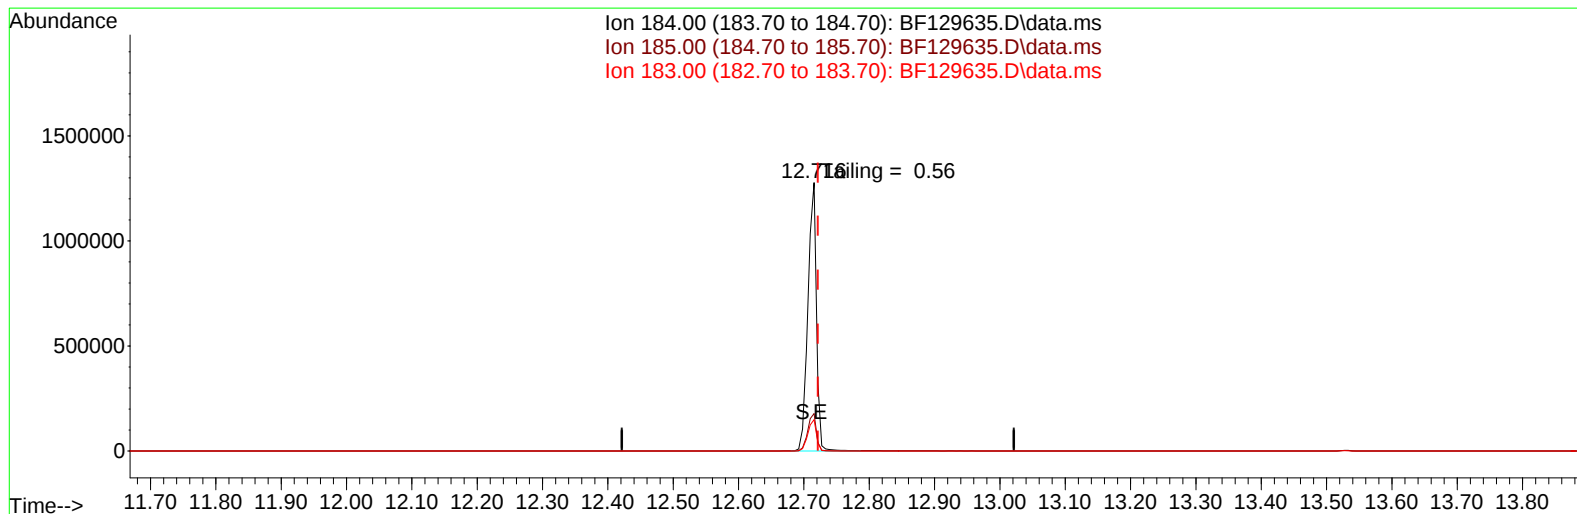

TIC: BF129635.D\data.ms

(77) Benzidine

12.716min (-0.006) 158520.07 ng

response 1159225


Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.97
183.00	11.60	11.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080822\
 Data File : BF129635.D
 Acq On : 08 Aug 2022 17:02
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 05 16:27:34 2022

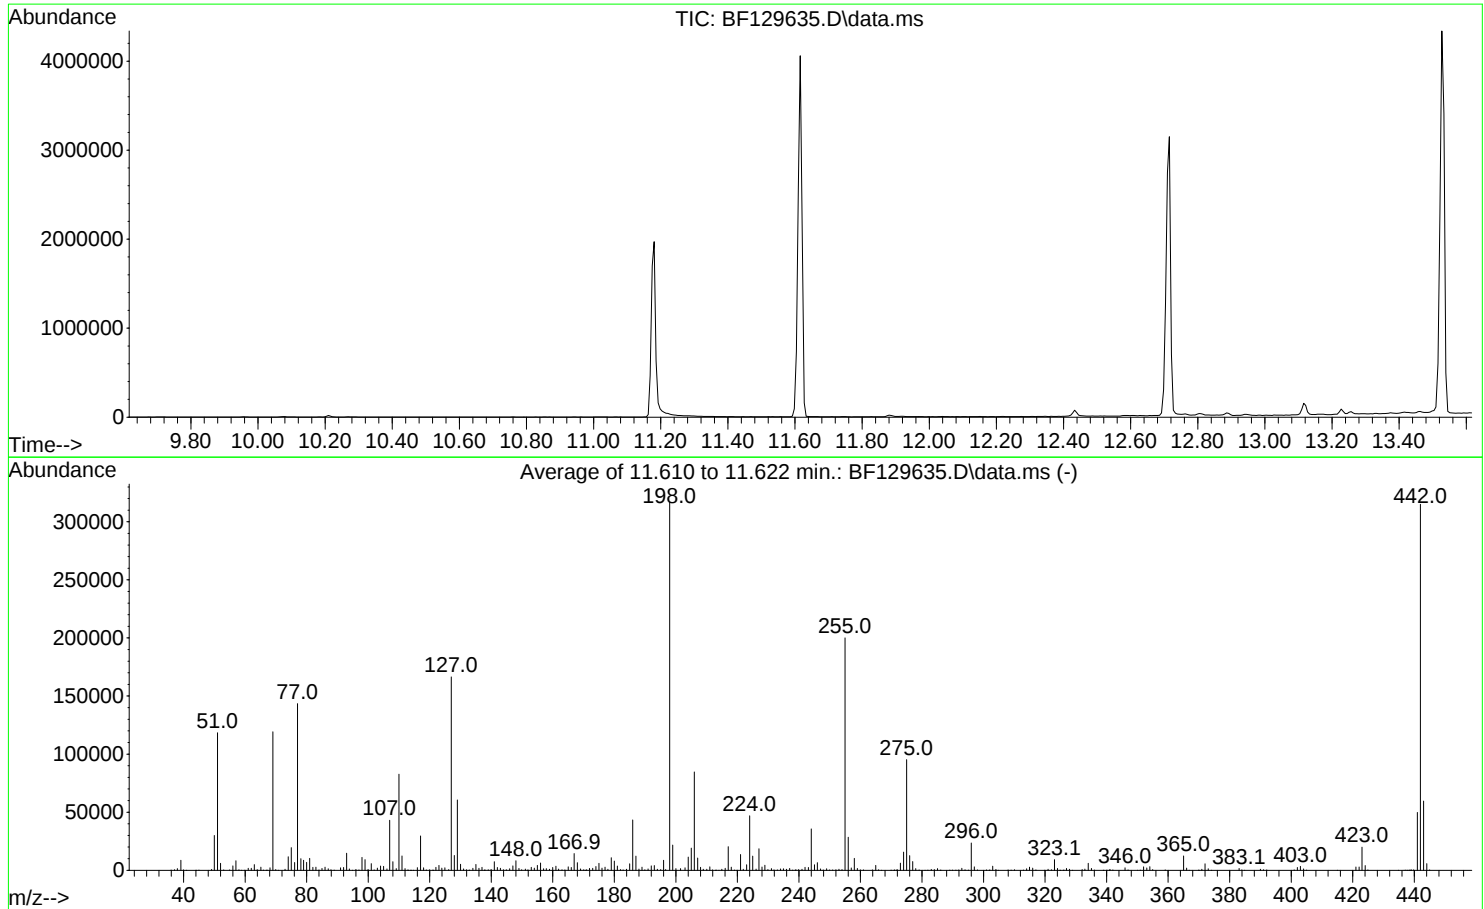

AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	118365	PASS
68	69	0.00	2	1.8	2128	PASS
69	198	0.00	100	37.6	119197	PASS
70	69	0.00	2	0.5	608	PASS
127	198	10	80	52.6	166472	PASS
197	198	0.00	2	0.2	648	PASS
198	198	100	100	100.0	316672	PASS
199	198	5	9	6.9	21761	PASS
275	198	10	60	30.1	95208	PASS
365	198	1	100	3.9	12329	PASS
441	198	0.01	100	15.7	49736	PASS
442	442	50	100	100.0	315008	PASS
443	442	15	24	18.9	59597	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/8/2022	BNA_F	<u>BF129635.D</u>
Compound Name	Response	Retention Time
DDT	741387	13.527
DDD	15174	13.227
DDE	2926	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18100	759487	2.38

Instrument :
BNA_F
ClientSampleId :
DFTPP