
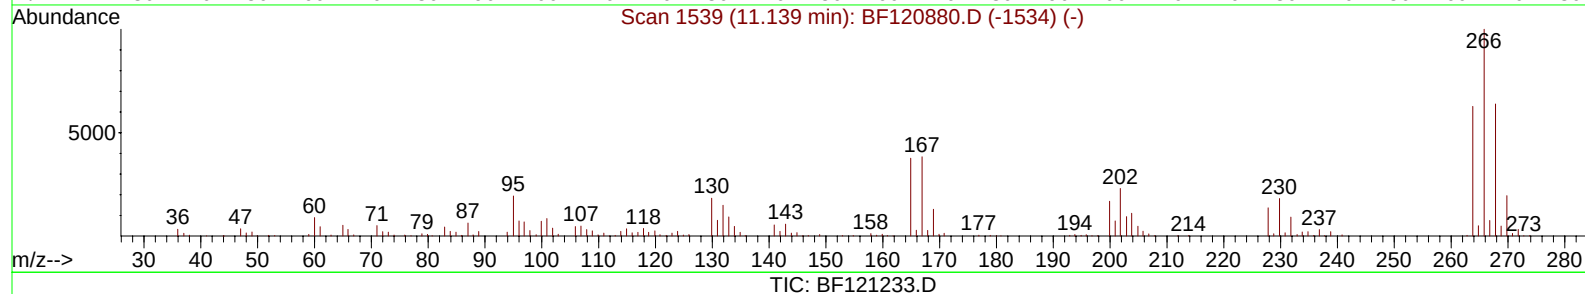
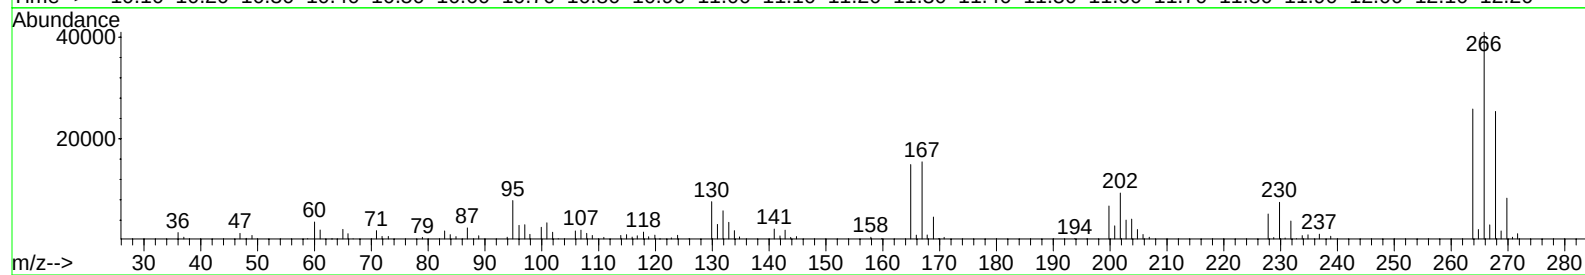


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081020\
Data File : BF121233.D
Acq On : 10 Aug 2020 12:17
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 16:56:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 29 14:55:43 2020
Response via : Initial Calibration

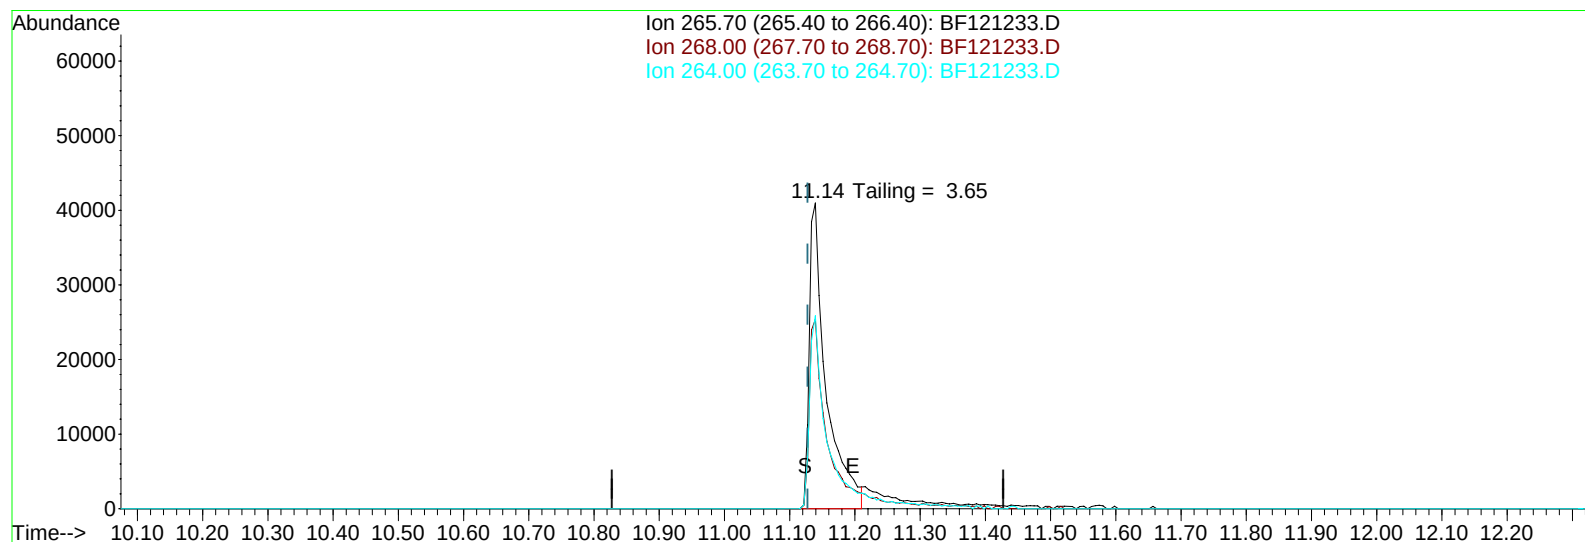

(70) Pentachlorophenol (C)




11.139min (+0.012) 74408.62ng

response 83286

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	61.97
264.00	63.00	63.12
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081020\
 Data File : BF121233.D
 Acq On : 10 Aug 2020 12:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 10 16:56:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 29 14:55:43 2020
 Response via : Initial Calibration

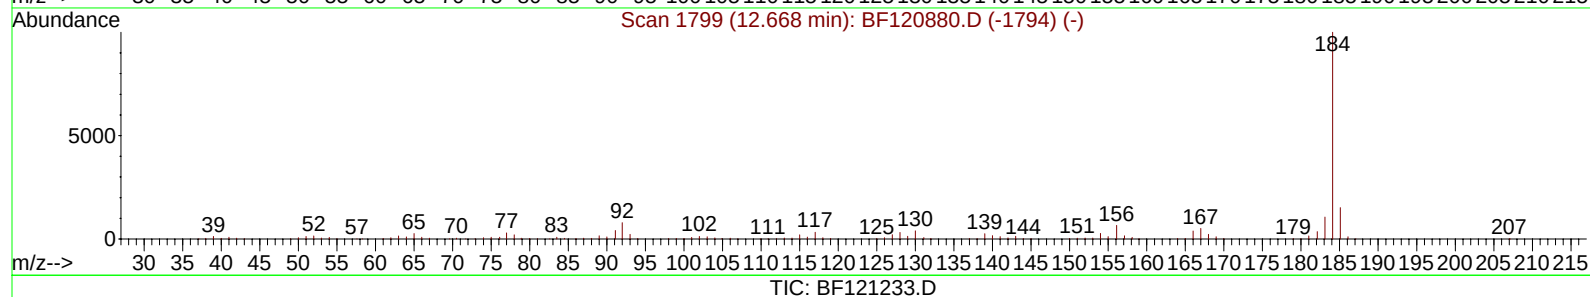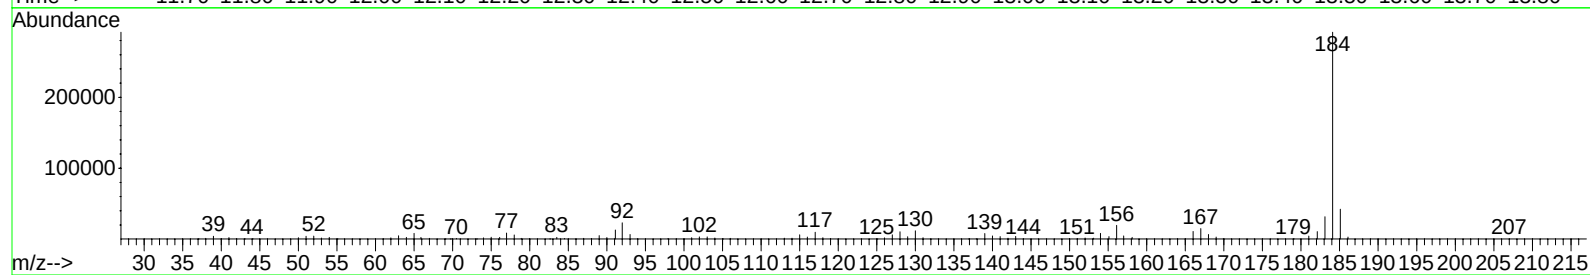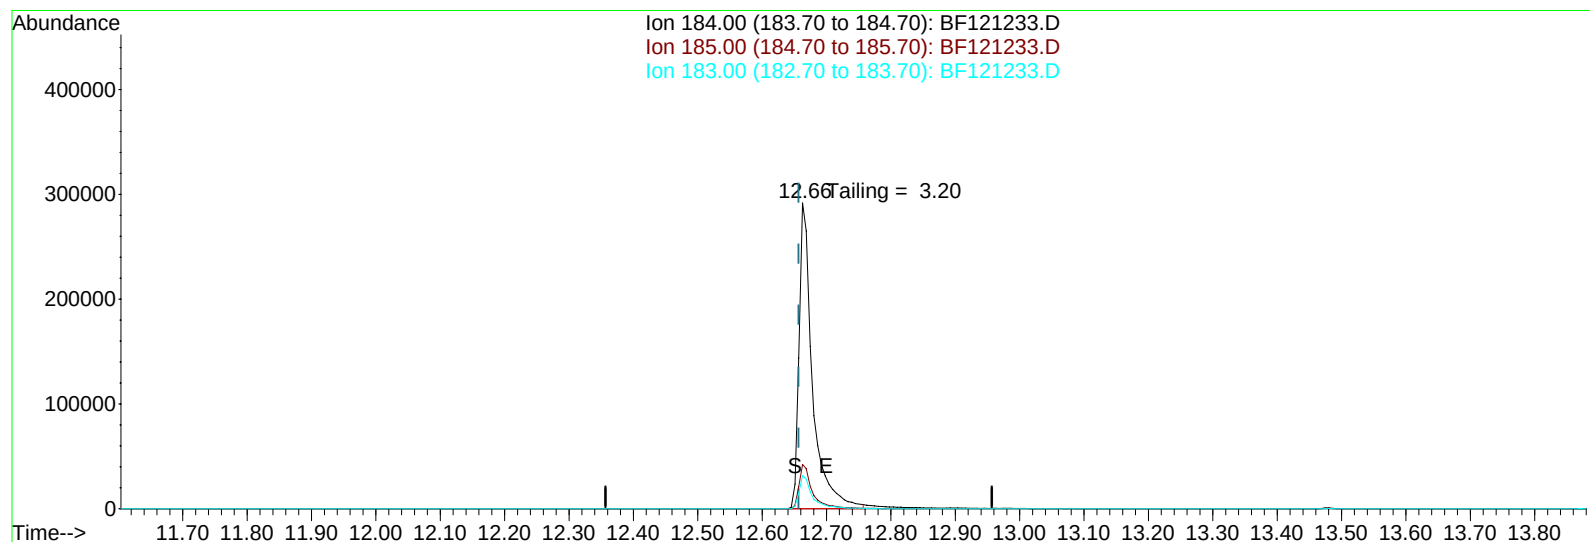

(77) Benzidine

12.663min (+0.006) 0.00ng

response 436443

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.48
183.00	11.20	10.86
0.00	0.00	0.00